


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG062818\
 Data File : BG035480.D
 Acq On : 28 Jun 2018 15:43
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG060718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 08 17:16:28 2018

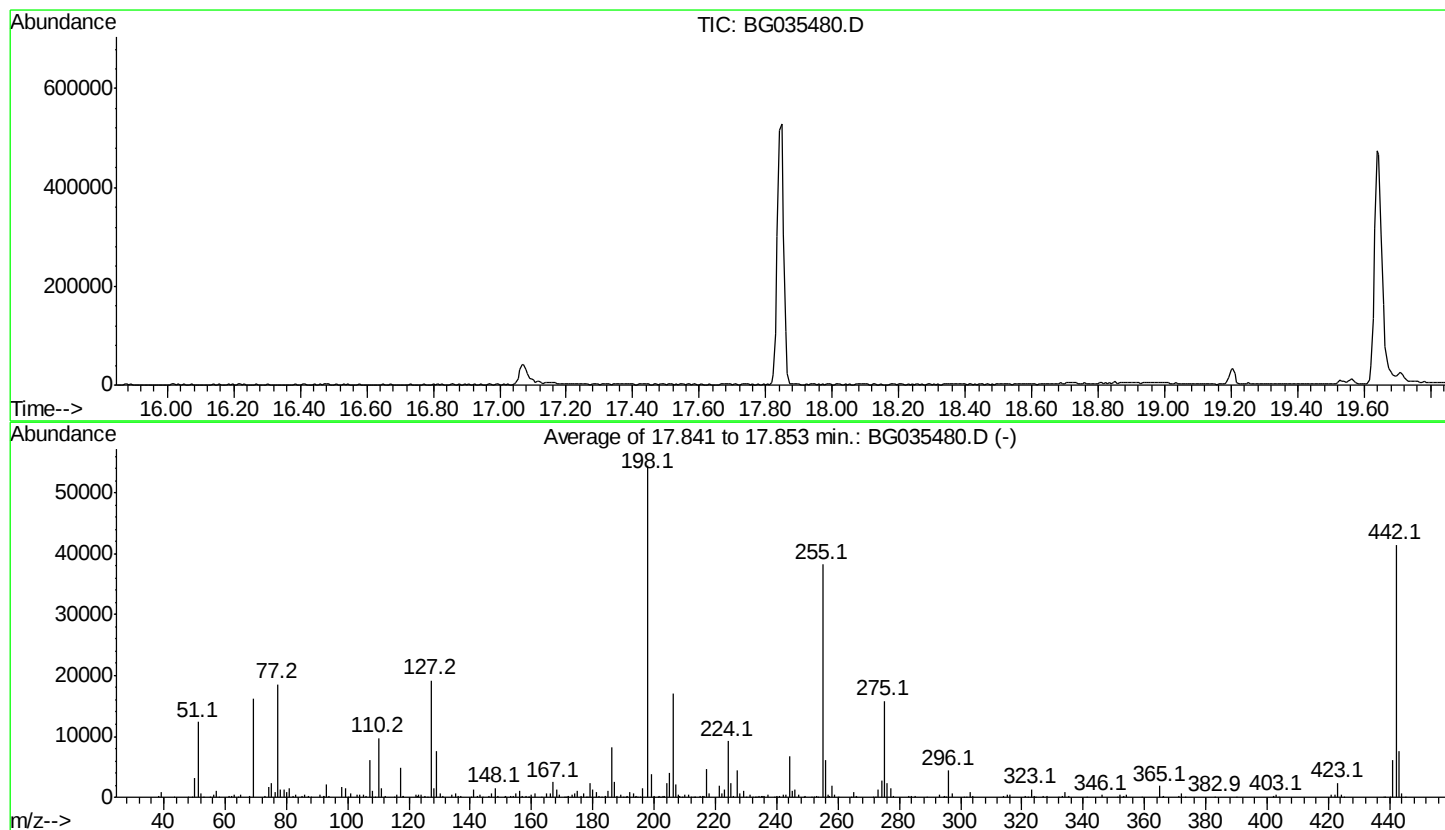

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.7	12386	PASS
68	69	0.00	2	1.6	265	PASS
69	198	0.00	100	29.6	16123	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	35.2	19200	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	54506	PASS
199	198	5	9	7.0	3799	PASS
275	198	10	60	29.1	15872	PASS
365	198	1	100	3.5	1889	PASS
441	443	0.01	100	82.6	6185	PASS
442	198	50	100	76.1	41498	PASS
443	442	15	24	18.0	7488	PASS