
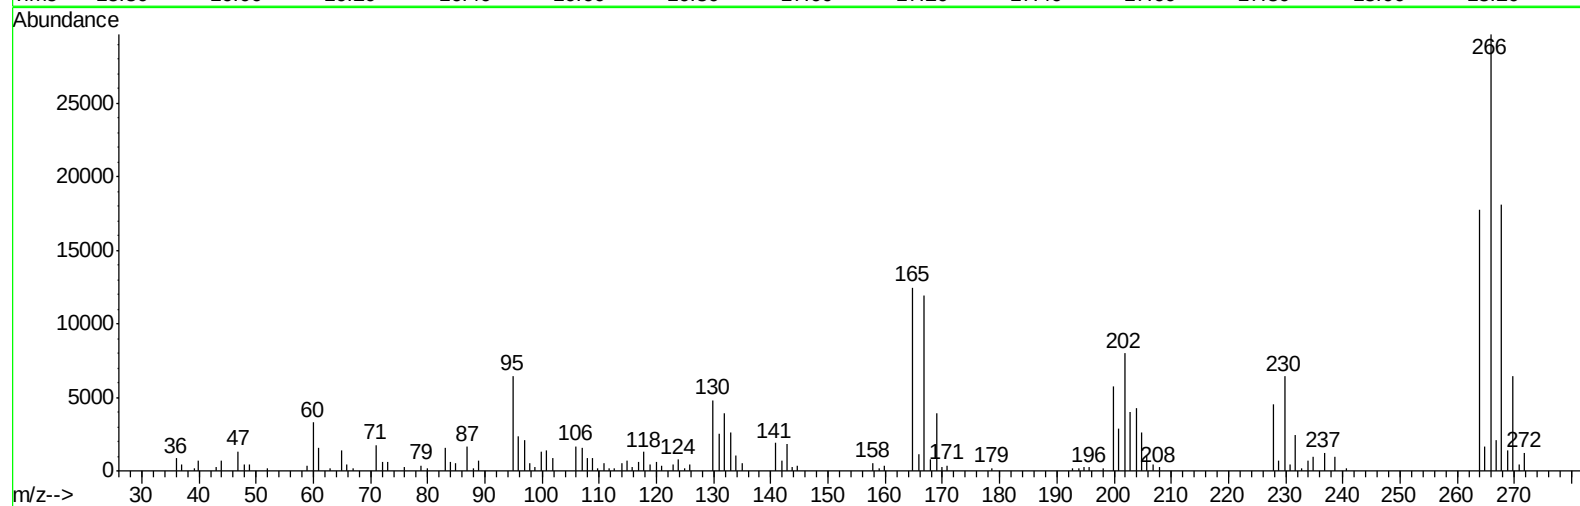


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG062819\
Data File : BG041507.D
Acq On : 28 Jun 2019 11:12
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 28 13:56:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG062619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 27 13:25:55 2019
Response via : Initial Calibration

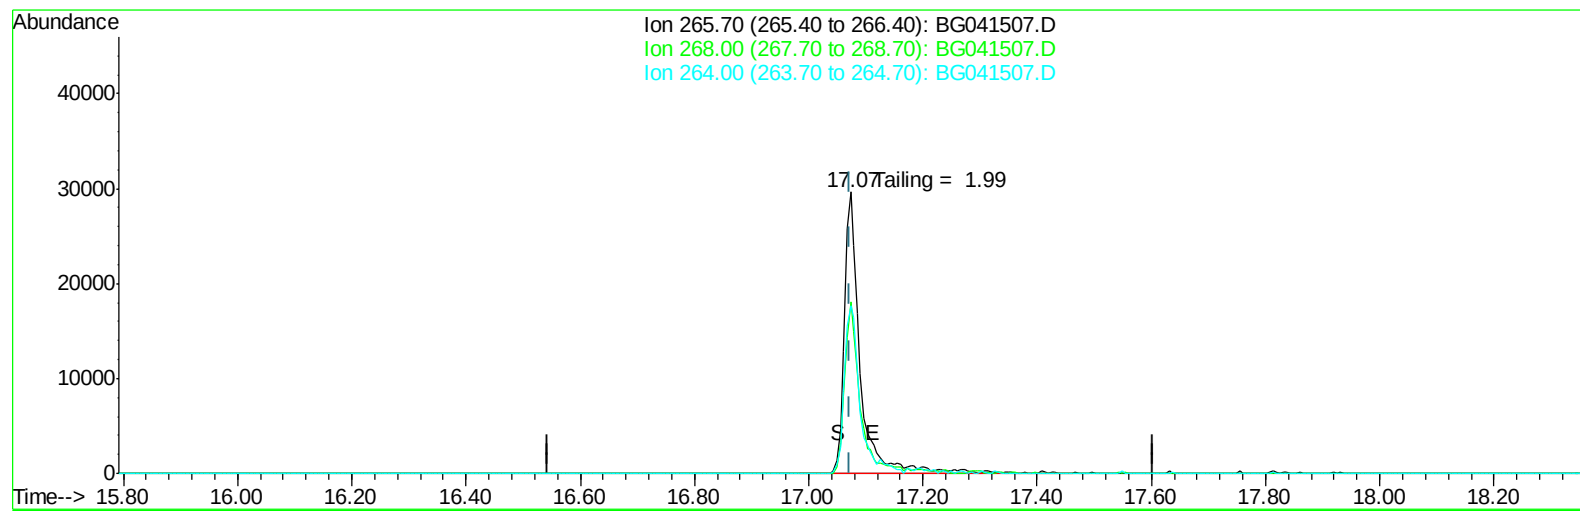

TIC: BG041507.D

(70) Pentachlorophenol (C)



17.073min (-0.001) 24135.33ng

response 53941

Ion	Exp%	Act%
265.70	100	100
268.00	58.70	61.07
264.00	59.20	59.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG062819\
Data File : BG041507.D
Acq On : 28 Jun 2019 11:12
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 28 13:56:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG062619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 27 13:25:55 2019
Response via : Initial Calibration

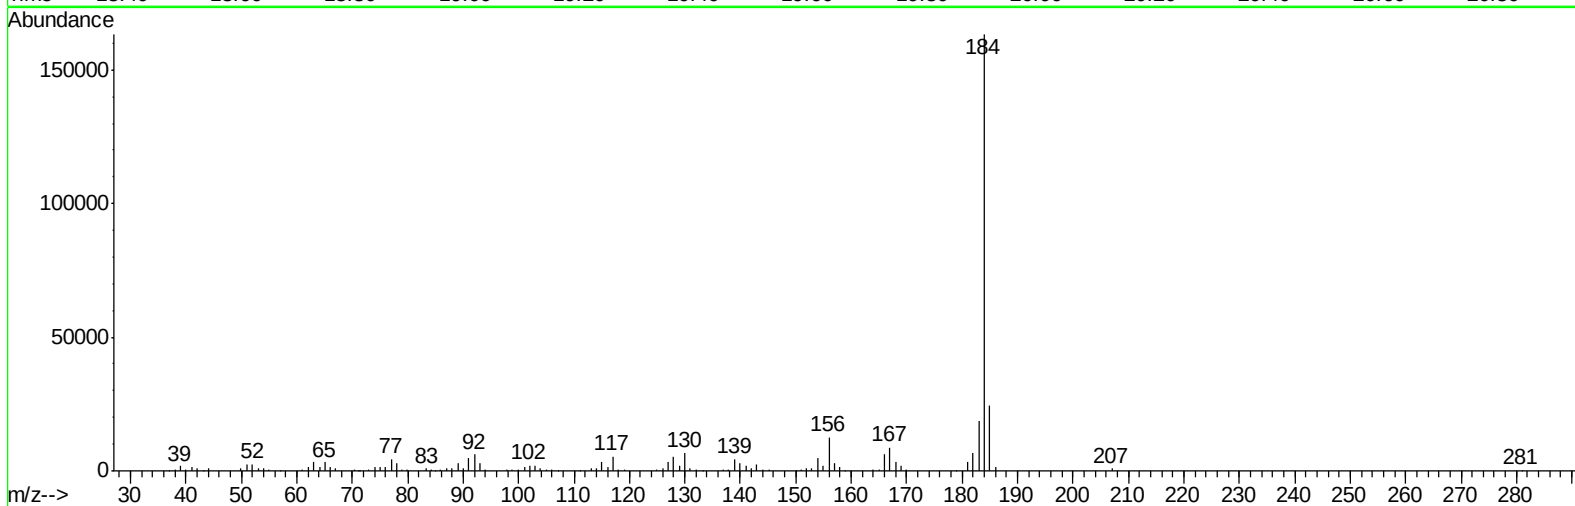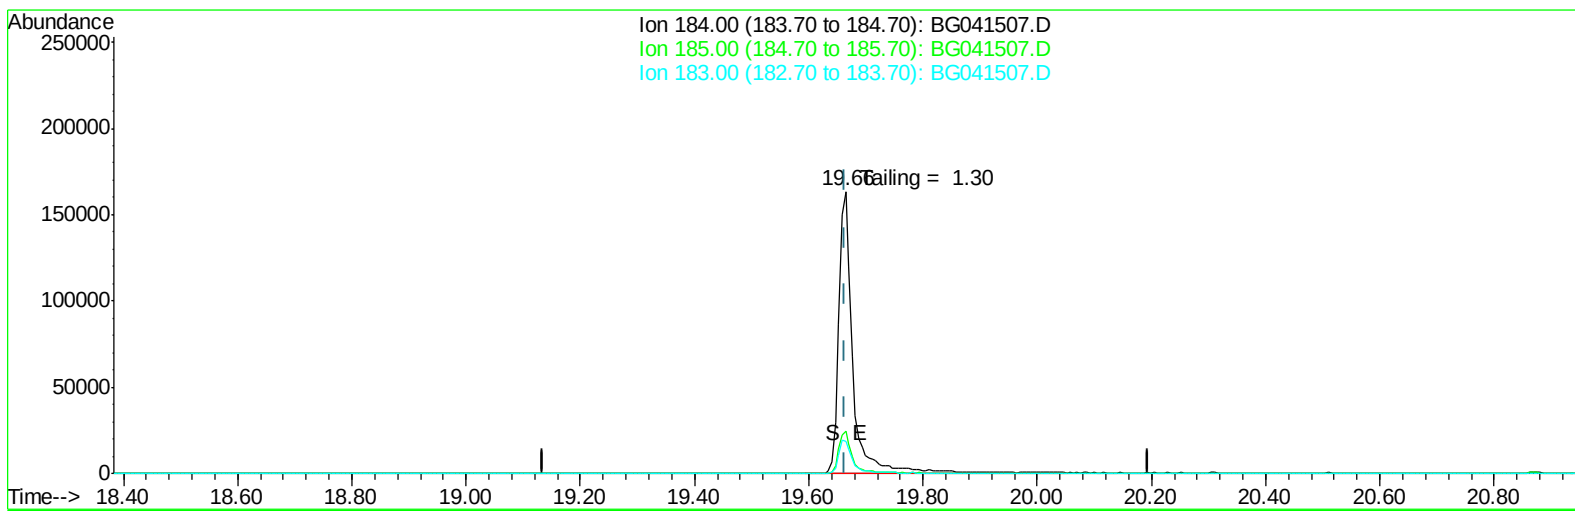

TIC: BG041507.D

(77) Benzidine

19.664min (-0.001) 0.00ng

response 272521

Ion	Exp%	Act%
184.00	100	100
185.00	15.90	14.98
183.00	11.80	11.34
0.00	0.00	0.00