
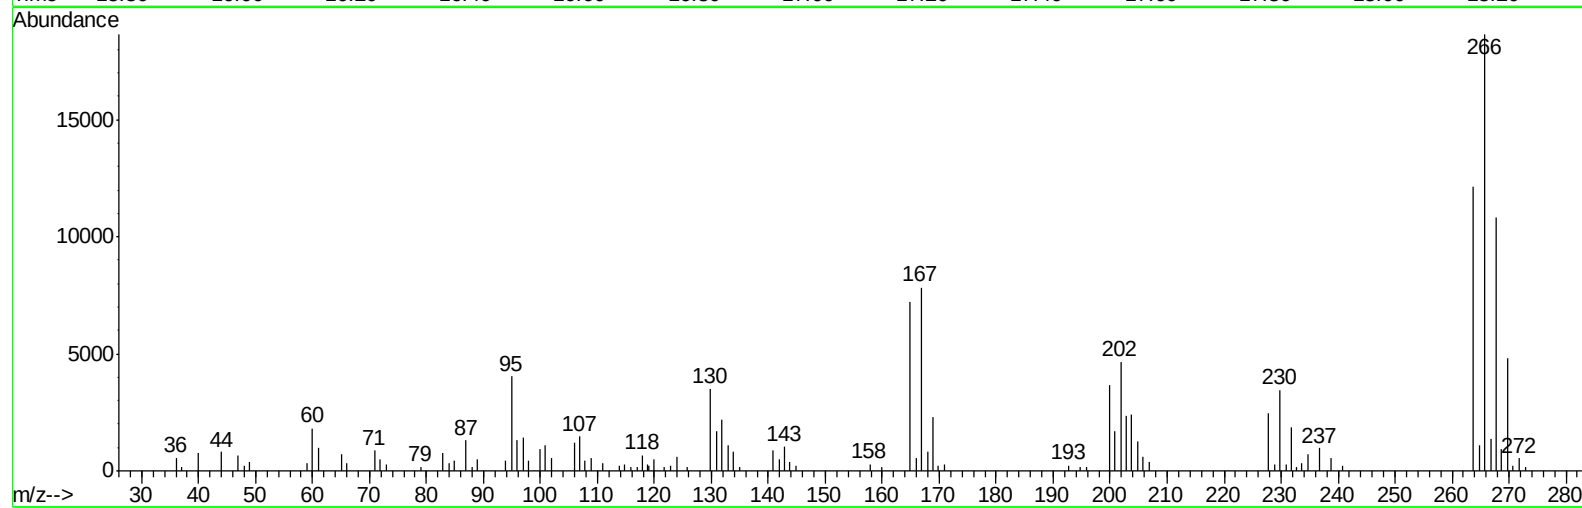


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG062819\
Data File : BG041526.D
Acq On : 29 Jun 2019 00:52
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 29 05:36:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG062619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 27 13:25:55 2019
Response via : Initial Calibration

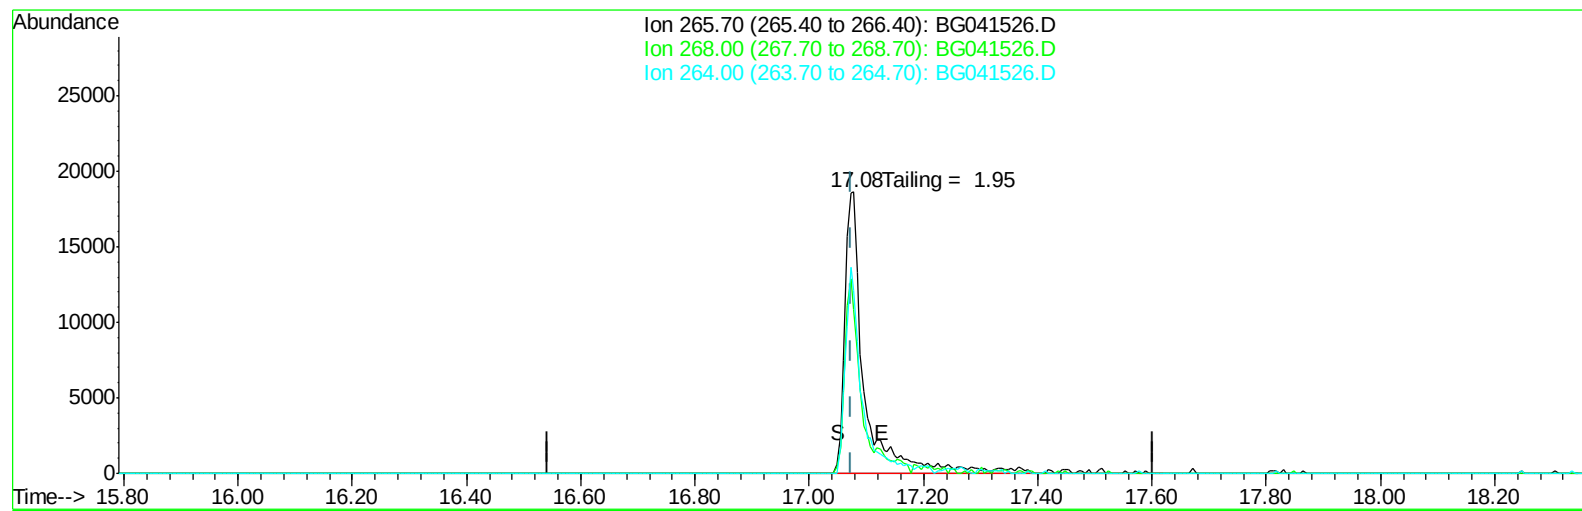

TIC: BG041526.D

(70) Pentachlorophenol (C)



17.078min (+0.004) 22547.14ng

response 41667

Ion	Exp%	Act%
265.70	100	100
268.00	58.70	62.98
264.00	59.20	65.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG062819\
Data File : BG041526.D
Acq On : 29 Jun 2019 00:52
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 29 05:36:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG062619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 27 13:25:55 2019
Response via : Initial Calibration

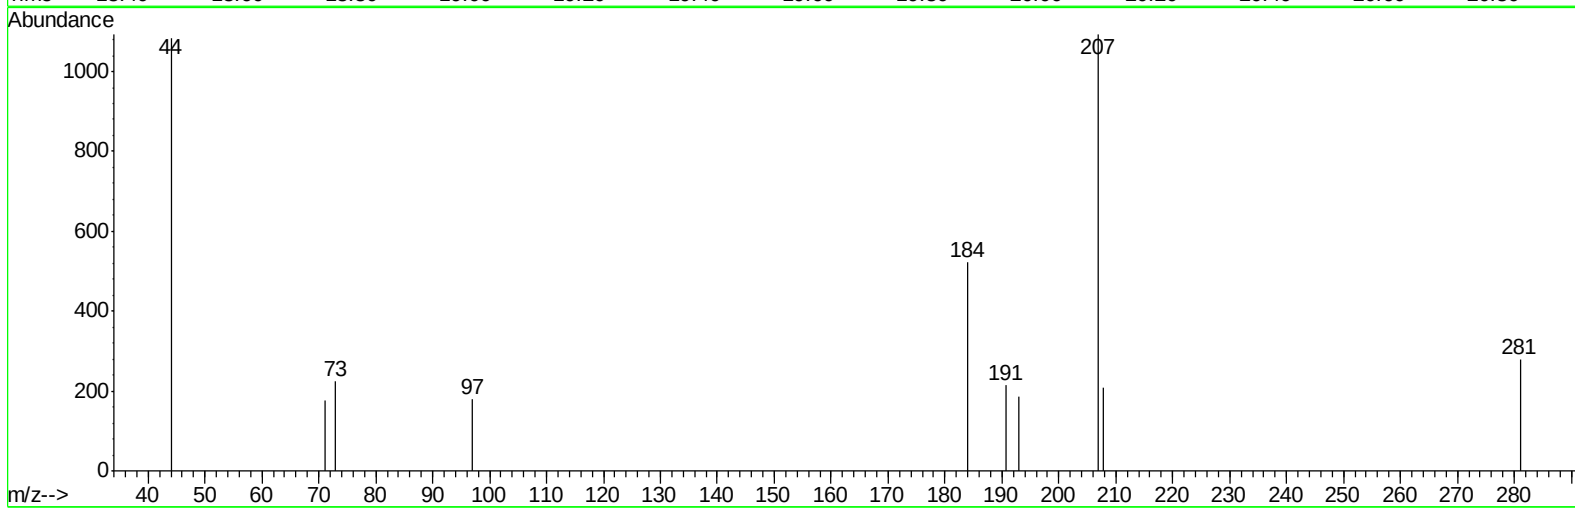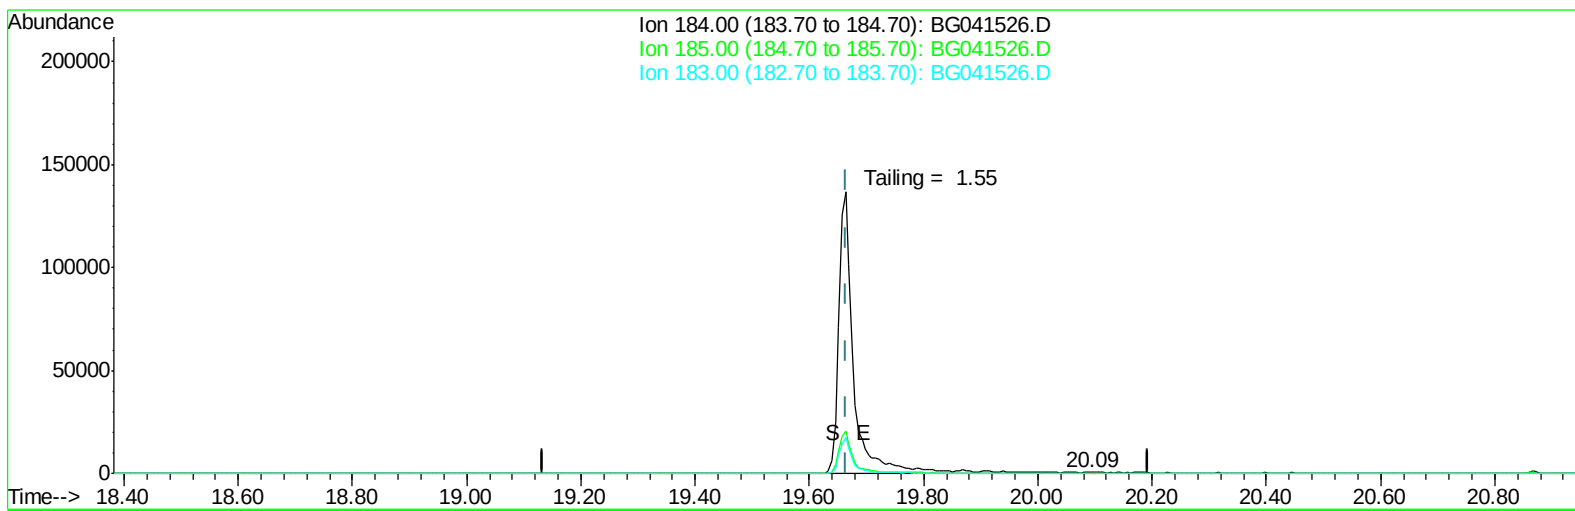

TIC: BG041526.D

(77) Benzidine

20.092min (+0.427) 230.79ng m

response 297

Ion	Exp%	Act%
184.00	100	100
185.00	15.90	0.00#
183.00	11.80	0.00#
0.00	0.00	0.00