


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062819\
 Data File : BG041507.D
 Acq On : 28 Jun 2019 11:12
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG062619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 27 13:25:55 2019

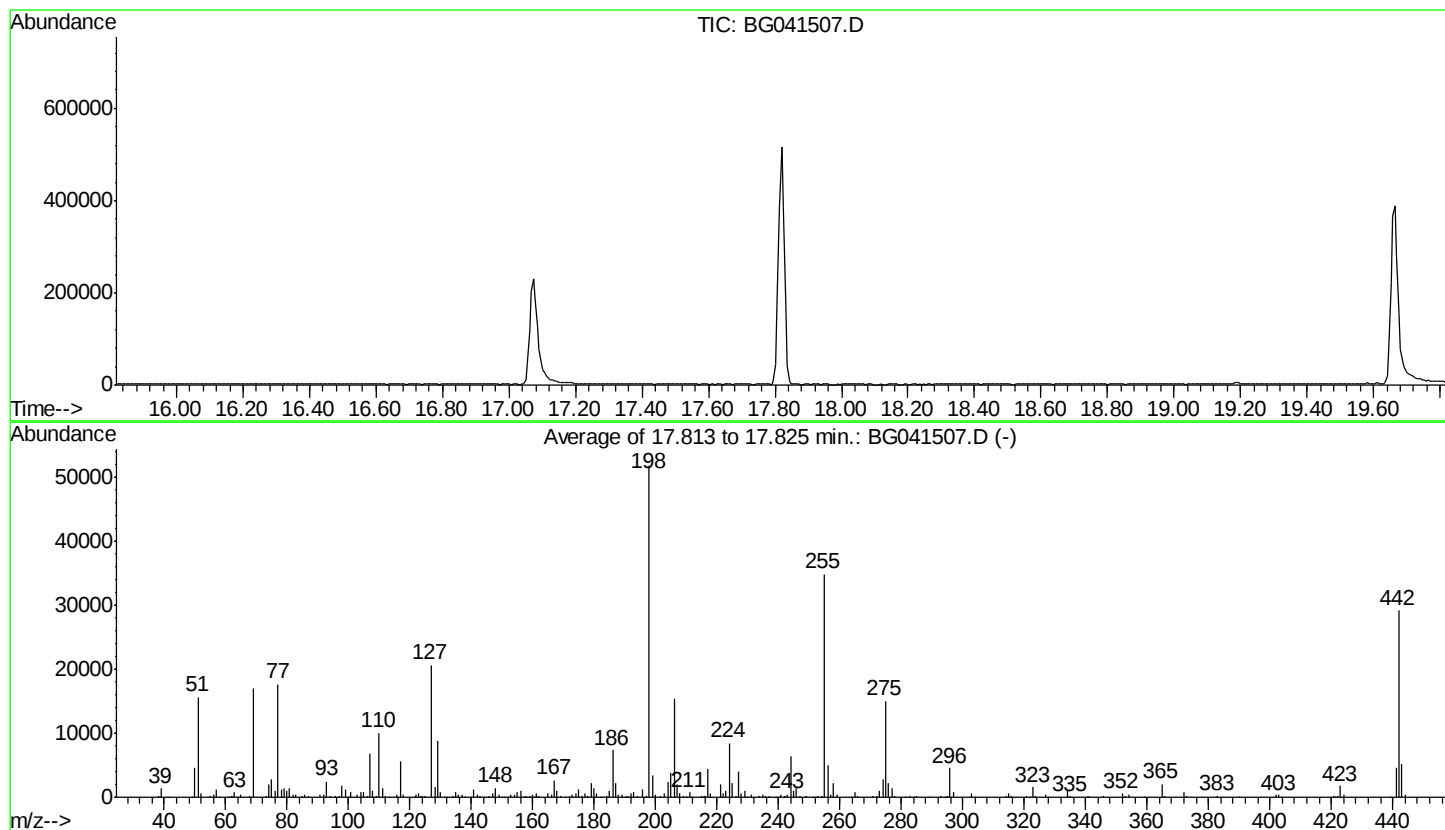

AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2500

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.2	15624	PASS
68	69	0.00	2	1.4	232	PASS
69	198	0.00	100	32.8	16970	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	39.9	20645	PASS
197	198	0.00	2	0.3	168	PASS
198	198	100	100	100.0	51784	PASS
199	198	5	9	6.7	3492	PASS
275	198	10	60	29.1	15074	PASS
365	198	1	100	4.0	2058	PASS
441	198	0.01	100	9.1	4692	PASS
442	198	50	100	56.2	29098	PASS
443	442	15	24	18.2	5296	PASS