


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_G\DATA\BG062819\  
 Data File : BG041526.D  
 Acq On : 29 Jun 2019 00:52  
 Operator : HP/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG062619.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Jun 27 13:25:55 2019

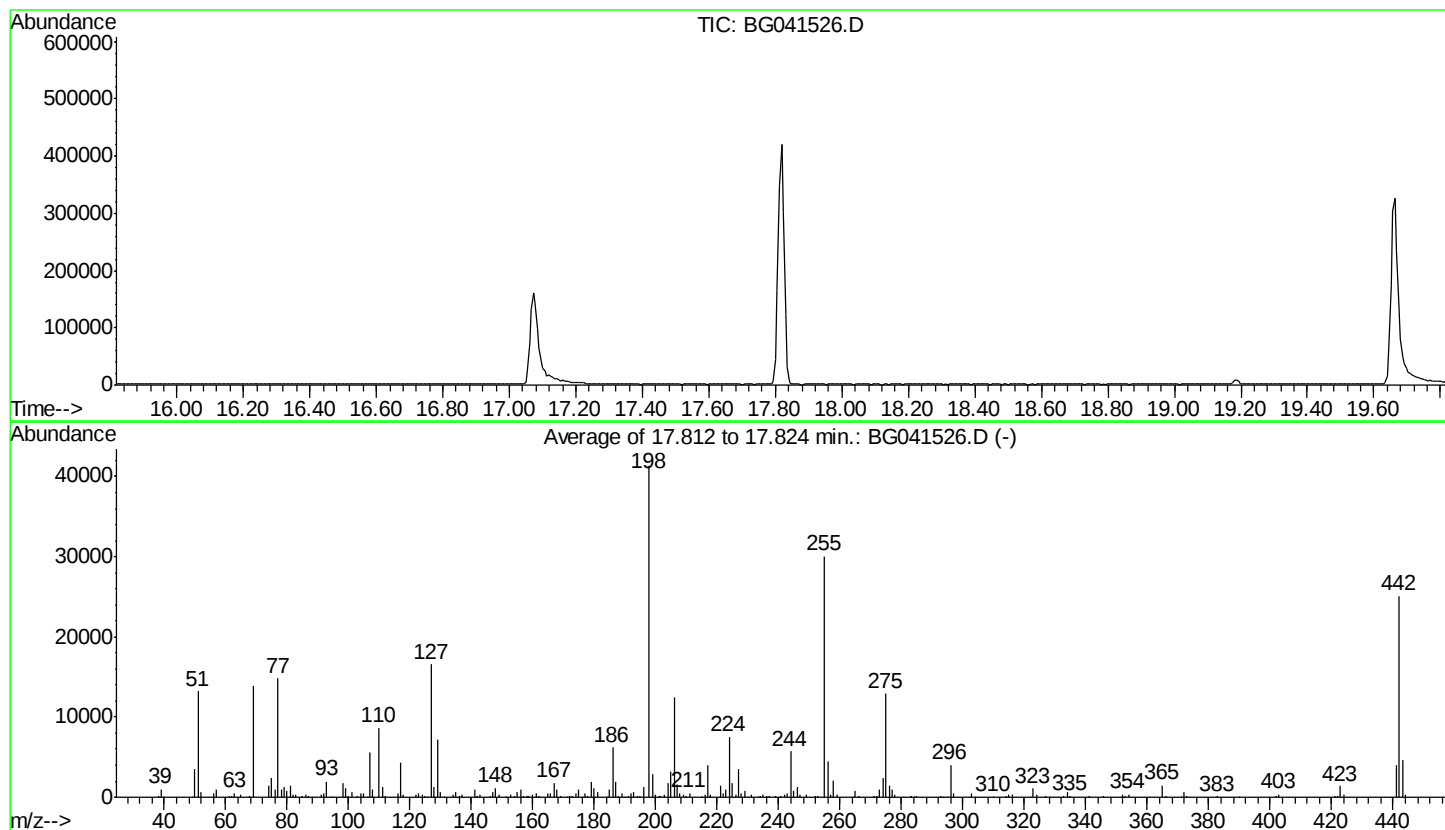

AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2500

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 31.9      | 13205   | PASS             |
| 68          | 69           | 0.00         | 2            | 0.8       | 111     | PASS             |
| 69          | 198          | 0.00         | 100          | 33.7      | 13925   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 40.1      | 16589   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 41352   | PASS             |
| 199         | 198          | 5            | 9            | 7.1       | 2938    | PASS             |
| 275         | 198          | 10           | 60           | 31.1      | 12879   | PASS             |
| 365         | 198          | 1            | 100          | 3.7       | 1516    | PASS             |
| 441         | 198          | 0.01         | 100          | 9.6       | 3986    | PASS             |
| 442         | 198          | 50           | 100          | 60.6      | 25072   | PASS             |
| 443         | 442          | 15           | 24           | 18.6      | 4665    | PASS             |