
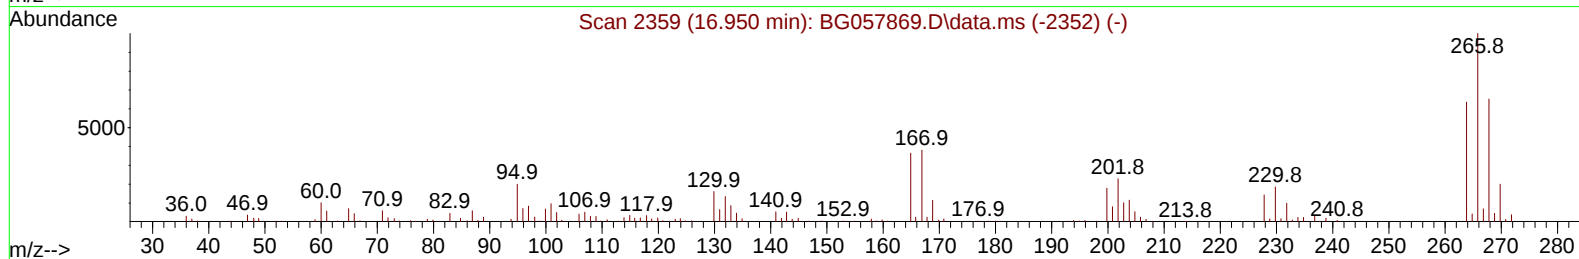
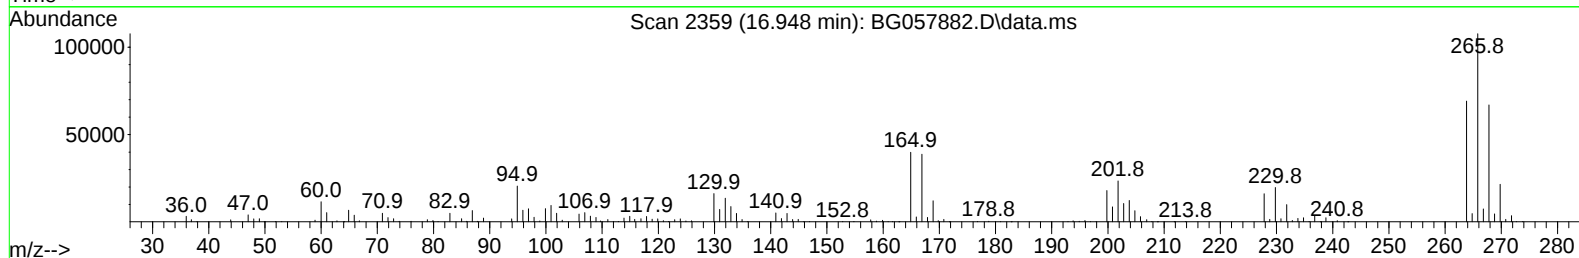


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062823\
Data File : BG057882.D
Acq On : 28 Jun 2023 7:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 28 11:48:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG062723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 28 01:12:33 2023
Response via : Initial Calibration

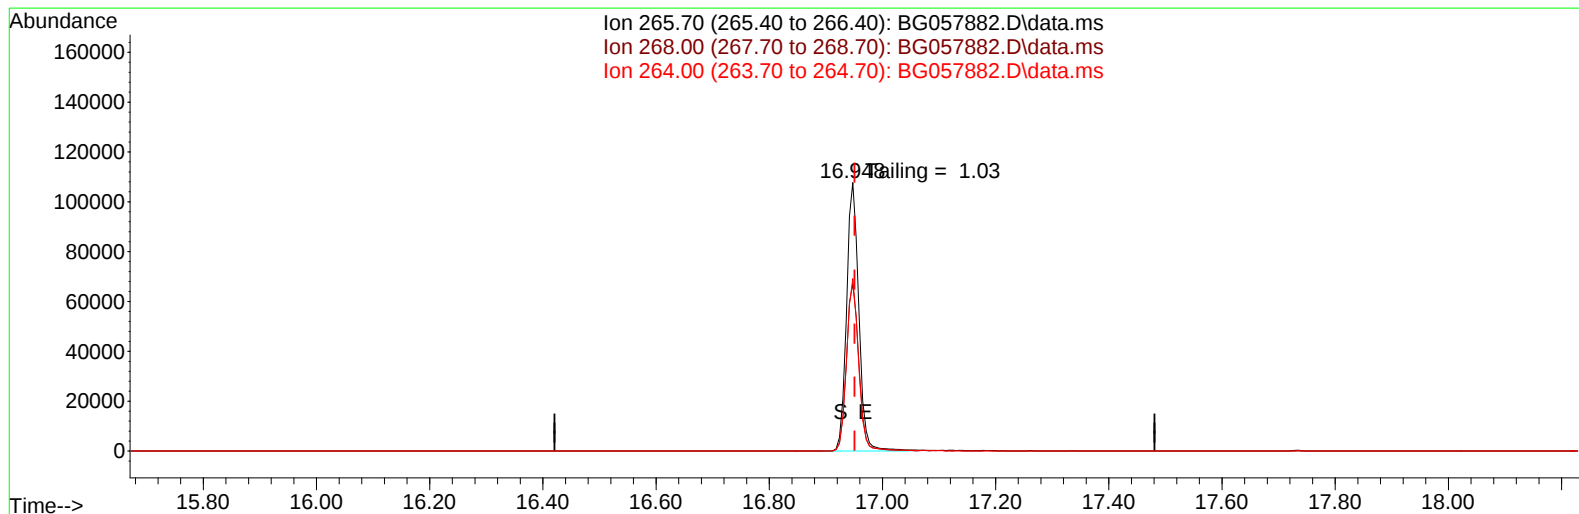

TIC: BG057882.D\data.ms

(70) Pentachlorophenol (C)




16.948min (-0.003) 29473.42 ng

response 161805

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.20	62.20
264.00	63.60	64.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062823\
Data File : BG057882.D
Acq On : 28 Jun 2023 7:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 28 11:48:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG062723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 28 01:12:33 2023
Response via : Initial Calibration

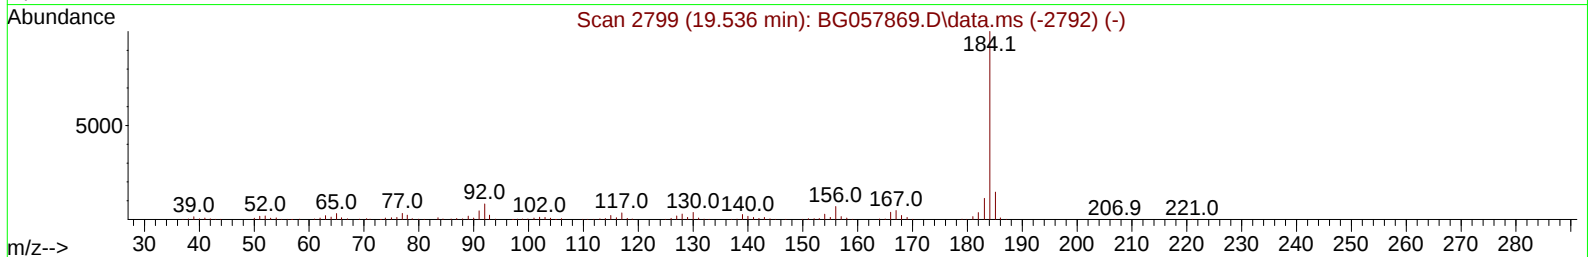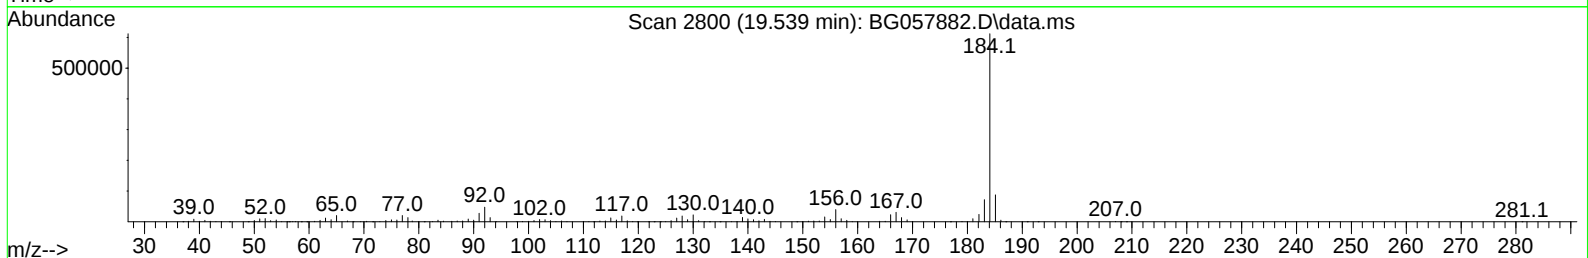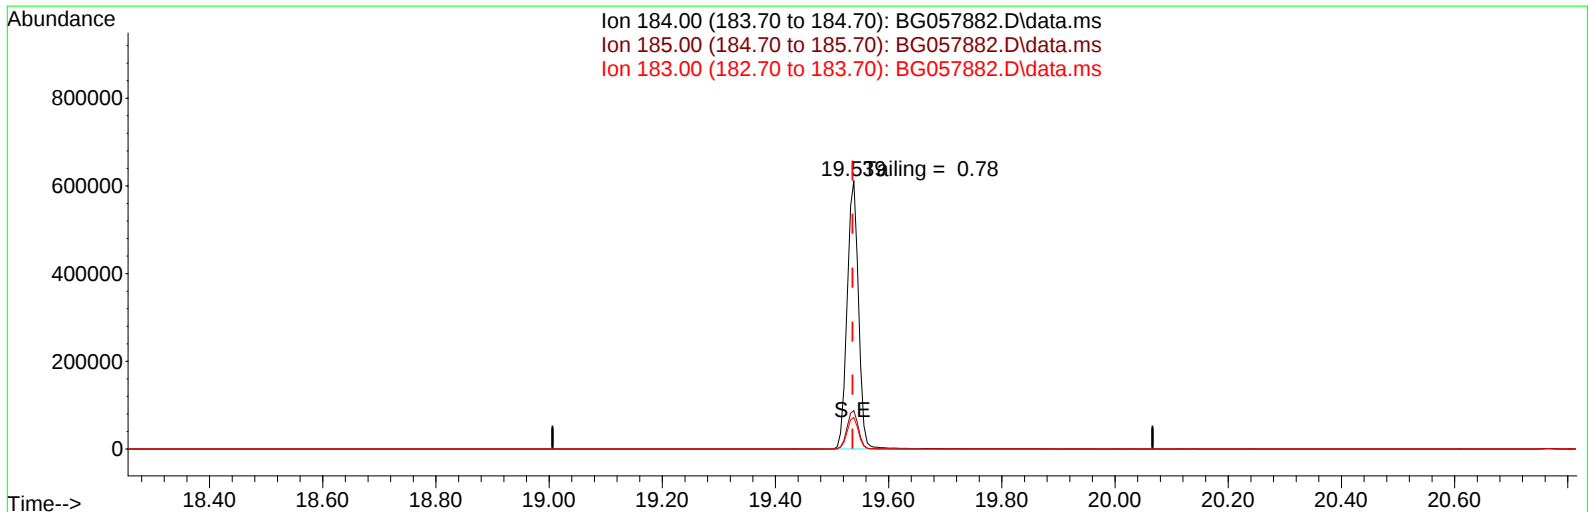

TIC: BG057882.D\data.ms

(77) Benzidine**19.539min (+ 0.003) 0.00 ng****response 856292**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.35
183.00	11.20	11.78
0.00	0.00	0.00