


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062823\
Data File : BG057882.D
Acq On : 28 Jun 2023 7:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG062723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jun 28 01:12:33 2023

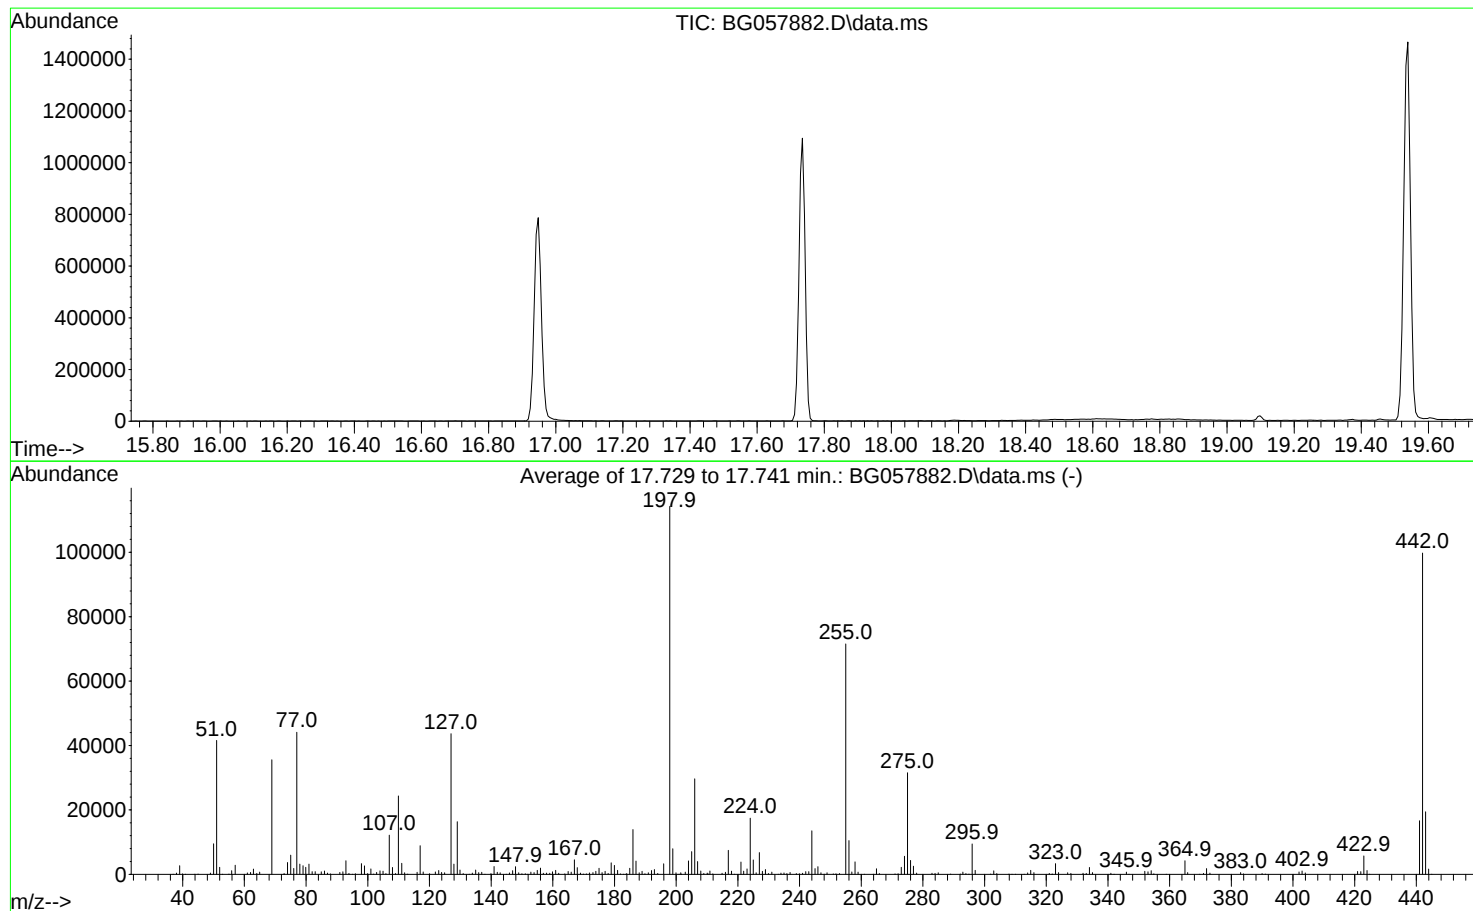

AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.4	41568	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.2	35592	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	38.3	43691	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	114208	PASS
199	198	5	9	7.0	7972	PASS
275	198	10	60	27.6	31571	PASS
365	198	1	100	3.7	4204	PASS
441	198	0.01	100	14.6	16634	PASS
442	442	50	100	100.0	99765	PASS
443	442	15	24	19.5	19442	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/28/2023	BNA_G	<u>BG057882.D</u>
Compound Name	Response	Retention Time
DDT	387295	20.767
DDD	20186	20.326
DDE	439	19.815
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20625	407920	5.06

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062823\
Data File : BG057882.D
Acq On : 28 Jun 2023 7:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 28 11:48:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG062723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 28 01:12:33 2023
Response via : Initial Calibration

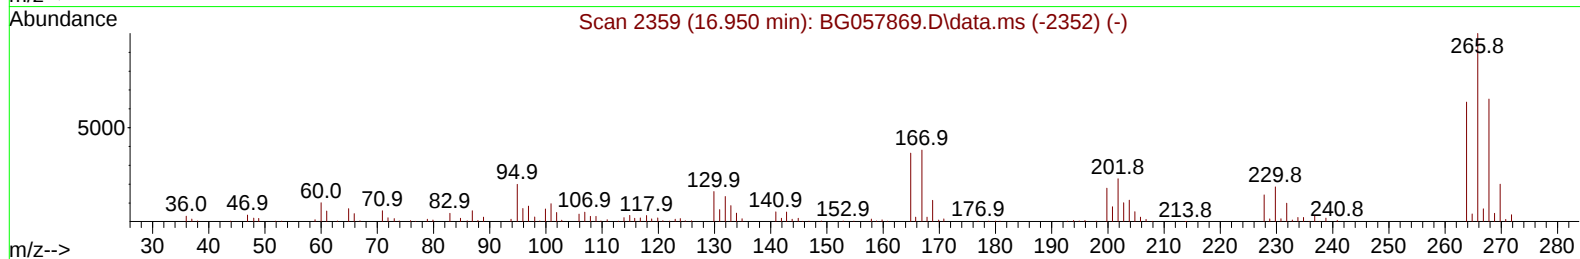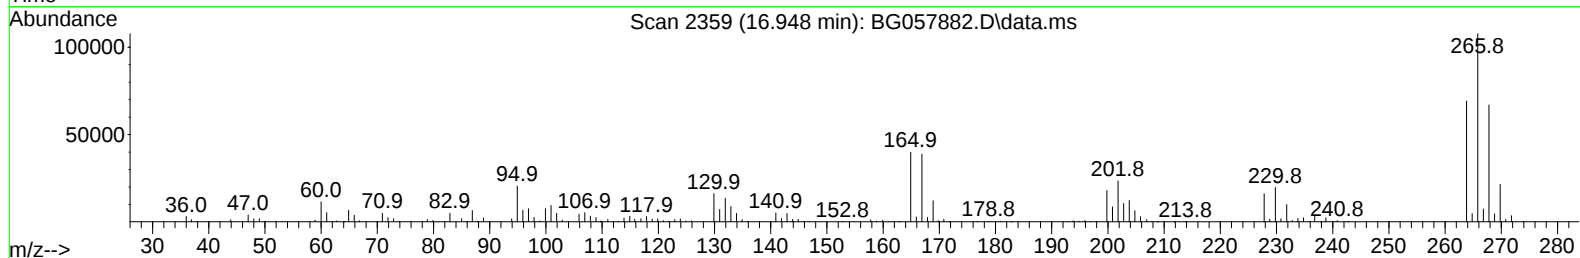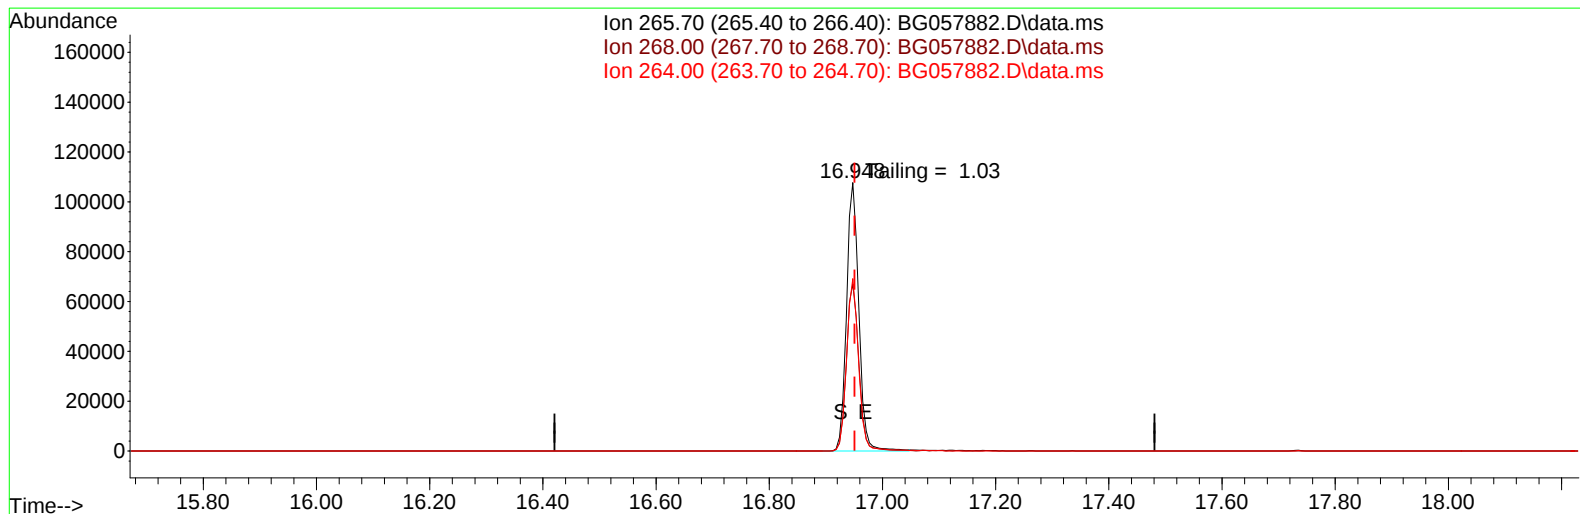

TIC: BG057882.D\data.ms

(70) Pentachlorophenol (C)

16.948min (-0.003) 29473.42 ng




response 161805

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.20	62.20
264.00	63.60	64.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062823\
Data File : BG057882.D
Acq On : 28 Jun 2023 7:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 28 11:48:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG062723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 28 01:12:33 2023
Response via : Initial Calibration

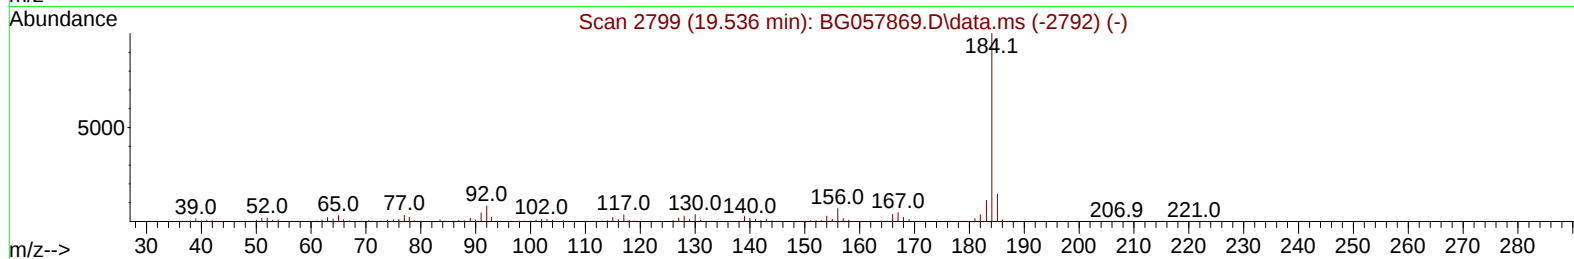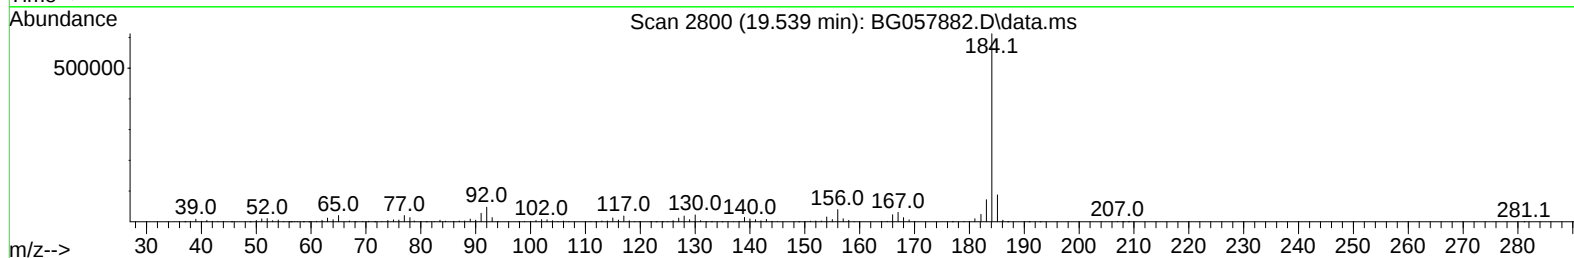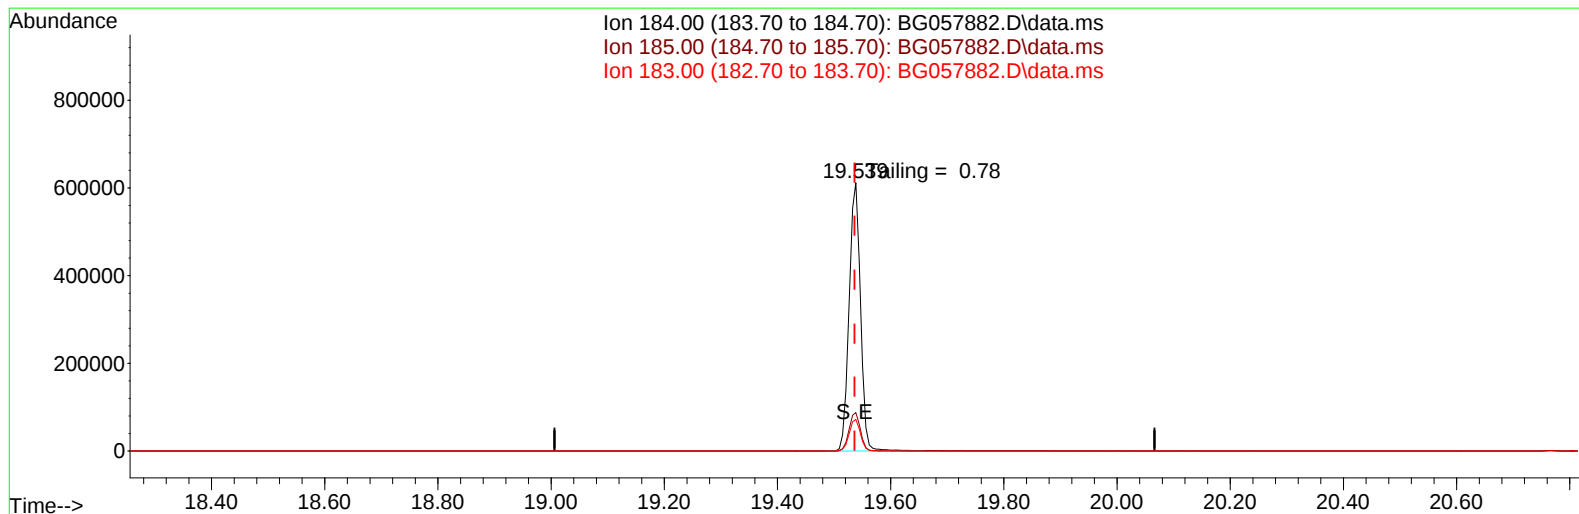

TIC: BG057882.D\data.ms

(77) Benzidine

19.539min (+ 0.003) 0.00 ng

response 856292

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.35
183.00	11.20	11.78
0.00	0.00	0.00