

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062824\
 Data File : BG061801.D
 Acq On : 29 Jun 2024 11:15
 Operator : MA/JU
 Sample : P2897-21
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 COT69

Quant Time: Jul 01 00:29:14 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 27 12:23:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.054	152	73220	20.000	ng/ul	0.00
20) Naphthalene-d8	10.869	136	340183	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.682	164	228108	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.426	188	509090	20.000	ng/ul	0.00
79) Chrysene-d12	21.691	240	413572	20.000	ng/ul	0.00
88) Perylene-d12	24.905	264	477355	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.454	96	9004	4.442	ng/uL	0.00
4) Pyridine-d5	3.871	84	128216	20.922	ng/ul	0.00
7) Phenol-d5	7.202	99	183704	23.111	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.379	67	111095	22.420	ng/ul	0.00
11) 2-Chlorophenol-d4	7.584	132	127082	23.298	ng/ul	0.00
15) 4-Methylphenol-d8	8.753	113	136138	22.155	ng/ul	0.00
21) Nitrobenzene-d5	9.218	128	64220	27.803	ng/ul	0.00
24) 2-Nitrophenol-d4	9.940	143	74477	31.836	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.481	165	139784	25.234	ng/ul	0.00
31) 4-Chloroaniline-d4	10.998	131	192725	22.980	ng/ul	0.00
46) Dimethylphthalate-d6	14.088	166	444304	25.311	ng/ul	0.00
49) Acenaphthylene-d8	14.382	160	514148	26.726	ng/ul	0.00
54) 4-Nitrophenol-d4	14.864	143	71589	23.746	ng/ul	0.00
60) Fluorene-d10	15.675	176	396610	25.809	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.780	200	40978	18.824	ng/ul	0.00
73) Anthracene-d10	17.525	188	632297	27.210	ng/ul	0.00
81) Pyrene-d10	19.811	212	688561	29.806	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.688	264	650329	28.524	ng/ul	0.00
Target Compounds						
					Qvalue	
30) Naphthalene	10.916	128	78458	4.122	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062824\
Data File : BG061801.D
Acq On : 29 Jun 2024 11:15
Operator : MA/JU
Sample : P2897-21
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0T69

Quant Time: Jul 01 00:29:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 27 12:23:53 2024
Response via : Initial Calibration

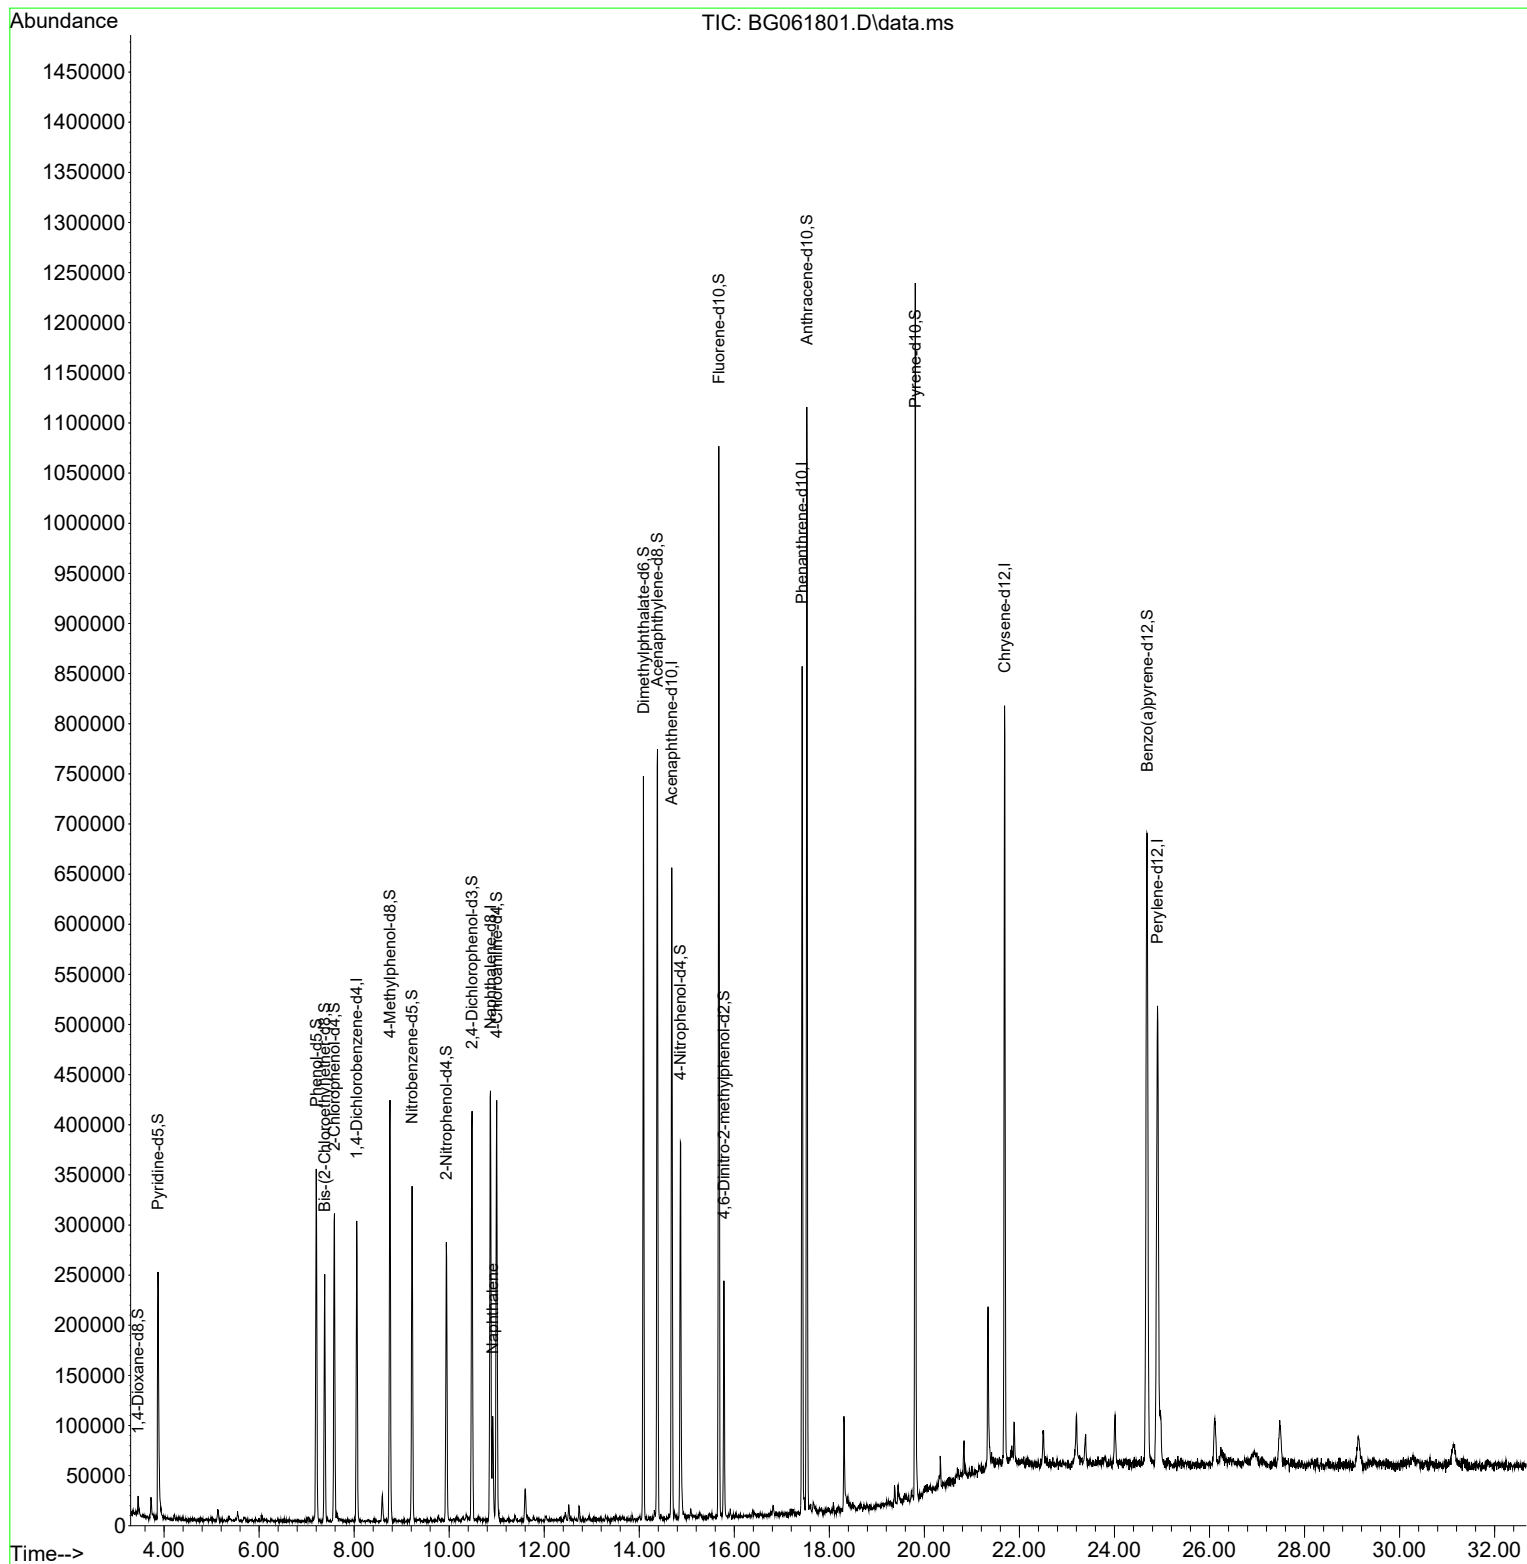

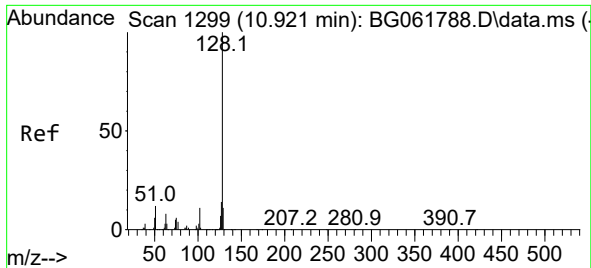

#30
Naphthalene
Concen: 4.122 ng/ul
RT: 10.916 min Scan# 11
Delta R.T. -0.005 min
Lab File: BG061801.D
Acq: 29 Jun 2024 11:15

Instrument :
BNA_G
ClientSampleId :
C0T69

Tgt Ion:128 Resp: 78458
Ion Ratio Lower Upper
128 100
129 10.4 9.0 13.6
127 14.3 10.5 15.7

