

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062824\
 Data File : BG061803.D
 Acq On : 29 Jun 2024 12:35
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD020546

Quant Time: Jul 01 00:29:56 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 27 12:23:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.054	152	81929	20.000	ng/u1	0.00
20) Naphthalene-d8	10.868	136	381229	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.687	164	266101	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.425	188	620393	20.000	ng/u1	0.00
79) Chrysene-d12	21.691	240	513453	20.000	ng/u1	0.00
88) Perylene-d12	24.905	264	598431	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.459	96	18141	7.999	ng/uL	0.00
4) Pyridine-d5	3.870	84	133298	19.439	ng/u1	0.00
7) Phenol-d5	7.202	99	174902	19.665	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.378	67	109729	19.791	ng/u1	0.00
11) 2-Chlorophenol-d4	7.584	132	121757	19.949	ng/u1	0.00
15) 4-Methylphenol-d8	8.753	113	134783	19.603	ng/u1	0.00
21) Nitrobenzene-d5	9.223	128	59343	22.925	ng/u1	0.00
24) 2-Nitrophenol-d4	9.940	143	72240	27.555	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.480	165	136744	22.028	ng/u1	0.00
31) 4-Chloroaniline-d4	10.997	131	187833	19.985	ng/u1	0.00
46) Dimethylphthalate-d6	14.088	166	424096	20.710	ng/u1	0.00
49) Acenaphthylene-d8	14.382	160	480077	21.392	ng/u1	0.00
54) 4-Nitrophenol-d4	14.869	143	73052	20.772	ng/u1	0.00
60) Fluorene-d10	15.674	176	379966	21.195	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.786	200	59793	22.539	ng/u1	0.00
73) Anthracene-d10	17.525	188	610176	21.547	ng/u1	0.00
81) Pyrene-d10	19.805	212	633805	22.099	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.681	264	613507	21.465	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.494	88	20285	7.197	ng/uL#	79
5) Pyridine	3.888	79	143214	19.429	ng/u1	91
6) Benzaldehyde	7.196	77	108359	24.758	ng/u1	97
8) Phenol	7.231	94	182155	19.462	ng/u1	95
10) Bis(2-Chloroethyl)ether	7.472	93	132813	18.853	ng/u1#	91
12) 2-Chlorophenol	7.619	128	127641	20.845	ng/u1	98
13) 2-Methylphenol	8.489	108	129115	19.717	ng/u1	93
14) 2,2'-oxybis(1-Chloropr...	8.583	45	283736	19.714	ng/u1	96
16) Acetophenone	8.882	105	211224	18.656	ng/u1	97
17) N-Nitroso-di-n-propyla...	8.859	70	110279	18.132	ng/u1#	96
18) 4-Methylphenol	8.818	108	137410	18.730	ng/u1	92
19) Hexachloroethane	9.141	117	52737	21.480	ng/u1	91
22) Nitrobenzene	9.264	77	172982	23.197	ng/u1	94
23) Isophorone	9.787	82	341162	19.893	ng/u1	99
25) 2-Nitrophenol	9.975	139	70552	25.735	ng/u1#	74
26) 2,4-Dimethylphenol	10.028	107	160536	20.938	ng/u1	98
27) Bis(2-Chloroethoxy)met...	10.269	93	197601	20.368	ng/u1	95
29) 2,4-Dichlorophenol	10.504	162	125643	22.090	ng/u1	98
30) Naphthalene	10.915	128	434212	20.356	ng/u1	98
32) 4-Chloroaniline	11.021	127	178963	19.199	ng/u1	96
33) Hexachlorobutadiene	11.191	225	94069	23.944	ng/u1	93
34) Caprolactam	11.779	113	33840	14.389	ng/u1	93
35) 4-Chloro-3-methylphenol	12.137	107	166982	20.995	ng/u1	92
36) 2-Methylnaphthalene	12.519	142	290755	19.317	ng/u1	94

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062824\
 Data File : BG061803.D
 Acq On : 29 Jun 2024 12:35
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD020546

Quant Time: Jul 01 00:29:56 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 27 12:23:53 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.737	142	307360	19.138	ng/ul#	91
39) 1,2,4,5-Tetrachloroben...	12.878	216	164282	21.814	ng/ul	97
40) Hexachlorocyclopentadiene	12.854	237	57310	12.790	ng/ul#	99
41) 2,4,6-Trichlorophenol	13.118	196	112335	23.120	ng/ul	93
42) 2,4,5-Trichlorophenol	13.118	196	98360	18.572	ng/ul	93
43) 1,1'-Biphenyl	13.518	154	414943	21.527	ng/ul	99
44) 2-Chloronaphthalene	13.565	162	312224	21.087	ng/ul	99
45) 2-Nitroaniline	13.765	65	133551	26.348	ng/ul	92
47) Dimethylphthalate	14.135	163	414641	20.391	ng/ul	99
48) 2,6-Dinitrotoluene	14.258	165	88804	26.317	ng/ul#	93
50) Acenaphthylene	14.405	152	508313	20.291	ng/ul	98
51) 3-Nitroaniline	14.587	138	88359	25.570	ng/ul#	98
52) Acenaphthene	14.746	153	360556	20.783	ng/ul	89
53) 2,4-Dinitrophenol	14.787	184	35449	20.673	ng/ul#	84
55) 4-Nitrophenol	14.887	109	79059	21.769	ng/ul	95
56) Dibenzofuran	15.081	168	501434	20.655	ng/ul	92
57) 2,4-Dinitrotoluene	15.040	165	133945	26.742	ng/ul	95
58) 2,3,4,6-Tetrachlorophenol	15.304	232	108281	20.852	ng/ul#	96
59) Diethylphthalate	15.498	149	436323	20.834	ng/ul	97
61) Fluorene	15.727	166	419777	20.893	ng/ul	91
62) 4-Chlorophenyl-phenyle...	15.721	204	209438	20.998	ng/ul	95
63) 4-Nitroaniline	15.745	138	93208	25.461	ng/ul	95
66) 4,6-Dinitro-2-methylph...	15.798	198	64816	21.570	ng/ul#	90
67) N-Nitrosodiphenylamine	15.933	169	352260	21.957	ng/ul	98
68) 4-Bromophenyl-phenylether	16.614	248	145169	22.726	ng/ul	95
69) Hexachlorobenzene	16.726	284	170237	21.961	ng/ul	93
70) Atrazine	16.879	200	137299	21.426	ng/ul	97
71) Pentachlorophenol	17.067	266	94093	19.926	ng/ul	98
72) Phenanthrene	17.472	178	673618	20.639	ng/ul	99
74) Anthracene	17.560	178	704907	21.120	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.483	216	165568	23.954	ng/ul	97
76) Pentachlorobenzene	14.999	250	191075	23.020	ng/ul	95
77) Carbazole	17.825	167	601136	21.212	ng/ul	98
78) Di-n-butylphthalate	18.383	149	762367	22.493	ng/ul	98
80) Fluoranthene	19.476	202	772828	23.224	ng/ul	96
82) Pyrene	19.834	202	786513	22.228	ng/ul	97
83) Butylbenzylphthalate	20.721	149	319938	24.834	ng/ul	96
84) 3,3'-Dichlorobenzidine	21.585	252	252071	23.218	ng/ul#	96
85) Benzo(a)anthracene	21.667	228	765555	21.241	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.579	149	458374	24.205	ng/ul#	98
87) Chrysene	21.732	228	711826	20.872	ng/ul	98
89) Di-n-octyl phthalate	22.795	149	787605	24.953	ng/ul	100
90) Benzo(b)fluoranthene	23.882	252	755847	21.011	ng/ul	96
91) Benzo(k)fluoranthene	23.947	252	785542	21.233	ng/ul	99
93) Benzo(a)pyrene	24.752	252	730019	21.079	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	28.559	276	936152	21.692	ng/ul	97
95) Dibenzo(a,h)anthracene	28.636	278	771780	21.506	ng/ul	97
96) Benzo(g,h,i)perylene	29.711	276	741146	21.304	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062824\
Data File : BG061803.D
Acq On : 29 Jun 2024 12:35
Operator : MA/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SSTD020546

Quant Time: Jul 01 00:29:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 27 12:23:53 2024
Response via : Initial Calibration




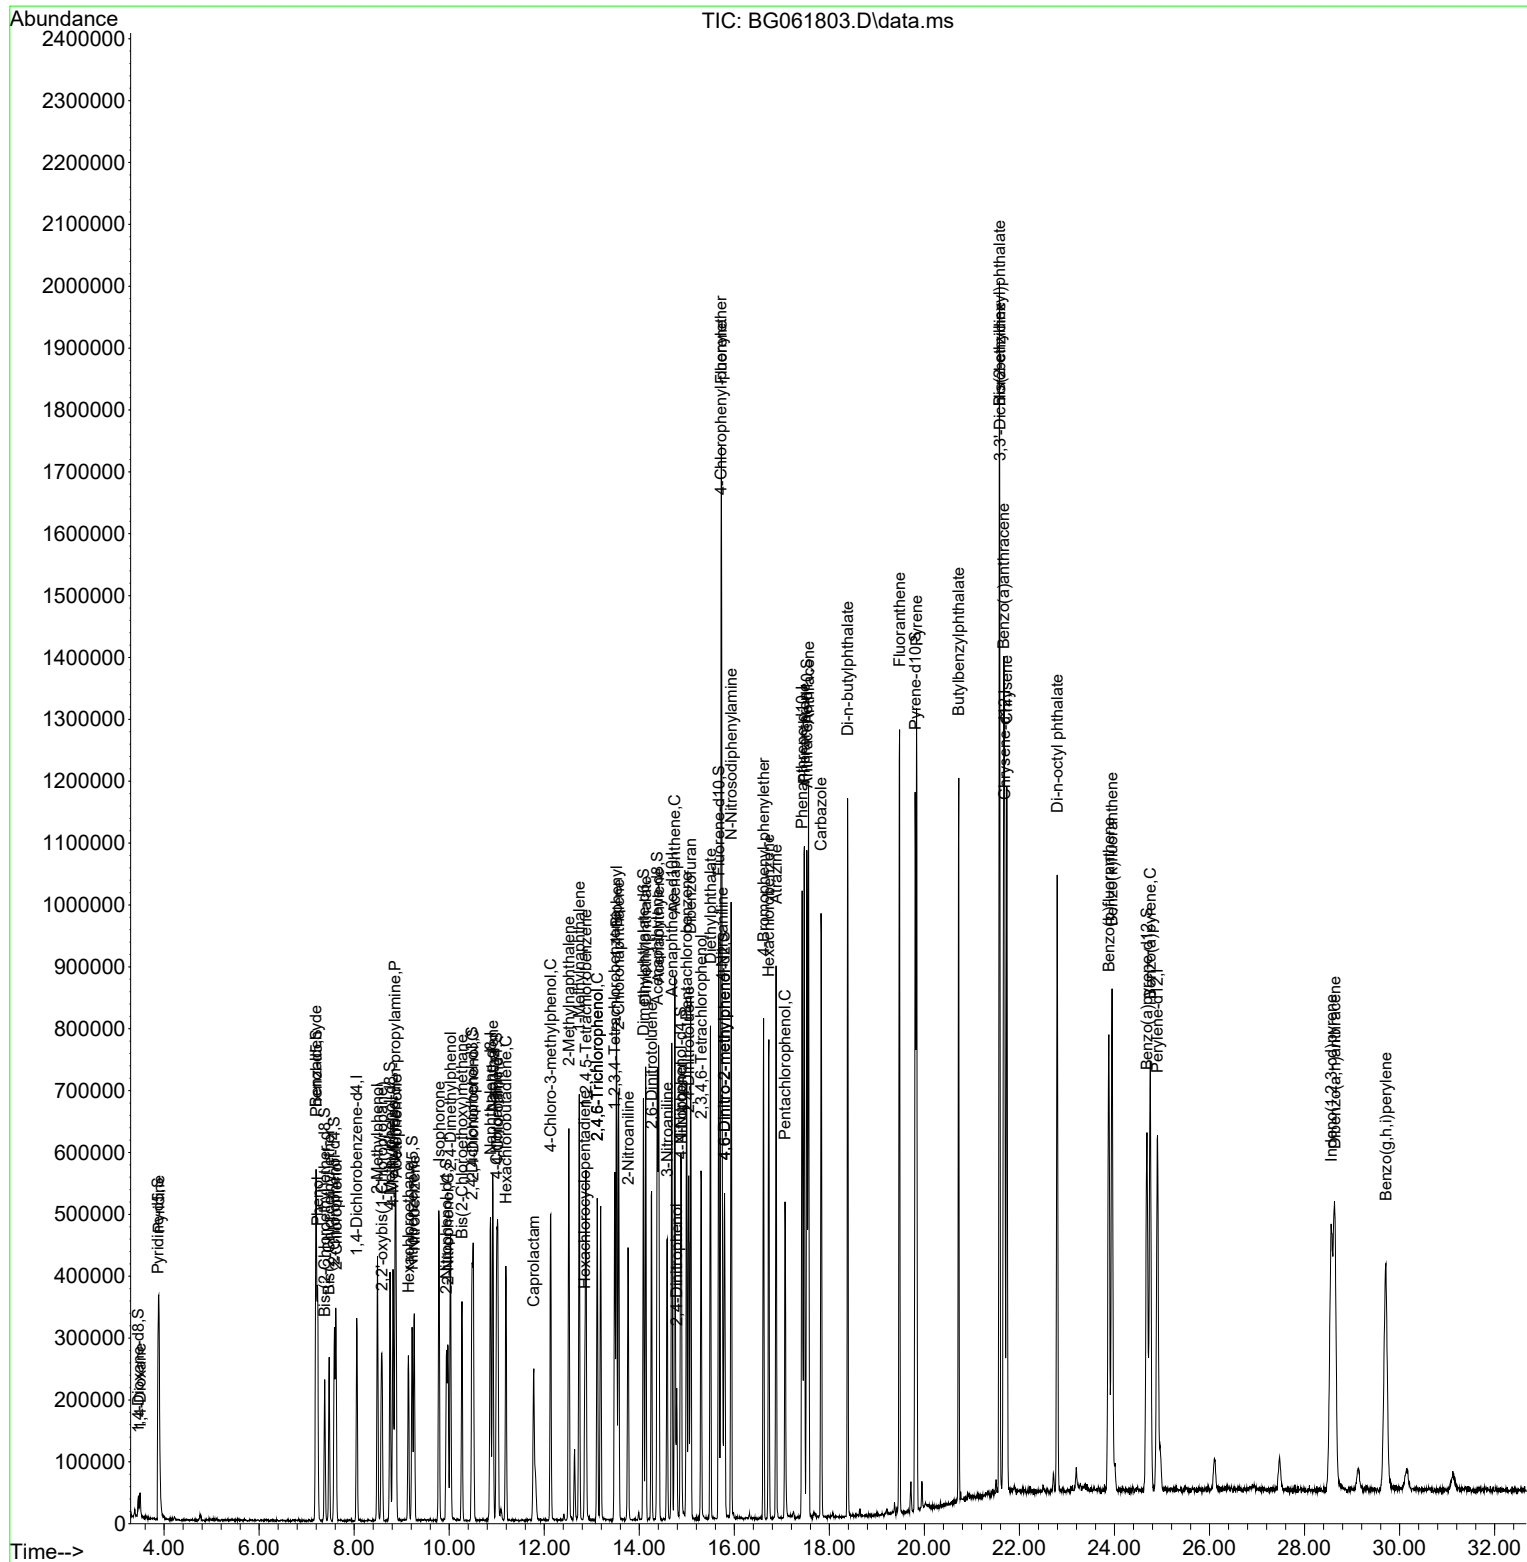




#2
1,4-Dioxane
Concen: 7.197 ng/uL
RT: 3.494 min Scan# 31
Delta R.T. 0.006 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35




Instrument :
BNA_G
ClientSampleId :
SSTD020546


Tgt Ion: 88 Resp: 20285
Ion Ratio Lower Upper
88 100
43 50.9 24.1 36.1#
58 90.8 63.0 94.6



#5
Pyridine
Concen: 19.429 ng/uL
RT: 3.888 min Scan# 102
Delta R.T. -0.005 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35

Tgt Ion: 79 Resp: 143214
Ion Ratio Lower Upper
79 100
52 118.8 84.4 126.6
51 55.4 43.0 64.6









#6
Benzaldehyde
Concen: 24.758 ng/ul
RT: 7.196 min Scan# 665
Delta R.T. 0.001 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35




Instrument :
BNA_G
ClientSampleId :
SSTD020546


Tgt Ion: 77 Resp: 108359
Ion Ratio Lower Upper
77 100
105 86.0 71.0 106.6
106 76.8 63.5 95.3

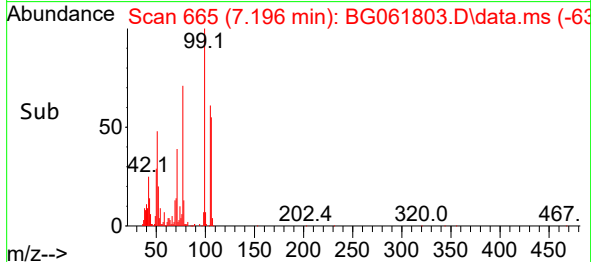

#8
Phenol
Concen: 19.462 ng/ul
RT: 7.231 min Scan# 671
Delta R.T. 0.001 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35

Tgt Ion: 94 Resp: 182155
Ion Ratio Lower Upper
94 100
65 28.8 25.8 38.6
66 43.3 36.9 55.3


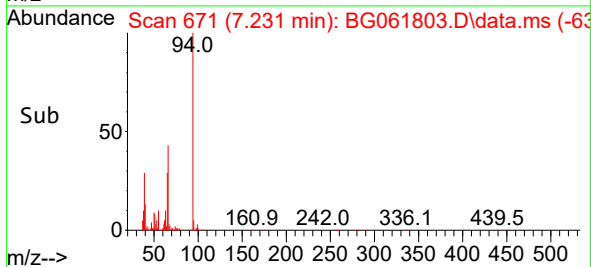

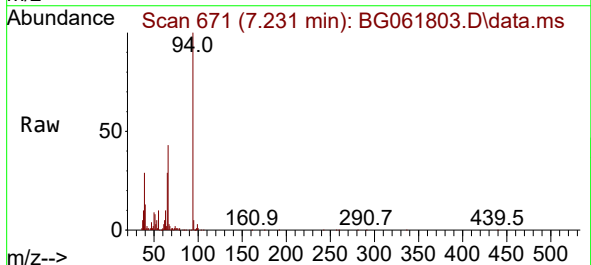




#10
Bis(2-Chloroethyl)ether
Concen: 18.853 ng/ul
RT: 7.472 min Scan# 712
Delta R.T. -0.005 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35




Instrument :
BNA_G
ClientSampleId :
SSTD020546


Tgt Ion: 93 Resp: 132813
Ion Ratio Lower Upper
93 100
63 98.3 72.5 108.7
95 33.9 21.8 32.8#



#12
2-Chlorophenol
Concen: 20.845 ng/ul
RT: 7.619 min Scan# 737
Delta R.T. 0.006 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35

Tgt Ion:128 Resp: 127641
Ion Ratio Lower Upper
128 100
64 55.5 43.2 64.8
130 31.5 24.1 36.1



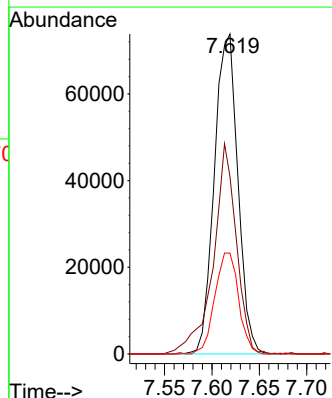





#13
2-Methylphenol
Concen: 19.717 ng/ul
RT: 8.489 min Scan# 886
Delta R.T. 0.001 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35




Instrument :
BNA_G
ClientSampleId :
SSTD020546


Tgt Ion:108 Resp: 129115
Ion Ratio Lower Upper
108 100
107 92.4 69.0 103.4



#14
2,2'-oxybis(1-Chloropropane)
Concen: 19.714 ng/ul
RT: 8.583 min Scan# 901
Delta R.T. 0.006 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35

Tgt Ion: 45 Resp: 283736
Ion Ratio Lower Upper
45 100
77 9.2 8.9 13.3
79 6.7 5.8 8.8









#16
Acetophenone
Concen: 18.656 ng/ul
RT: 8.882 min Scan# 91
Delta R.T. 0.001 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35




Instrument :
BNA_G
ClientSampleId :
SSTD020546


Tgt Ion:105 Resp: 211224
Ion Ratio Lower Upper
105 100
77 77.7 60.4 90.6
51 37.1 31.1 46.7



#17
N-Nitroso-di-n-propylamine
Concen: 18.132 ng/ul
RT: 8.859 min Scan# 948
Delta R.T. -0.005 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35

Tgt Ion: 70 Resp: 110279
Ion Ratio Lower Upper
70 100
42 81.9 62.7 94.1
101 10.3 5.8 8.8#
130 14.9 13.3 19.9









#18
4-Methylphenol
Concen: 18.730 ng/ul
RT: 8.818 min Scan# 941
Delta R.T. 0.001 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35




Instrument :
BNA_G
ClientSampleId :
SSTD020546


Tgt Ion:108 Resp: 137410
Ion Ratio Lower Upper
108 100
107 121.3 90.2 135.2



#19
Hexachloroethane
Concen: 21.480 ng/ul
RT: 9.141 min Scan# 996
Delta R.T. -0.005 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35

Tgt Ion:117 Resp: 52737
Ion Ratio Lower Upper
117 100
201 105.4 79.3 118.9
199 65.8 61.9 92.9









#22
Nitrobenzene
Concen: 23.197 ng/ul
RT: 9.264 min Scan# 1017
Delta R.T. 0.001 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35




Instrument :
BNA_G
ClientSampleId :
SSTD020546


Tgt Ion: 77 Resp: 172982
Ion Ratio Lower Upper
77 100
123 39.9 29.0 43.6
65 15.9 11.0 16.6



#23
Isophorone
Concen: 19.893 ng/ul
RT: 9.787 min Scan# 1106
Delta R.T. 0.001 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35

Tgt Ion: 82 Resp: 341162
Ion Ratio Lower Upper
82 100
95 7.4 6.4 9.6
138 15.2 11.7 17.5









#25
2-Nitrophenol
Concen: 25.735 ng/ul
RT: 9.975 min Scan# 1138
Delta R.T. 0.001 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35




Instrument :
BNA_G
ClientSampleId :
SSTD020546


Tgt Ion:139 Resp: 70552
Ion Ratio Lower Upper
139 100
65 75.9 42.2 63.4#
109 42.3 27.0 40.4#



#26
2,4-Dimethylphenol
Concen: 20.938 ng/ul
RT: 10.028 min Scan# 1147
Delta R.T. 0.001 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35

Tgt Ion:107 Resp: 160536
Ion Ratio Lower Upper
107 100
121 46.1 34.5 51.7
122 76.0 60.3 90.5







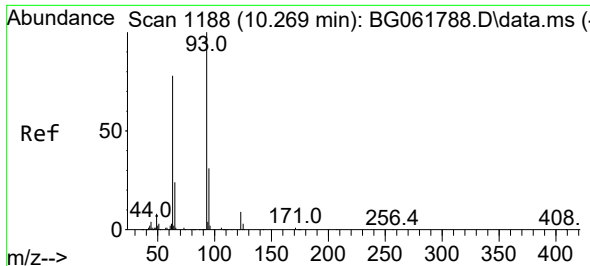

#27
 Bis(2-Chloroethoxy)methane
 Concen: 20.368 ng/ul
 RT: 10.269 min Scan# 1188
 Delta R.T. -0.005 min
 Lab File: BG061803.D
 Acq: 29 Jun 2024 12:35




Instrument :
 BNA_G
 ClientSampleId :
 SSTD020546


Tgt Ion: 93 Resp: 197601
 Ion Ratio Lower Upper
 93 100
 95 30.9 27.4 41.2
 123 8.8 6.7 10.1

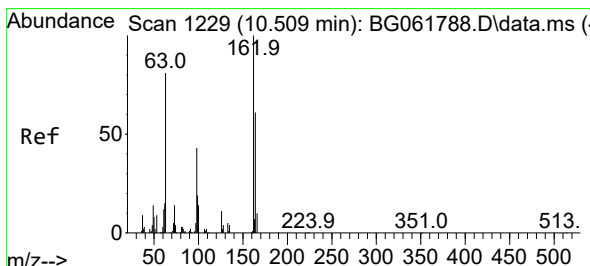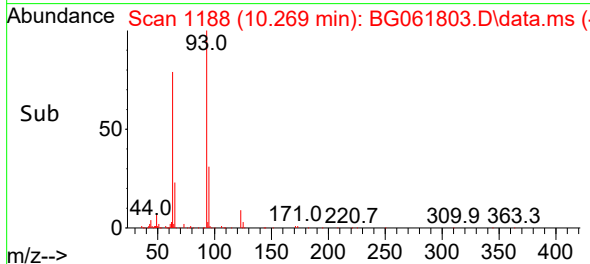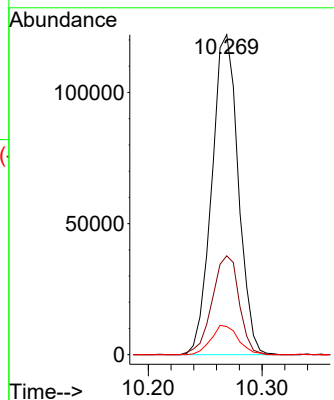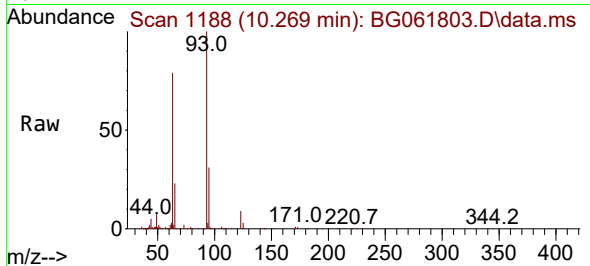

#29
 2,4-Dichlorophenol
 Concen: 22.090 ng/ul
 RT: 10.504 min Scan# 1228
 Delta R.T. -0.005 min
 Lab File: BG061803.D
 Acq: 29 Jun 2024 12:35

Tgt Ion:162 Resp: 125643
 Ion Ratio Lower Upper
 162 100
 164 63.3 51.7 77.5
 98 42.4 34.9 52.3


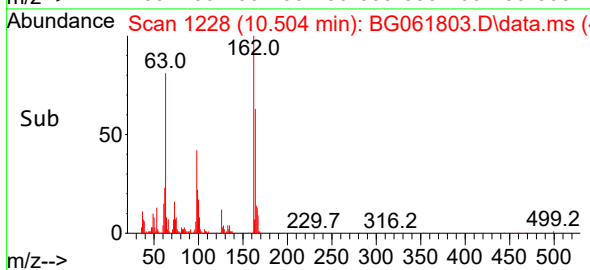
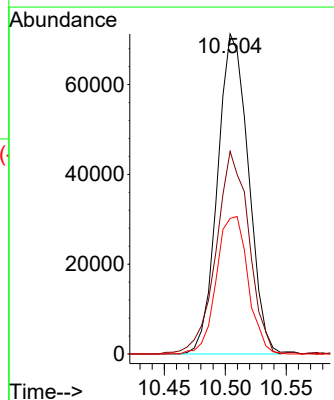
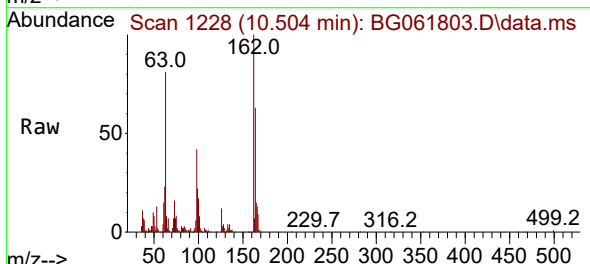




#30
Naphthalene
Concen: 20.356 ng/ul
RT: 10.915 min Scan# 11
Delta R.T. -0.005 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35




Instrument :
BNA_G
ClientSampleId :
SSTD020546


Tgt Ion:128 Resp: 434212
Ion Ratio Lower Upper
128 100
129 10.3 9.0 13.6
127 13.9 10.5 15.7



#32
4-Chloroaniline
Concen: 19.199 ng/ul
RT: 11.021 min Scan# 1316
Delta R.T. -0.005 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35

Tgt Ion:127 Resp: 178963
Ion Ratio Lower Upper
127 100
129 30.7 22.9 34.3









#33
Hexachlorobutadiene
Concen: 23.944 ng/ul
RT: 11.191 min Scan# 11
Delta R.T. -0.005 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35




Instrument :
BNA_G
ClientSampleId :
SSTD020546


Tgt Ion:	225	Resp:	94069
Ion Ratio	Lower	Upper	
225	100		
223	58.0	49.4	74.0
227	64.3	45.6	68.4



#34
Caprolactam
Concen: 14.389 ng/ul
RT: 11.779 min Scan# 1445
Delta R.T. 0.006 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35

Tgt Ion:	113	Resp:	33840
Ion Ratio	Lower	Upper	
113	100		
55	264.8	207.4	311.2
56	189.7	167.2	250.8









#35
4-Chloro-3-methylphenol
Concen: 20.995 ng/ul
RT: 12.137 min Scan# 1506
Delta R.T. 0.006 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35




Instrument :
BNA_G
ClientSampleId :
SSTD020546


Tgt Ion:107 Resp: 166982
Ion Ratio Lower Upper
107 100
144 20.1 19.6 29.4
142 68.7 60.2 90.4

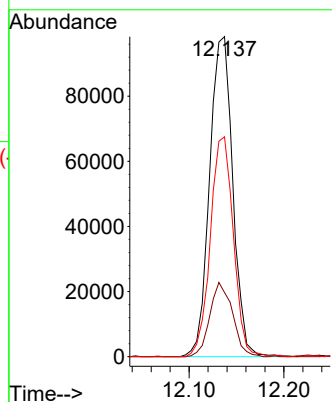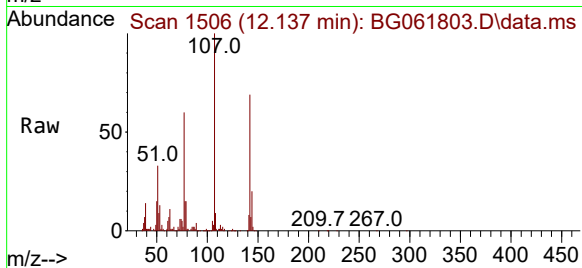

#36
2-Methylnaphthalene
Concen: 19.317 ng/ul
RT: 12.519 min Scan# 1571
Delta R.T. 0.001 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35

Tgt Ion:142 Resp: 290755
Ion Ratio Lower Upper
142 100
141 80.5 68.5 102.7

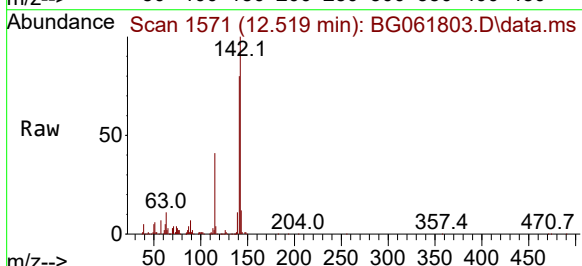



#37

1-Methylnaphthalene

Concen: 19.138 ng/ul

RT: 12.737 min Scan# 1

Delta R.T. 0.001 min

Lab File: BG061803.D

Acq: 29 Jun 2024 12:35

Instrument :

BNA_G

ClientSampleId :

SSTD020546





Tgt Ion:142 Resp: 307360

Ion Ratio Lower Upper

142 100

141 89.4 64.6 97.0

116 4.9 3.0 4.6#

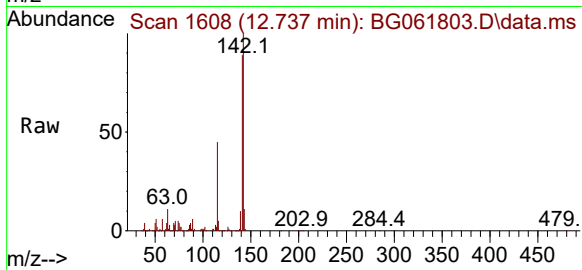

#39

1,2,4,5-Tetrachlorobenzene

Concen: 21.814 ng/ul

RT: 12.878 min Scan# 1632

Delta R.T. -0.005 min

Lab File: BG061803.D

Acq: 29 Jun 2024 12:35

Tgt Ion:216 Resp: 164282




Ion Ratio Lower Upper


216 100

214 78.6 61.4 92.2

179 19.6 17.1 25.7

108 14.9 14.3 21.5



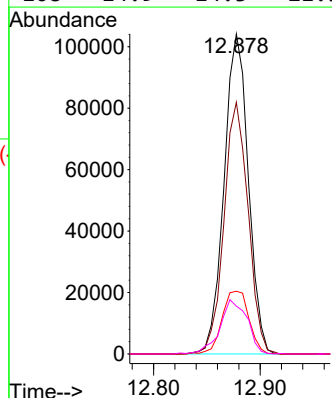
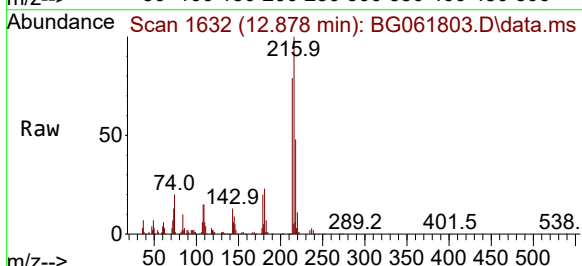




#40
Hexachlorocyclopentadiene
Concen: 12.790 ng/ul
RT: 12.854 min Scan# 1628
Delta R.T. -0.005 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35




Instrument :
BNA_G
ClientSampleId :
SSTD020546


Tgt Ion:237 Resp: 57310
Ion Ratio Lower Upper
237 100
235 63.8 51.0 76.6
272 14.0 9.1 13.7#

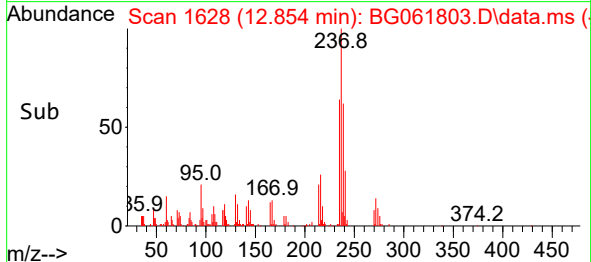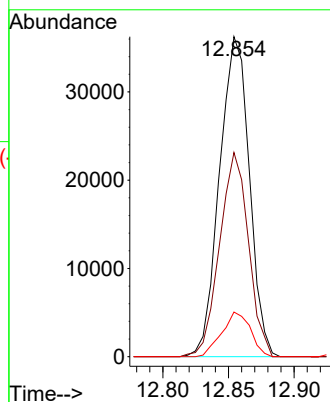

#41
2,4,6-Trichlorophenol
Concen: 23.120 ng/ul
RT: 13.118 min Scan# 1673
Delta R.T. 0.001 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35

Tgt Ion:196 Resp: 112335
Ion Ratio Lower Upper
196 100
198 99.4 73.1 109.7
200 32.2 26.4 39.6



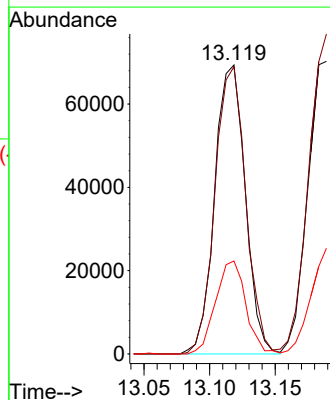





#42
2,4,5-Trichlorophenol
Concen: 18.572 ng/ul
RT: 13.118 min Scan# 1
Delta R.T. -0.070 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35




Instrument :
BNA_G
ClientSampleId :
SSTD020546


Tgt Ion:196 Resp: 98360
Ion Ratio Lower Upper
196 100
198 99.4 72.7 109.1
200 32.2 27.0 40.6

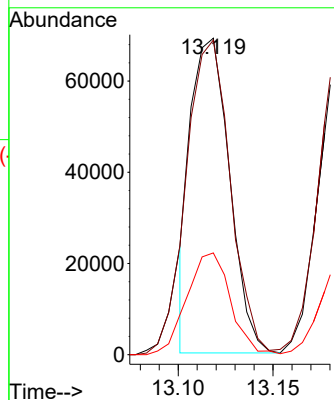

#43
1,1'-Biphenyl
Concen: 21.527 ng/ul
RT: 13.518 min Scan# 1741
Delta R.T. -0.005 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35

Tgt Ion:154 Resp: 414943
Ion Ratio Lower Upper
154 100
153 39.4 31.4 47.0
76 12.7 11.0 16.4

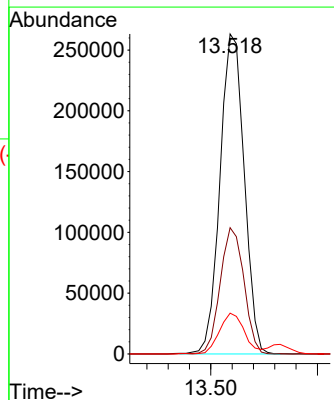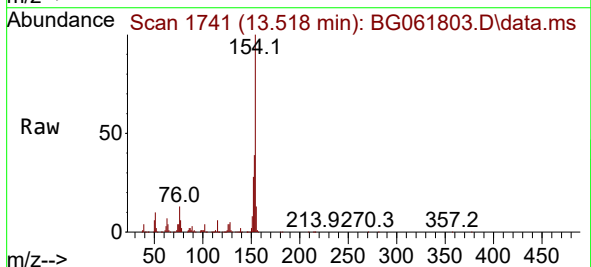



#44

2-Chloronaphthalene

Concen: 21.087 ng/ul

RT: 13.565 min Scan# 1

Delta R.T. 0.001 min

Lab File: BG061803.D

Acq: 29 Jun 2024 12:35

Instrument :

BNA_G

ClientSampleId :

SSTD020546





Tgt Ion:162 Resp: 312224

Ion Ratio Lower Upper

162 100

164 32.4 25.1 37.7

127 42.5 33.7 50.5

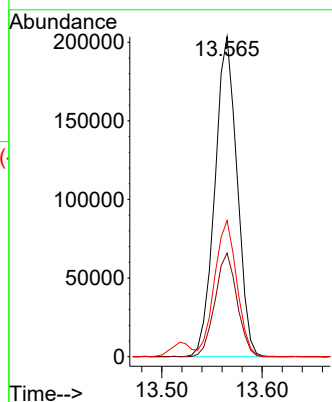

#45

2-Nitroaniline

Concen: 26.348 ng/ul

RT: 13.765 min Scan# 1783

Delta R.T. 0.001 min

Lab File: BG061803.D

Acq: 29 Jun 2024 12:35




Tgt Ion: 65 Resp: 133551


Ion Ratio Lower Upper

65 100

92 53.2 51.4 77.0

138 76.8 63.0 94.6









#47
Dimethylphthalate
Concen: 20.391 ng/ul
RT: 14.135 min Scan# 1846
Delta R.T. -0.005 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35




Instrument :
BNA_G
ClientSampleId :
SSTD020546


Tgt Ion:163 Resp: 414641
Ion Ratio Lower Upper
163 100
194 3.6 2.5 3.7
164 10.0 7.6 11.4



#48
2,6-Dinitrotoluene
Concen: 26.317 ng/ul
RT: 14.258 min Scan# 1867
Delta R.T. 0.001 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35

Tgt Ion:165 Resp: 88804
Ion Ratio Lower Upper
165 100
89 67.7 55.9 83.9
121 20.8 23.4 35.2#





#50

Acenaphthylene

Concen: 20.291 ng/ul

RT: 14.405 min Scan# 1892

Delta R.T. -0.005 min

Lab File: BG061803.D

Acq: 29 Jun 2024 12:35

Instrument :

BNA_G

ClientSampleId :

SSTD020546





Tgt Ion:152 Resp: 508313

Ion Ratio Lower Upper

152 100

151 20.4 15.3 22.9

153 13.0 11.0 16.4



#51

3-Nitroaniline

Concen: 25.570 ng/ul

RT: 14.587 min Scan# 1923

Delta R.T. 0.001 min

Lab File: BG061803.D

Acq: 29 Jun 2024 12:35




Tgt Ion:138 Resp: 88359


Ion Ratio Lower Upper

138 100

108 13.1 14.3 21.5#

92 142.4 115.0 172.4









#52
Acenaphthene
Concen: 20.783 ng/ul
RT: 14.746 min Scan# 1950
Delta R.T. -0.005 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35




Instrument :
BNA_G
ClientSampleId :
SSTD020546


Tgt Ion:153 Resp: 360556
Ion Ratio Lower Upper
153 100
152 42.5 40.0 60.0
154 81.8 74.1 111.1

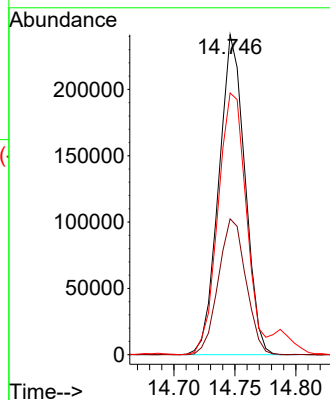

#53
2,4-Dinitrophenol
Concen: 20.673 ng/ul
RT: 14.787 min Scan# 1957
Delta R.T. 0.001 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35

Tgt Ion:184 Resp: 35449
Ion Ratio Lower Upper
184 100
63 87.3 74.2 111.4
154 75.2 80.4 120.6#



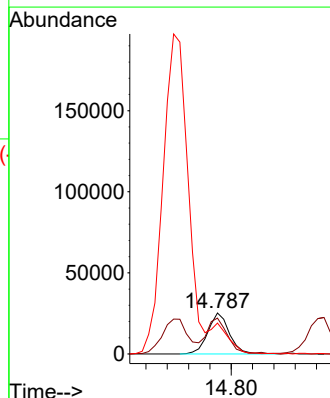





#55
4-Nitrophenol
Concen: 21.769 ng/ul
RT: 14.887 min Scan# 1974
Delta R.T. 0.006 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35




Instrument :
BNA_G
ClientSampleId :
SSTD020546


Tgt Ion:109 Resp: 79059
Ion Ratio Lower Upper
109 100
139 94.6 77.1 115.7
65 129.9 110.9 166.3

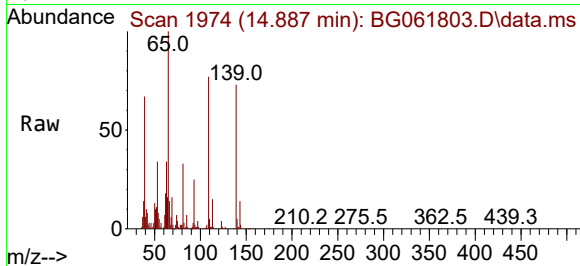

#56
Dibenzofuran
Concen: 20.655 ng/ul
RT: 15.081 min Scan# 2007
Delta R.T. -0.005 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35

Tgt Ion:168 Resp: 501434
Ion Ratio Lower Upper
168 100
139 38.5 27.0 40.4

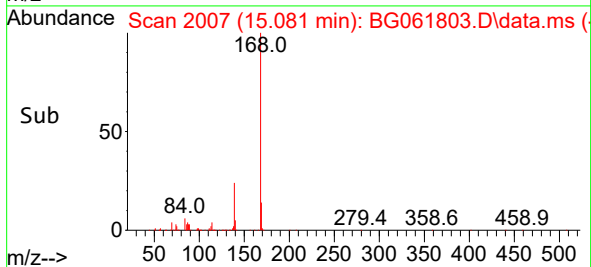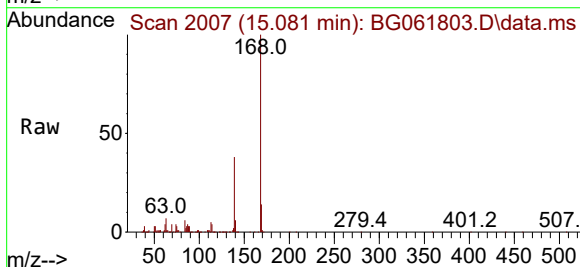



#57

2,4-Dinitrotoluene

Concen: 26.742 ng/ul

RT: 15.040 min Scan# 2000

Delta R.T. 0.001 min

Lab File: BG061803.D

Acq: 29 Jun 2024 12:35

Instrument :

BNA_G

ClientSampleId :

SSTD020546





Tgt Ion:165 Resp: 133945

Ion Ratio Lower Upper

165 100

63 58.1 49.4 74.0

182 2.1 1.6 2.4

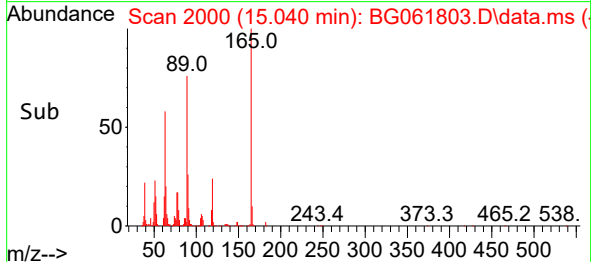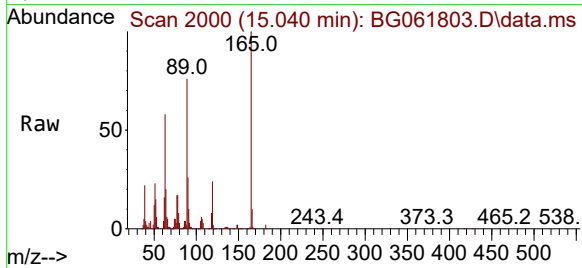

#58

2,3,4,6-Tetrachlorophenol

Concen: 20.852 ng/ul

RT: 15.304 min Scan# 2045

Delta R.T. 0.001 min

Lab File: BG061803.D

Acq: 29 Jun 2024 12:35

Tgt Ion:232 Resp: 108281




Ion Ratio Lower Upper


232 100

131 43.1 33.1 49.7

130 2.0 2.6 3.8#

166 32.1 23.4 35.0


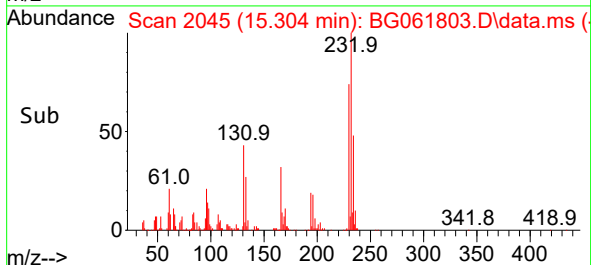
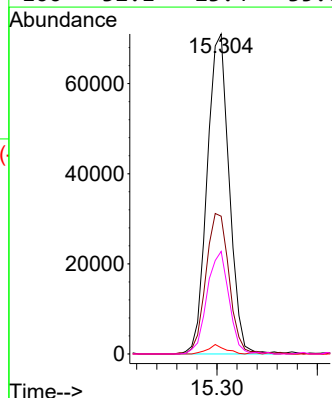
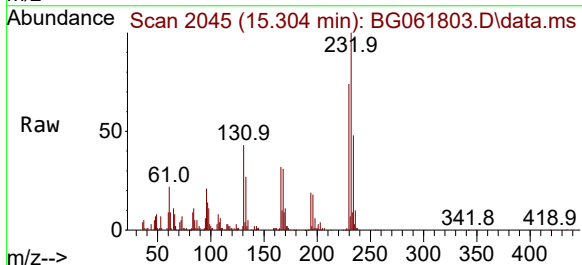




#59
Diethylphthalate
Concen: 20.834 ng/ul
RT: 15.498 min Scan# 2078
Delta R.T. 0.001 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35




Instrument :
BNA_G
ClientSampleId :
SSTD020546


Tgt Ion:149 Resp: 436323
Ion Ratio Lower Upper
149 100
177 22.9 19.6 29.4
150 12.2 9.2 13.8



#61
Fluorene
Concen: 20.893 ng/ul
RT: 15.727 min Scan# 2117
Delta R.T. -0.005 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35

Tgt Ion:166 Resp: 419777
Ion Ratio Lower Upper
166 100
165 95.5 84.9 127.3
167 14.1 10.9 16.3




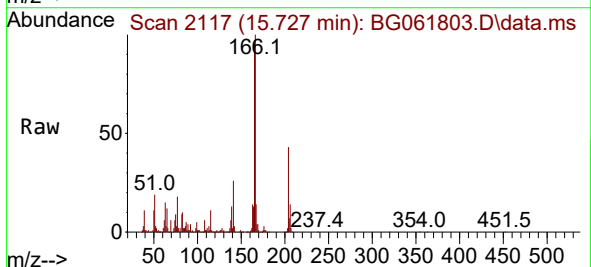




#62
4-Chlorophenyl-phenylether
Concen: 20.998 ng/ul
RT: 15.721 min Scan# 2116
Delta R.T. -0.005 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35




Instrument :
BNA_G
ClientSampleId :
SSTD020546


Tgt Ion:204 Resp: 209438
Ion Ratio Lower Upper
204 100
206 32.2 26.4 39.6
141 59.0 51.1 76.7



#63
4-Nitroaniline
Concen: 25.461 ng/ul
RT: 15.745 min Scan# 2120
Delta R.T. 0.001 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35

Tgt Ion:138 Resp: 93208
Ion Ratio Lower Upper
138 100
92 61.1 54.8 82.2
108 107.8 84.2 126.2


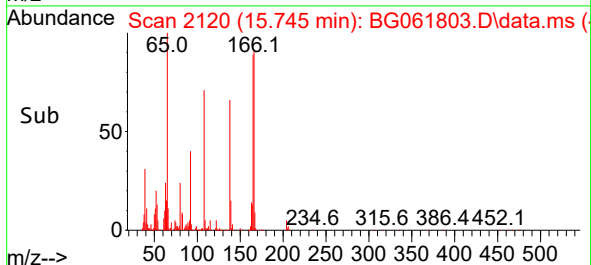
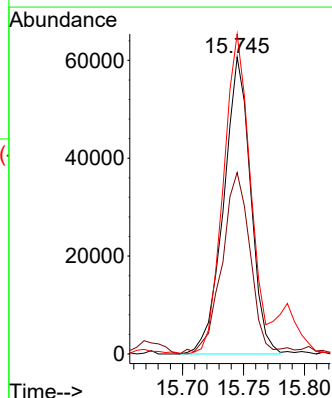
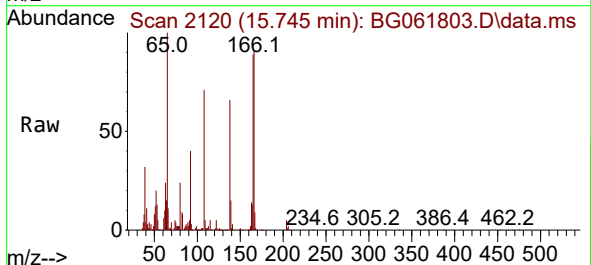




#66
 4,6-Dinitro-2-methylphenol
 Concen: 21.570 ng/ul
 RT: 15.798 min Scan# 2129
 Delta R.T. 0.001 min
 Lab File: BG061803.D
 Acq: 29 Jun 2024 12:35




Instrument :
 BNA_G
 ClientSampleId :
 SSTD020546


Tgt Ion:198 Resp: 64816
 Ion Ratio Lower Upper
 198 100
 182 4.3 3.6 5.4
 77 30.0 19.5 29.3#

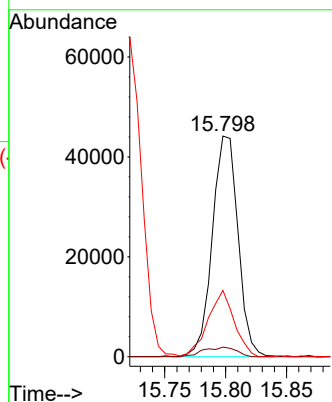

#67
 N-Nitrosodiphenylamine
 Concen: 21.957 ng/ul
 RT: 15.933 min Scan# 2152
 Delta R.T. -0.005 min
 Lab File: BG061803.D
 Acq: 29 Jun 2024 12:35

Tgt Ion:169 Resp: 352260
 Ion Ratio Lower Upper
 169 100
 168 69.8 54.6 81.8
 167 36.1 27.8 41.6









#68
4-Bromophenyl-phenylether
Concen: 22.726 ng/ul
RT: 16.614 min Scan# 21
Delta R.T. -0.005 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35




Instrument :
BNA_G
ClientSampleId :
SSTD020546


Tgt Ion:	248	Resp:	145169
Ion Ratio	Lower	Upper	
248	100		
250	98.5	82.1	123.1
141	67.0	57.6	86.4

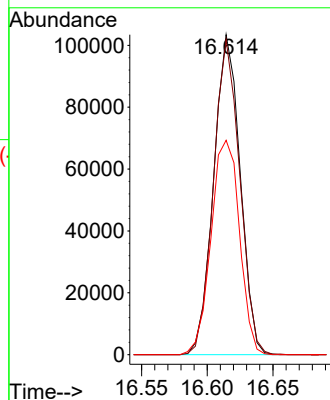

#69
Hexachlorobenzene
Concen: 21.961 ng/ul
RT: 16.726 min Scan# 2287
Delta R.T. 0.001 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35

Tgt Ion:	284	Resp:	170237
Ion Ratio	Lower	Upper	
284	100		
142	28.4	25.2	37.8
249	29.0	26.9	40.3

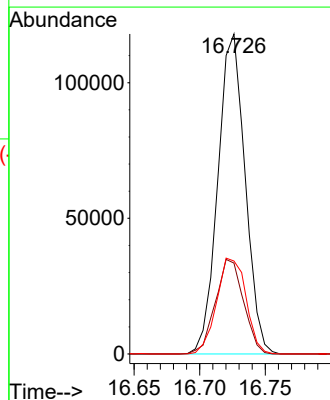



#70

Atrazine

Concen: 21.426 ng/ul

RT: 16.879 min Scan# 21

Delta R.T. -0.005 min

Lab File: BG061803.D

Acq: 29 Jun 2024 12:35

Instrument :

BNA_G

ClientSampleId :

SSTD020546





Tgt Ion:200 Resp: 137299

Ion Ratio Lower Upper

200 100

173 24.3 18.2 27.2

215 43.4 36.6 54.8

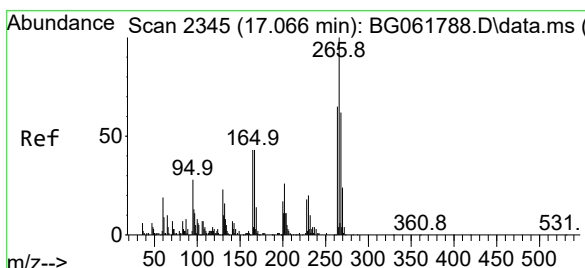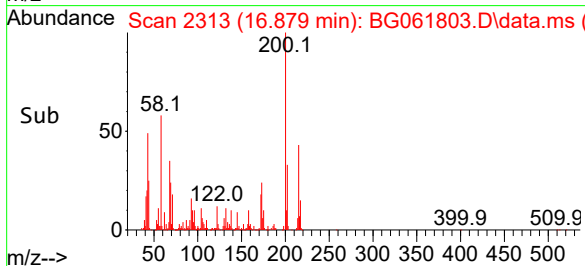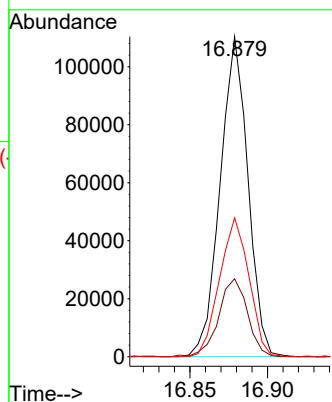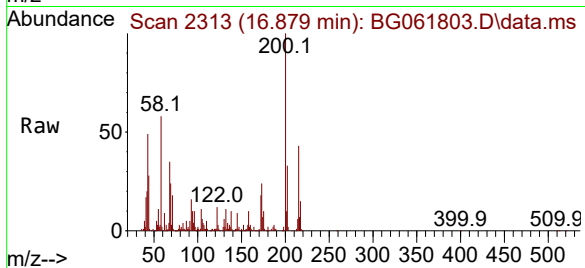

#71

Pentachlorophenol

Concen: 19.926 ng/ul

RT: 17.067 min Scan# 2345

Delta R.T. -0.005 min

Lab File: BG061803.D

Acq: 29 Jun 2024 12:35




Tgt Ion:266 Resp: 94093


Ion Ratio Lower Upper

266 100

264 64.4 52.5 78.7

268 62.1 47.5 71.3


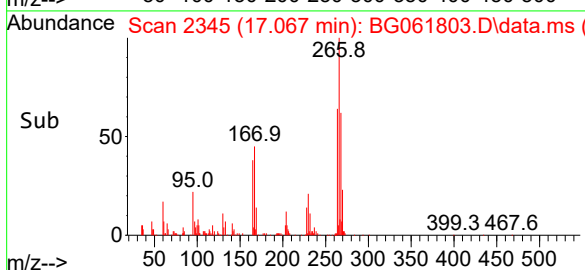

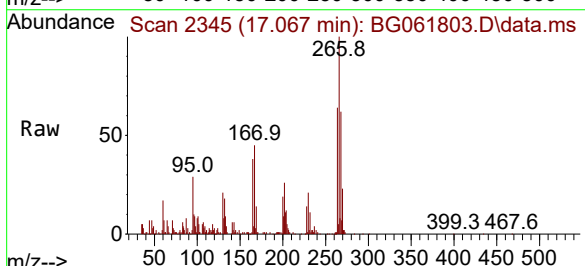




#72
Phenanthrene
Concen: 20.639 ng/ul
RT: 17.472 min Scan# 2414
Delta R.T. 0.001 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35




Instrument :
BNA_G
ClientSampleId :
SSTD020546


Tgt Ion:178 Resp: 673618
Ion Ratio Lower Upper
178 100
179 14.9 12.0 18.0
176 19.8 16.2 24.2



#74
Anthracene
Concen: 21.120 ng/ul
RT: 17.560 min Scan# 2429
Delta R.T. -0.005 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35

Tgt Ion:178 Resp: 704907
Ion Ratio Lower Upper
178 100
179 14.8 11.4 17.2
176 18.3 14.7 22.1





#75

1,2,3,4-Tetrachlorobenzene

Concen: 23.954 ng/ul

RT: 13.483 min Scan# 1

Delta R.T. 0.001 min

Lab File: BG061803.D

Acq: 29 Jun 2024 12:35

Instrument :

BNA_G

ClientSampleId :

SSTD020546





Tgt Ion:216 Resp: 165568

Ion Ratio Lower Upper

216 100

214 75.5 61.9 92.9

218 45.8 39.6 59.4

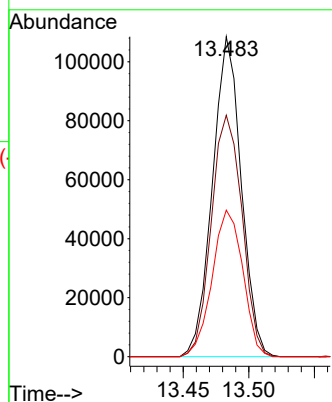

#76

Pentachlorobenzene

Concen: 23.020 ng/ul

RT: 14.999 min Scan# 1993

Delta R.T. 0.001 min

Lab File: BG061803.D

Acq: 29 Jun 2024 12:35




Tgt Ion:250 Resp: 191075


Ion Ratio Lower Upper

250 100

248 63.7 45.7 68.5

252 61.1 48.3 72.5





#77

Carbazole

Concen: 21.212 ng/ul

RT: 17.825 min Scan# 2474

Delta R.T. -0.005 min

Lab File: BG061803.D

Acq: 29 Jun 2024 12:35

Instrument :

BNA_G

ClientSampleId :

SSTD020546





Tgt Ion:167 Resp: 601136

Ion Ratio Lower Upper

167 100

166 22.4 17.5 26.3

139 12.9 9.4 14.2

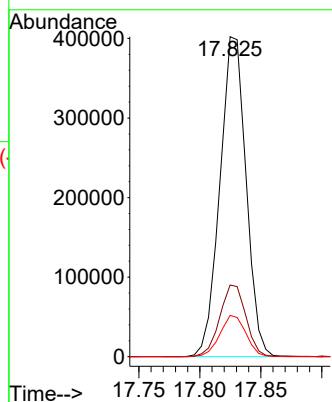

#78

Di-n-butylphthalate

Concen: 22.493 ng/ul

RT: 18.383 min Scan# 2569

Delta R.T. -0.011 min

Lab File: BG061803.D

Acq: 29 Jun 2024 12:35




Tgt Ion:149 Resp: 762367


Ion Ratio Lower Upper

149 100

150 9.4 6.7 10.1

104 5.9 4.6 6.8





#80

Fluoranthene

Concen: 23.224 ng/ul

RT: 19.476 min Scan# 2755

Delta R.T. 0.001 min

Lab File: BG061803.D

Acq: 29 Jun 2024 12:35

Instrument :

BNA_G

ClientSampleId :

SSTD020546





Tgt Ion:202 Resp: 772828

Ion Ratio Lower Upper

202 100

101 8.7 7.8 11.6

100 7.9 7.7 11.5

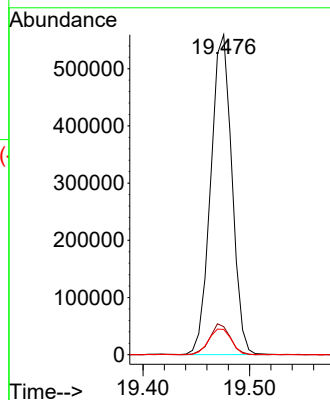

#82

Pyrene

Concen: 22.228 ng/ul

RT: 19.834 min Scan# 2816

Delta R.T. -0.005 min

Lab File: BG061803.D

Acq: 29 Jun 2024 12:35




Tgt Ion:202 Resp: 786513


Ion Ratio Lower Upper

202 100

101 11.4 10.1 15.1

100 11.6 9.9 14.9

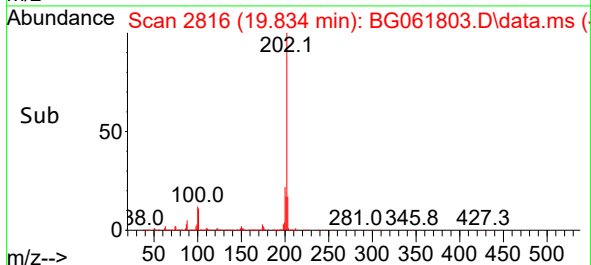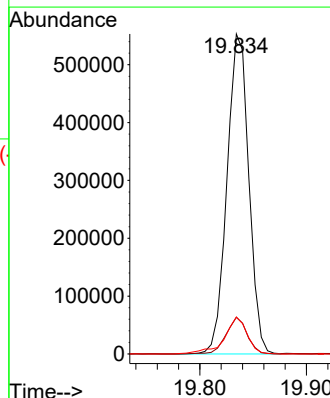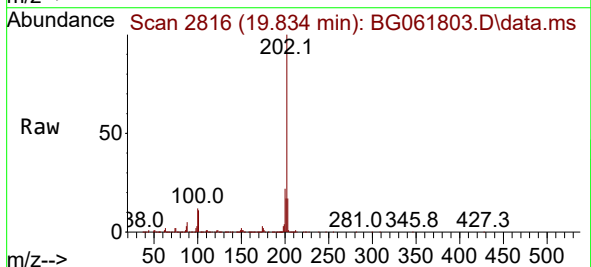



#83

Butylbenzylphthalate

Concen: 24.834 ng/ul

RT: 20.721 min Scan# 2967

Delta R.T. -0.005 min

Lab File: BG061803.D

Acq: 29 Jun 2024 12:35

Instrument :

BNA_G

ClientSampleId :

SSTD020546





Tgt Ion:149 Resp: 319938

Ion Ratio Lower Upper

149 100

91 80.7 68.1 102.1

206 22.1 17.9 26.9

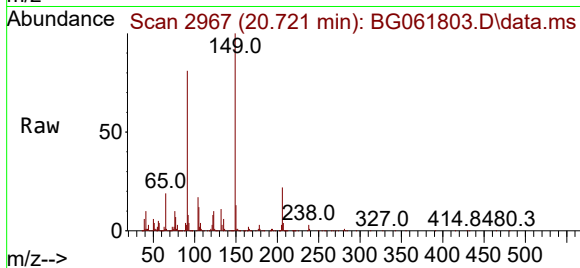

#84

3,3'-Dichlorobenzidine

Concen: 23.218 ng/ul

RT: 21.585 min Scan# 3114

Delta R.T. -0.005 min

Lab File: BG061803.D

Acq: 29 Jun 2024 12:35




Tgt Ion:252 Resp: 252071


Ion Ratio Lower Upper

252 100

254 64.8 53.9 80.9

126 8.0 8.1 12.1#



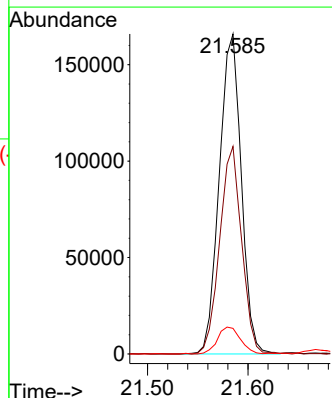
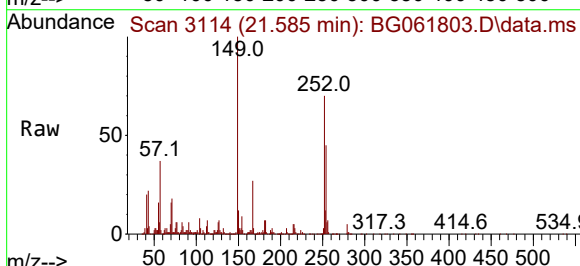




#85
Benzo(a)anthracene
Concen: 21.241 ng/ul
RT: 21.667 min Scan# 3128
Delta R.T. -0.005 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35




Instrument :
BNA_G
ClientSampleId :
SSTD020546


Tgt Ion:228 Resp: 765555
Ion Ratio Lower Upper
228 100
229 18.9 15.8 23.8
226 26.8 21.4 32.2



#86
Bis(2-ethylhexyl)phthalate
Concen: 24.205 ng/ul
RT: 21.579 min Scan# 3113
Delta R.T. -0.011 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35

Tgt Ion:149 Resp: 458374
Ion Ratio Lower Upper
149 100
167 26.8 20.5 30.7
279 4.6 2.9 4.3#







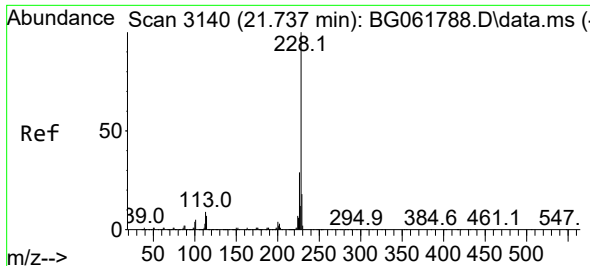

#87
Chrysene
Concen: 20.872 ng/ul
RT: 21.732 min Scan# 3140
Delta R.T. -0.005 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35




Instrument :
BNA_G
ClientSampleId :
SSTD020546


Tgt Ion:228 Resp: 711826
Ion Ratio Lower Upper
228 100
226 30.4 24.2 36.2
229 19.1 16.5 24.7

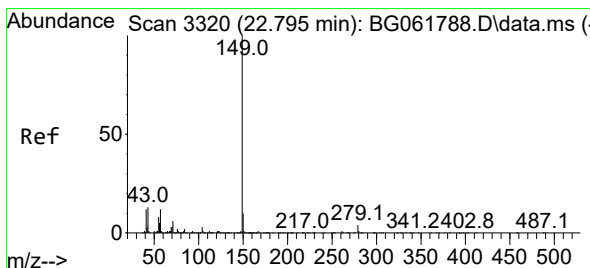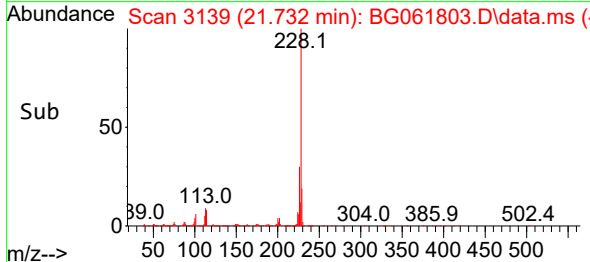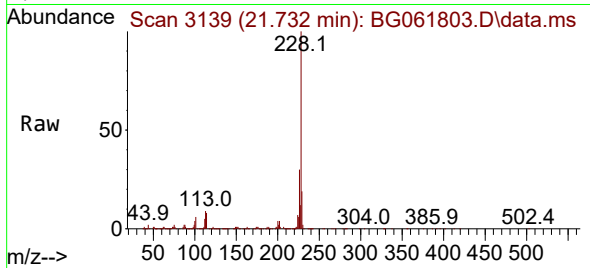

#89
Di-n-octyl phthalate
Concen: 24.953 ng/ul
RT: 22.795 min Scan# 3320
Delta R.T. -0.011 min
Lab File: BG061803.D
Acq: 29 Jun 2024 12:35

Tgt Ion:149 Resp: 787605

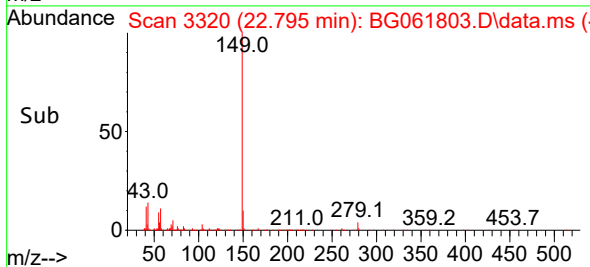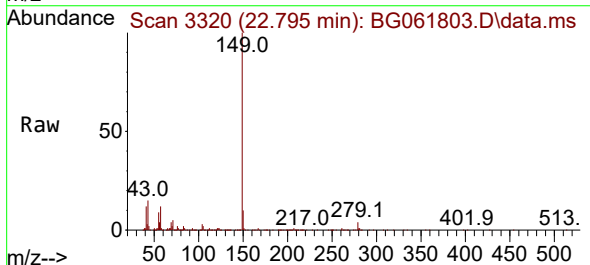



#90

Benzo(b)fluoranthene

Concen: 21.011 ng/ul

RT: 23.882 min Scan# 3505

Delta R.T. -0.005 min

Lab File: BG061803.D

Acq: 29 Jun 2024 12:35

Instrument :

BNA_G

ClientSampleId :

SSTD020546





Tgt Ion:252 Resp: 755847

Ion Ratio Lower Upper

252 100

253 20.6 18.6 27.8

125 8.4 7.0 10.6

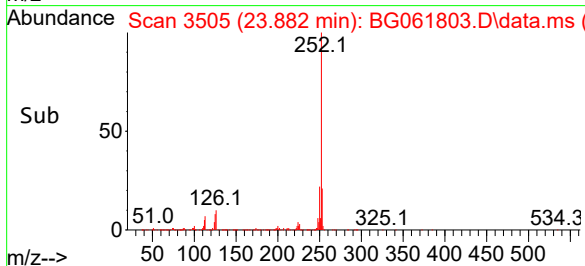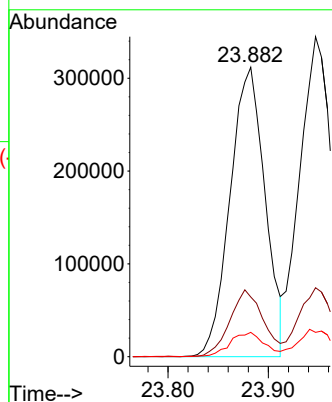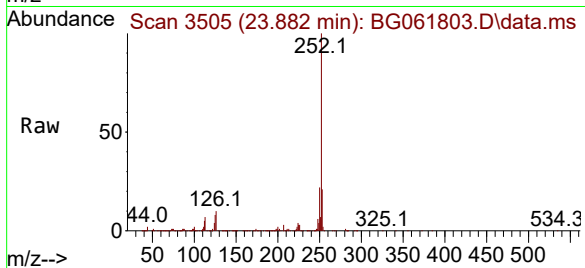

#91

Benzo(k)fluoranthene

Concen: 21.233 ng/ul

RT: 23.947 min Scan# 3516

Delta R.T. -0.011 min

Lab File: BG061803.D

Acq: 29 Jun 2024 12:35




Tgt Ion:252 Resp: 785542


Ion Ratio Lower Upper

252 100

253 21.5 17.8 26.6

125 7.6 6.2 9.2

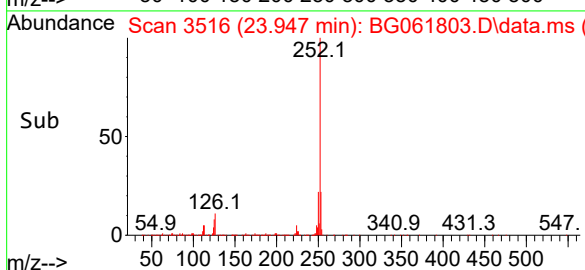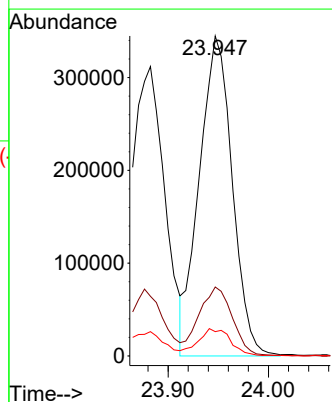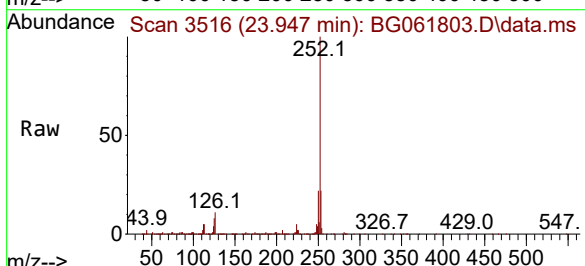



#93

Benzo(a)pyrene

Concen: 21.079 ng/ul

RT: 24.752 min Scan# 3

Delta R.T. -0.011 min

Lab File: BG061803.D

Acq: 29 Jun 2024 12:35

Instrument :

BNA_G

ClientSampleId :

SSTD020546





Tgt Ion:252 Resp: 730019

Ion Ratio Lower Upper

252 100

253 21.0 16.8 25.2

125 9.2 6.5 9.7

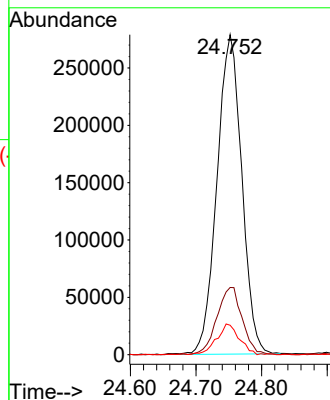

#94

Indeno(1,2,3-cd)pyrene

Concen: 21.692 ng/ul

RT: 28.559 min Scan# 4301

Delta R.T. -0.005 min

Lab File: BG061803.D

Acq: 29 Jun 2024 12:35




Tgt Ion:276 Resp: 936152


Ion Ratio Lower Upper

276 100

138 14.1 12.2 18.4

277 23.2 19.7 29.5

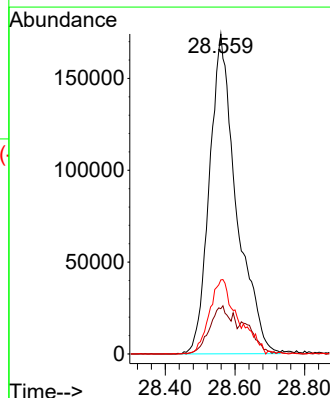



#95

Dibenzo(a,h)anthracene

Concen: 21.506 ng/ul

RT: 28.636 min Scan# 41

Delta R.T. 0.001 min

Lab File: BG061803.D

Acq: 29 Jun 2024 12:35

Instrument :

BNA_G

ClientSampleId :

SSTD020546





Tgt Ion:278 Resp: 771780

Ion Ratio Lower Upper

278 100

139 10.9 9.1 13.7

279 24.9 18.6 28.0

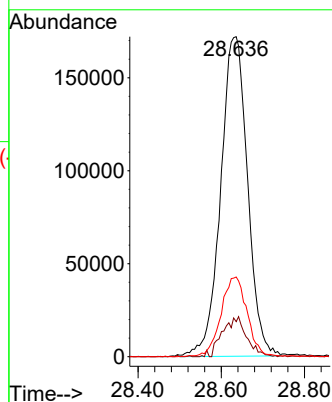

#96

Benzo(g,h,i)perylene

Concen: 21.304 ng/ul

RT: 29.711 min Scan# 4497

Delta R.T. 0.001 min

Lab File: BG061803.D

Acq: 29 Jun 2024 12:35

Tgt Ion:276 Resp: 741146

Ion Ratio Lower Upper

276 100

138 15.4 12.2 18.4

277 22.2 18.6 27.8

