

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062824\
 Data File : BG061783.D
 Acq On : 28 Jun 2024 22:26
 Operator : MA/JU
 Sample : P2898-19
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E1G82

Quant Time: Jun 29 03:14:46 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 27 12:23:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.055	152	67504	20.000	ng/ul	0.00
20) Naphthalene-d8	10.870	136	320284	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.683	164	209235	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.427	188	458806	20.000	ng/ul	0.00
79) Chrysene-d12	21.686	240	348139	20.000	ng/ul	0.00
88) Perylene-d12	24.906	264	402739	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.455	96	10833	5.797	ng/uL	0.00
4) Pyridine-d5	3.878	84	58130	10.289	ng/ul	0.00
7) Phenol-d5	7.203	99	66590	9.087	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.380	67	173434	37.965	ng/ul	0.00
11) 2-Chlorophenol-d4	7.585	132	155535	30.929	ng/ul	0.00
15) 4-Methylphenol-d8	8.755	113	115469	20.382	ng/ul	0.00
21) Nitrobenzene-d5	9.219	128	97475	44.822	ng/ul	0.00
24) 2-Nitrophenol-d4	9.941	143	109586	49.754	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.482	165	190844	36.592	ng/ul	0.00
31) 4-Chloroaniline-d4	10.999	131	234632	29.715	ng/ul	0.00
46) Dimethylphthalate-d6	14.089	166	630387	39.151	ng/ul	0.00
49) Acenaphthylene-d8	14.377	160	715830	40.567	ng/ul	0.00
54) 4-Nitrophenol-d4	14.865	143	24306	8.790	ng/ul	0.00
60) Fluorene-d10	15.676	176	556310	39.466	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.782	200	52538	26.779	ng/ul	0.00
73) Anthracene-d10	17.527	188	877171	41.884	ng/ul	0.00
81) Pyrene-d10	19.806	212	914867	47.046	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.689	264	842944	43.823	ng/ul	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.581	149	14522	1.131	ng/ul#	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062824\
Data File : BG061783.D
Acq On : 28 Jun 2024 22:26
Operator : MA/JU
Sample : P2898-19
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E1G82

Quant Time: Jun 29 03:14:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 27 12:23:53 2024
Response via : Initial Calibration

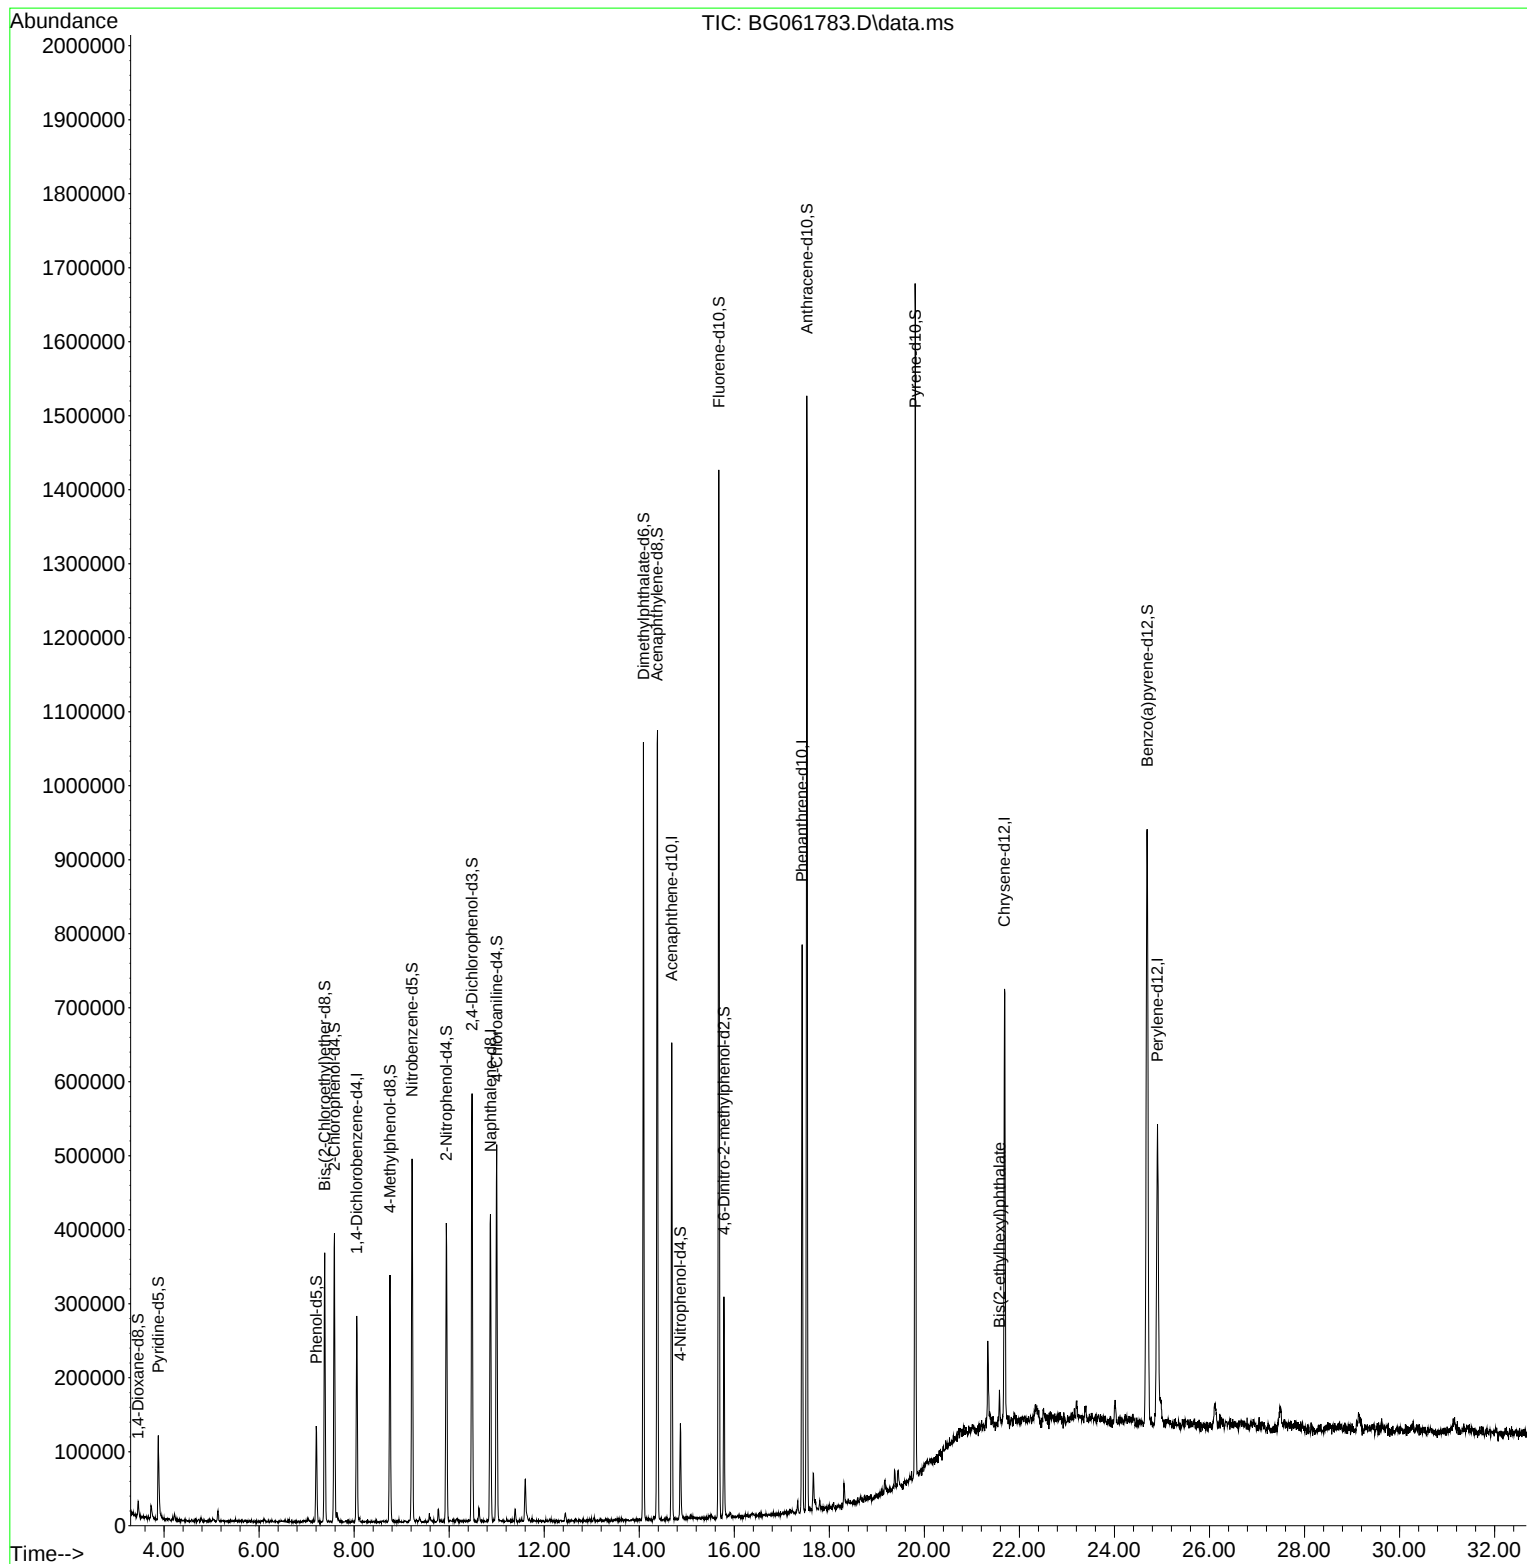

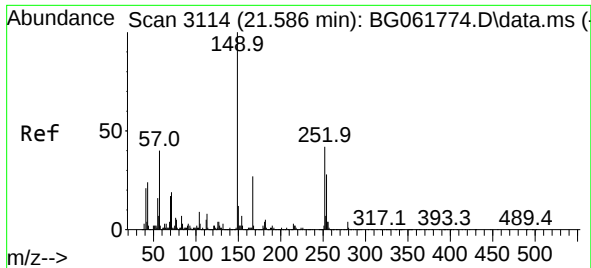

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.131 ng/ul
 RT: 21.581 min Scan# 31
 Delta R.T. -0.010 min
 Lab File: BG061783.D
 Acq: 28 Jun 2024 22:26

Instrument :
 BNA_G
 ClientSampleId :
 E1G82

Tgt Ion:149 Resp: 14522
 Ion Ratio Lower Upper
 149 100
 167 24.5 20.5 30.7
 279 9.9 2.9 4.3#

