

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062824\
 Data File : BG061789.D
 Acq On : 29 Jun 2024 3:12
 Operator : MA/JU
 Sample : PB161592BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK592

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG061789.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.458	25	29	33	rBV5	20059	33707	1.66%	0.135%
2	3.546	42	44	46	rVB3	4967	3381	0.17%	0.014%
3	3.875	96	100	116	rBV	318502	616928	30.45%	2.479%
4	4.099	135	138	139	rVB3	5506	4827	0.24%	0.019%
5	4.216	151	158	163	rVB4	6436	11796	0.58%	0.047%
6	4.580	217	220	222	rBV3	3903	4631	0.23%	0.019%
7	5.321	344	346	348	rBV2	3346	3601	0.18%	0.014%
8	5.609	393	395	396	rBV	4075	3402	0.17%	0.014%
9	5.920	446	448	452	rVB4	3117	3314	0.16%	0.013%
10	6.372	519	525	526	rBV3	4342	7569	0.37%	0.030%
11	6.496	544	546	549	rBV4	3803	5086	0.25%	0.020%
12	6.543	552	554	556	rBV2	3168	3114	0.15%	0.013%
13	6.584	556	561	562	rVB4	3034	4434	0.22%	0.018%
14	6.602	562	564	566	rBV2	3496	2938	0.15%	0.012%
15	6.701	579	581	584	rBV3	3028	3177	0.16%	0.013%
16	7.201	658	666	676	rVB	416794	732294	36.14%	2.943%
17	7.377	690	696	706	rVB	279910	474582	23.42%	1.907%
18	7.489	710	715	718	rBV4	3147	6705	0.33%	0.027%
19	7.524	718	721	724	rVB3	3616	3838	0.19%	0.015%
20	7.583	724	731	741	rBV	392591	662915	32.72%	2.664%
21	7.871	778	780	783	rVB2	4960	4698	0.23%	0.019%
22	7.912	783	787	790	rBV4	3222	6593	0.33%	0.026%
23	8.059	803	812	820	rBV2	306317	536338	26.47%	2.155%
24	8.217	835	839	842	rVB4	2485	3038	0.15%	0.012%
25	8.300	850	853	854	rBV2	3148	2897	0.14%	0.012%
26	8.435	874	876	880	rVB4	3185	3974	0.20%	0.016%
27	8.464	880	881	883	rBV	4757	3118	0.15%	0.013%
28	8.699	916	921	923	rVB3	3677	3787	0.19%	0.015%
29	8.752	923	930	938	rBV2	505784	872937	43.08%	3.508%
30	8.881	949	952	954	rBV3	3243	4282	0.21%	0.017%
31	9.216	1002	1009	1017	rBV	380795	682445	33.68%	2.742%
32	9.316	1021	1026	1029	rBV4	4285	6478	0.32%	0.026%
33	9.939	1125	1132	1140	rBV	332281	601346	29.68%	2.416%
34	10.039	1146	1149	1152	rVB4	3076	3751	0.19%	0.015%
35	10.086	1155	1157	1159	rBV2	3565	3281	0.16%	0.013%
36	10.286	1189	1191	1195	rVB3	3792	3714	0.18%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062824\
 Data File : BG061789.D
 Acq On : 29 Jun 2024 3:12
 Operator : MA/JU
 Sample : PB161592BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK592

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

37	10.344	1198	1201	1204	rVB4	2882	3817	0.19%	0.015%
38	10.421	1210	1214	1216	rBV2	3549	3623	0.18%	0.015%
39	10.479	1216	1224	1232	rVV	519481	900458	44.44%	3.618%
40	10.568	1236	1239	1242	rVB4	4236	5322	0.26%	0.021%

41	10.679	1254	1258	1263	rVB4	4597	6793	0.34%	0.027%
42	10.738	1267	1268	1273	rBV	2887	4191	0.21%	0.017%
43	10.867	1282	1290	1299	rBV	485936	841347	41.52%	3.381%
44	10.996	1303	1312	1322	rBV	521916	928079	45.80%	3.729%
45	11.308	1362	1365	1366	rBV	3607	3328	0.16%	0.013%

46	11.390	1376	1379	1382	rBV3	3833	4947	0.24%	0.020%
47	11.555	1406	1407	1411	rVB2	3066	3484	0.17%	0.014%
48	11.613	1414	1417	1419	rBV2	3300	3999	0.20%	0.016%
49	11.731	1436	1437	1441	rBV3	2770	3277	0.16%	0.013%
50	12.048	1487	1491	1494	rBV3	2452	4299	0.21%	0.017%

51	12.330	1537	1539	1541	rBV2	3202	3280	0.16%	0.013%
52	12.371	1544	1546	1549	rVB4	2824	3382	0.17%	0.014%
53	12.436	1555	1557	1558	rBV	6832	4923	0.24%	0.020%
54	12.959	1642	1646	1648	rBV2	3882	5516	0.27%	0.022%
55	12.994	1651	1652	1655	rVB3	4190	3336	0.16%	0.013%

56	13.029	1655	1658	1660	rBV2	3862	3947	0.19%	0.016%
57	13.206	1685	1688	1691	rVB4	2864	3380	0.17%	0.014%
58	13.817	1788	1792	1793	rBV2	3422	3302	0.16%	0.013%
59	13.858	1798	1799	1805	rVV3	3461	3501	0.17%	0.014%
60	13.999	1820	1823	1828	rBV4	3705	6210	0.31%	0.025%

61	14.087	1831	1838	1847	rVB	881210	1246435	61.52%	5.009%
62	14.152	1847	1849	1854	rBV4	3886	4246	0.21%	0.017%
63	14.234	1861	1863	1865	rBV2	3574	3467	0.17%	0.014%
64	14.316	1875	1877	1878	rBV2	3953	2920	0.14%	0.012%
65	14.381	1880	1888	1895	rVV	937221	1490791	73.58%	5.991%

66	14.510	1908	1910	1911	rBV2	4388	3110	0.15%	0.012%
67	14.680	1931	1939	1947	rVB	728010	1131696	55.85%	4.548%
68	14.863	1964	1970	1977	rBV	433073	691863	34.15%	2.780%
69	15.009	1991	1995	1996	rBV4	3612	3391	0.17%	0.014%
70	15.092	2007	2009	2015	rVB5	4426	7653	0.38%	0.031%

71	15.233	2032	2033	2037	rVB2	4320	3331	0.16%	0.013%
72	15.309	2045	2046	2049	rBV3	3291	2898	0.14%	0.012%
73	15.474	2072	2074	2077	rBV3	3882	4779	0.24%	0.019%
74	15.673	2101	2108	2115	rBV	1189444	1805653	89.12%	7.256%
75	15.779	2120	2126	2133	rBV2	298463	433079	21.37%	1.740%

76	15.908	2146	2148	2154	rVB4	6232	10043	0.50%	0.040%
----	--------	------	------	------	------	------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062824\
 Data File : BG061789.D
 Acq On : 29 Jun 2024 3:12
 Operator : MA/JU
 Sample : PB161592BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK592

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

77	16.008	2163	2165	2166	rBV	4149	2900	0.14%	0.012%
78	16.055	2170	2173	2175	rBV2	2702	2963	0.15%	0.012%
79	16.090	2178	2179	2183	rBV2	3488	3731	0.18%	0.015%
80	16.226	2201	2202	2205	rBV3	3960	4182	0.21%	0.017%
81	16.419	2233	2235	2237	rBV2	4975	3552	0.18%	0.014%
82	16.455	2237	2241	2244	rVV4	5559	7813	0.39%	0.031%
83	17.007	2333	2335	2338	rBV3	4398	5157	0.25%	0.021%
84	17.101	2349	2351	2354	rVB2	3971	3701	0.18%	0.015%
85	17.166	2361	2362	2365	rVB3	5312	3299	0.16%	0.013%
86	17.195	2365	2367	2369	rBV3	3037	3287	0.16%	0.013%
87	17.424	2400	2406	2415	rVB	911316	1352939	66.77%	5.437%
88	17.524	2417	2423	2430	rVB	1319942	1953972	96.44%	7.852%
89	17.659	2441	2446	2451	rBV6	21957	36820	1.82%	0.148%
90	18.029	2508	2509	2513	rVB3	4115	3422	0.17%	0.014%
91	18.082	2516	2518	2520	rVB2	5105	3106	0.15%	0.012%
92	18.535	2593	2595	2597	rBV3	4028	3542	0.17%	0.014%
93	18.975	2668	2670	2671	rBV2	4319	3623	0.18%	0.015%
94	19.375	2733	2738	2744	rBV7	19261	30663	1.51%	0.123%
95	19.445	2746	2750	2754	rVV2	19889	25685	1.27%	0.103%
96	19.528	2762	2764	2765	rBV2	7139	5165	0.25%	0.021%
97	19.804	2805	2811	2818	rBV2	1384598	2026161	100.00%	8.142%
98	21.684	3125	3131	3139	rVB2	763786	1228359	60.62%	4.936%
99	24.680	3632	3641	3651	rVB3	726073	1948097	96.15%	7.828%
100	24.904	3670	3679	3687	rBV2	462954	1285005	63.42%	5.164%

Sum of corrected areas: 24885156




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062824\
Data File : BG061789.D
Acq On : 29 Jun 2024 3:12
Operator : MA/JU
Sample : PB161592BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK592

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L

TIC Integration Parameters: LSCINT.P

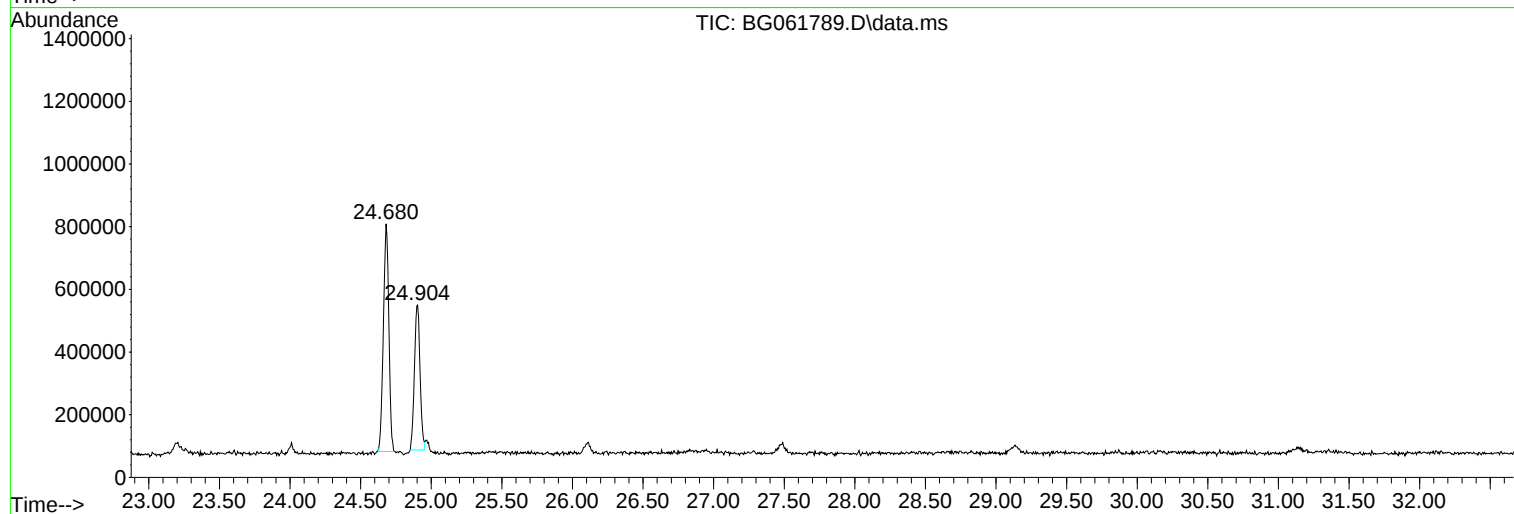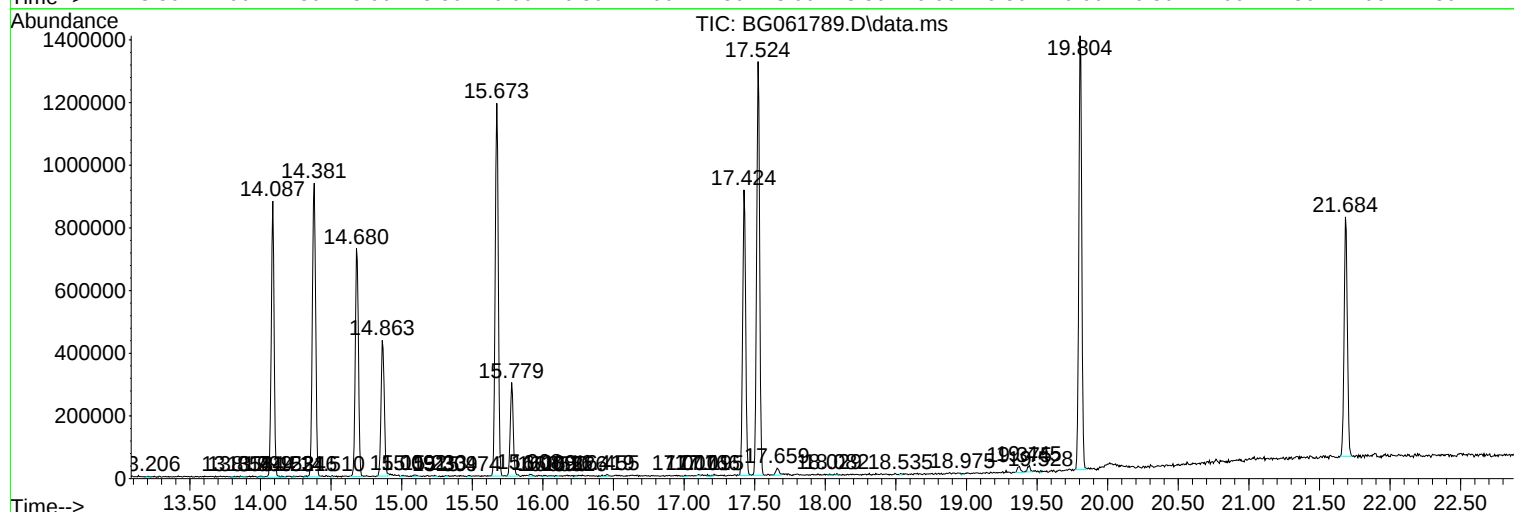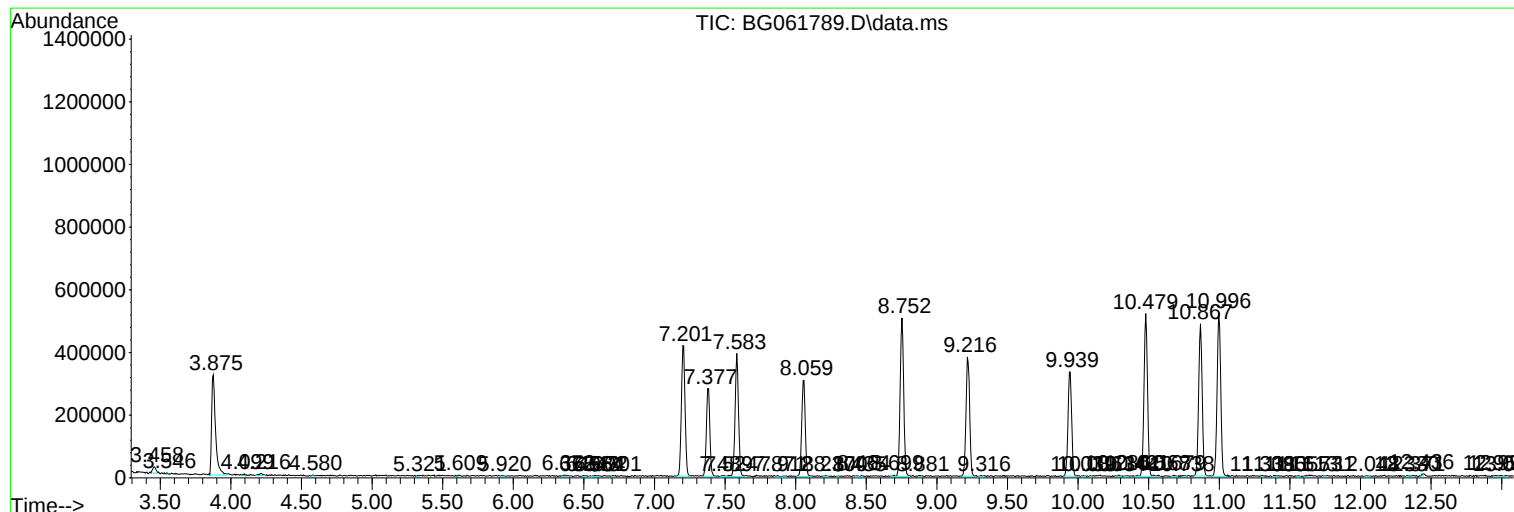

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062824\
Data File : BG061789.D
Acq On : 29 Jun 2024 3:12
Operator : MA/JU
Sample : PB161592BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK592

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062824\
Data File : BG061789.D
Acq On : 29 Jun 2024 3:12
Operator : MA/JU
Sample : PB161592BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK592

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc