

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062824\
 Data File : BG061790.D
 Acq On : 29 Jun 2024 3:52
 Operator : MA/JU
 Sample : P2897-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0SL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG061790.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.453	25	28	34	rVB	13322	21128	1.31%	0.106%
2	3.729	70	75	81	rBV	17837	26259	1.62%	0.132%
3	3.876	95	100	109	rBV	198178	366926	22.69%	1.846%
4	4.417	190	192	197	rVB3	3170	3896	0.24%	0.020%
5	4.464	197	200	204	rVB4	3131	4418	0.27%	0.022%
6	4.893	270	273	276	rBV4	3014	3921	0.24%	0.020%
7	4.993	285	290	292	rVV3	3283	5476	0.34%	0.028%
8	5.040	296	298	301	rBV4	3528	4397	0.27%	0.022%
9	5.128	309	313	319	rBV2	9352	16530	1.02%	0.083%
10	5.480	368	373	377	rVV3	2629	4358	0.27%	0.022%
11	6.115	476	481	488	rVB3	12499	24314	1.50%	0.122%
12	6.479	540	543	547	rBV3	2536	3634	0.22%	0.018%
13	7.020	632	635	637	rBV3	3489	3772	0.23%	0.019%
14	7.202	659	666	675	rVB	323850	538153	33.28%	2.708%
15	7.378	690	696	702	rBV	205377	338176	20.91%	1.701%
16	7.584	723	731	737	rBV	283652	470169	29.08%	2.365%
17	7.637	737	740	745	rVB3	7937	14342	0.89%	0.072%
18	7.989	798	800	804	rBV2	4279	5170	0.32%	0.026%
19	8.054	804	811	818	rVV	261297	449197	27.78%	2.260%
20	8.107	818	820	826	rVB4	9865	15292	0.95%	0.077%
21	8.459	877	880	883	rVB3	4180	3861	0.24%	0.019%
22	8.753	923	930	940	rVV	387190	644373	39.85%	3.242%
23	8.941	960	962	967	rVB4	2941	3527	0.22%	0.018%
24	9.217	1002	1009	1016	rBV	302232	508289	31.43%	2.557%
25	9.376	1031	1036	1041	rBV4	4221	7229	0.45%	0.036%
26	9.482	1049	1054	1058	rBV2	2617	4391	0.27%	0.022%
27	9.769	1098	1103	1110	rBV3	37047	62600	3.87%	0.315%
28	9.940	1122	1132	1141	rVB2	249481	441884	27.33%	2.223%
29	10.145	1164	1167	1169	rBV3	4182	4497	0.28%	0.023%
30	10.175	1171	1172	1176	rVB3	3122	3453	0.21%	0.017%
31	10.210	1176	1178	1181	rBV3	3569	3609	0.22%	0.018%
32	10.427	1212	1215	1216	rBV2	4291	3852	0.24%	0.019%
33	10.480	1216	1224	1232	rBV	375010	660831	40.87%	3.325%
34	10.627	1244	1249	1253	rBV4	4596	8408	0.52%	0.042%
35	10.745	1267	1269	1272	rVB3	3013	3463	0.21%	0.017%
36	10.868	1281	1290	1298	rVB	397694	710921	43.96%	3.577%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062824\
 Data File : BG061790.D
 Acq On : 29 Jun 2024 3:52
 Operator : MA/JU
 Sample : P2897-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0SL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

37	10.950	1300	1304	1305	rVV3	4504	6050	0.37%	0.030%
38	10.997	1305	1312	1321	rVB	376750	689374	42.63%	3.468%
39	11.091	1325	1328	1330	rBV2	2997	3903	0.24%	0.020%
40	11.232	1349	1352	1355	rVV2	3119	3444	0.21%	0.017%
41	11.385	1375	1378	1385	rVB3	14239	22930	1.42%	0.115%
42	11.603	1409	1415	1422	rVV	39512	75413	4.66%	0.379%
43	11.943	1469	1473	1475	rVB4	3354	4001	0.25%	0.020%
44	12.366	1542	1545	1551	rVB2	2957	4211	0.26%	0.021%
45	12.449	1555	1559	1562	rVV3	7003	10156	0.63%	0.051%
46	12.578	1580	1581	1584	rBV2	3521	3504	0.22%	0.018%
47	12.672	1595	1597	1599	rVV2	3480	3864	0.24%	0.019%
48	13.183	1680	1684	1688	rVB5	3596	5789	0.36%	0.029%
49	13.418	1721	1724	1727	rVV4	3182	3844	0.24%	0.019%
50	13.477	1733	1734	1738	rBV2	3430	4040	0.25%	0.020%
51	13.859	1796	1799	1802	rBV3	5261	5107	0.32%	0.026%
52	13.912	1805	1808	1811	rBV2	3636	6351	0.39%	0.032%
53	14.006	1817	1824	1829	rVB3	4773	9521	0.59%	0.048%
54	14.088	1829	1838	1844	rBV	691821	964056	59.62%	4.850%
55	14.323	1874	1878	1881	rBV5	6785	10530	0.65%	0.053%
56	14.382	1881	1888	1898	rVB	699257	1146275	70.89%	5.767%
57	14.487	1903	1906	1908	rBV2	3041	3562	0.22%	0.018%
58	14.581	1918	1922	1925	rBV4	3115	4504	0.28%	0.023%
59	14.681	1933	1939	1946	rVB	611490	955935	59.12%	4.809%
60	14.758	1949	1952	1953	rBV3	3933	3768	0.23%	0.019%
61	14.863	1963	1970	1980	rBV2	315122	534419	33.05%	2.689%
62	14.952	1984	1985	1987	rBV2	4505	3682	0.23%	0.019%
63	15.057	1999	2003	2004	rBV3	3141	4111	0.25%	0.021%
64	15.140	2016	2017	2020	rBV2	4429	4044	0.25%	0.020%
65	15.463	2068	2072	2075	rBV3	6573	12317	0.76%	0.062%
66	15.522	2079	2082	2084	rVB3	4977	5348	0.33%	0.027%
67	15.604	2094	2096	2098	rBV2	3507	3428	0.21%	0.017%
68	15.674	2101	2108	2114	rVV	913283	1386124	85.72%	6.974%
69	15.733	2116	2118	2121	rVV3	2853	3689	0.23%	0.019%
70	15.780	2121	2126	2133	rVV2	180373	258385	15.98%	1.300%
71	15.909	2146	2148	2151	rVV4	4075	3817	0.24%	0.019%
72	15.980	2155	2160	2163	rBV3	5581	9800	0.61%	0.049%
73	16.021	2165	2167	2171	rBV4	5495	7312	0.45%	0.037%
74	16.115	2181	2183	2186	rVB2	3484	3793	0.23%	0.019%
75	16.144	2186	2188	2191	rBV2	3721	3542	0.22%	0.018%
76	16.373	2222	2227	2228	rBV3	4456	6289	0.39%	0.032%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062824\
 Data File : BG061790.D
 Acq On : 29 Jun 2024 3:52
 Operator : MA/JU
 Sample : P2897-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 COSL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

77	16.491	2245	2247	2250	rBV3	3697	3667	0.23%	0.018%
78	16.714	2283	2285	2288	rVB2	3409	3623	0.22%	0.018%
79	16.967	2325	2328	2330	rVV3	4888	5582	0.35%	0.028%
80	17.172	2360	2363	2364	rBV3	7044	7042	0.44%	0.035%
81	17.208	2367	2369	2372	rVV4	4664	4802	0.30%	0.024%
82	17.331	2386	2390	2397	rVB7	9148	15109	0.93%	0.076%
83	17.425	2399	2406	2413	rVV	750731	1140212	70.51%	5.737%
84	17.525	2417	2423	2434	rVV2	1018297	1506772	93.18%	7.581%
85	17.607	2434	2437	2440	rVB4	6437	7964	0.49%	0.040%
86	17.660	2443	2446	2451	rVV5	14067	22665	1.40%	0.114%
87	17.701	2451	2453	2455	rVV3	5063	3610	0.22%	0.018%
88	18.089	2516	2519	2523	rBV4	5587	7758	0.48%	0.039%
89	18.230	2538	2543	2545	rBV4	5928	10431	0.65%	0.052%
90	18.306	2550	2556	2562	rVV6	34848	52168	3.23%	0.262%
91	18.636	2611	2612	2614	rBV2	8137	6686	0.41%	0.034%
92	18.782	2635	2637	2640	rVB4	5124	4988	0.31%	0.025%
93	19.170	2701	2703	2706	rBV4	8067	7147	0.44%	0.036%
94	19.370	2735	2737	2743	rVB6	15538	20604	1.27%	0.104%
95	19.805	2804	2811	2823	rBV	1123765	1617026	100.00%	8.135%
96	20.263	2887	2889	2890	rBV	12547	7927	0.49%	0.040%
97	21.338	3067	3072	3081	rBV3	165938	281290	17.40%	1.415%
98	21.685	3126	3131	3138	rVB	659645	1031904	63.81%	5.192%
99	24.681	3633	3641	3651	rVB2	560883	1492697	92.31%	7.510%
100	24.899	3670	3678	3688	rBV2	369271	1019678	63.06%	5.130%


Sum of corrected areas: 19876300

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062824\
Data File : BG061790.D
Acq On : 29 Jun 2024 3:52
Operator : MA/JU
Sample : P2897-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
COSL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

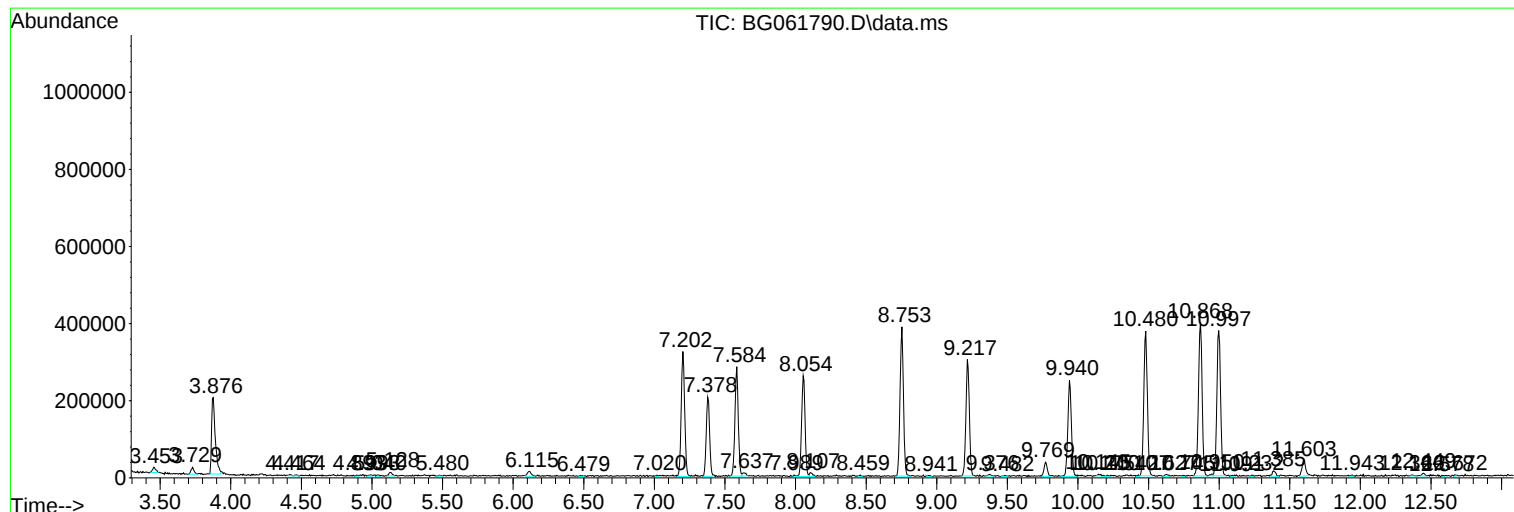

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062824\
Data File : BG061790.D
Acq On : 29 Jun 2024 3:52
Operator : MA/JU
Sample : P2897-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0SL2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1-Phenoxypropan-2-ol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.603	2.12 ng/ul	75413	Naphthalene-d8	10.868

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Phenoxypropan-2-ol			152	C9H12O2	000770-35-4	96
2	1-Phenoxypropan-2-ol			152	C9H12O2	000770-35-4	95
3	1-Phenoxypropan-2-ol			152	C9H12O2	000770-35-4	93
4	1-Propanol, 3-phenoxy-			152	C9H12O2	006180-61-6	91
5	1-Phenoxypropan-2-ol			152	C9H12O2	000770-35-4	90

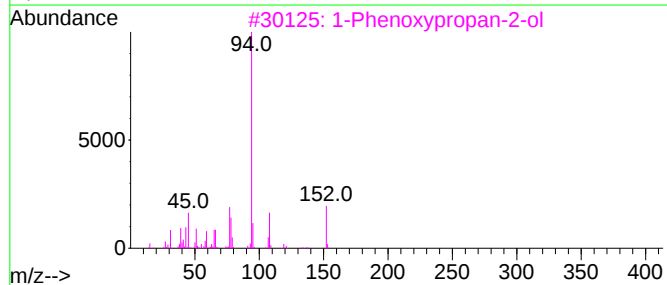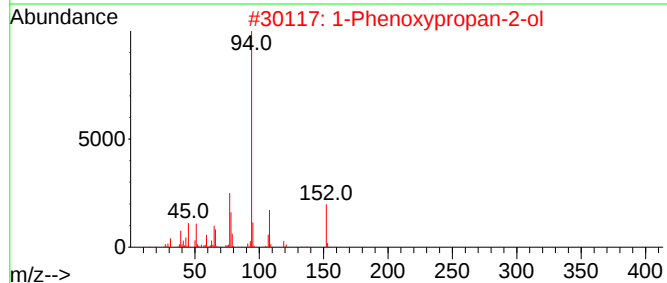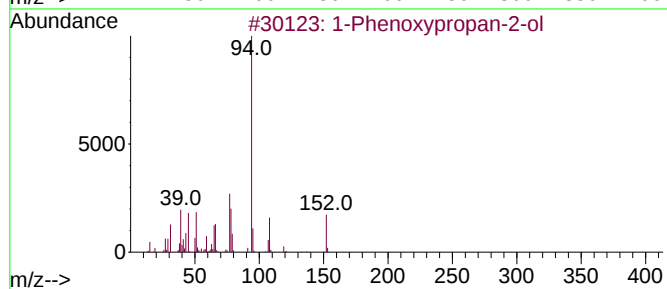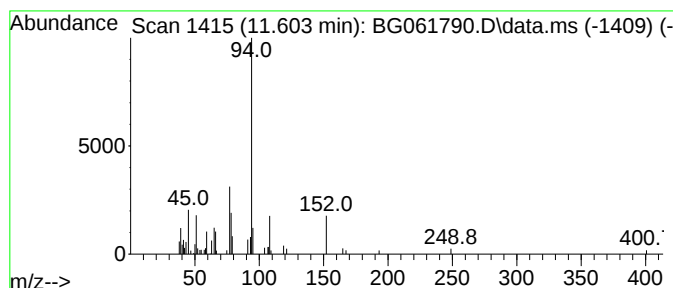

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062824\
Data File : BG061790.D
Acq On : 29 Jun 2024 3:52
Operator : MA/JU
Sample : P2897-04
Misc :
ALS Vial : 19 Sample Multiplier: 1










Instrument :
BNA_G
ClientSampleId :
COSL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.	
21.338	5.45 ng/ul	281290	Chrysene-d12		21.685	
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	1-Nonadecene		266	C19H38	018435-45-5	90
2	Heptafluorobutyric acid, n-octad...		466	C22H37F7O2	000400-57-7	90
3	Heptadecyl heptafluorobutyrate		452	C21H35F7O2	959085-66-6	90
4	Heptadecyl trifluoroacetate		352	C19H35F3O2	1010351-87-0	87
5	Eicosyl trifluoroacetate		394	C22H41F3O2	1000351-75-2	87

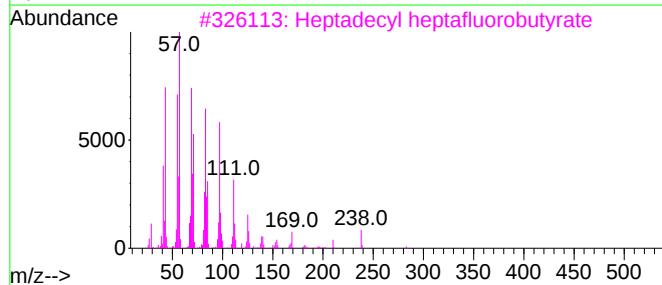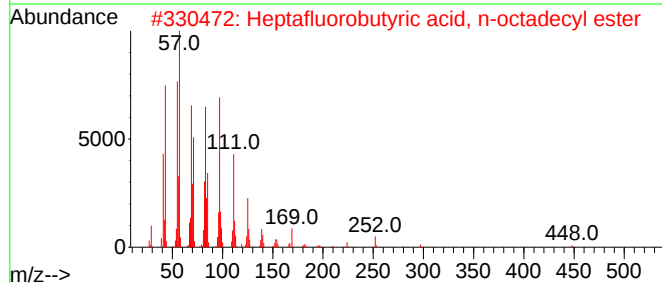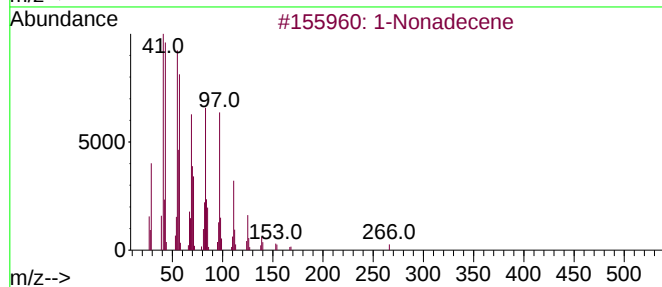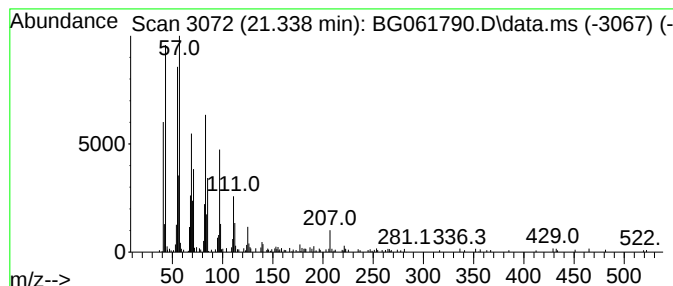

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062824\
Data File : BG061790.D
Acq On : 29 Jun 2024 3:52
Operator : MA/JU
Sample : P2897-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0SL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Phenoxypropan...	11.603	2.1	ng/u1	75413	2	10.868	710921	20.0
(DEL) Alkane: S...	21.338	5.5	ng/u1	281290	5	21.685	1031900	20.0