

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062824\
 Data File : BG061792.D
 Acq On : 29 Jun 2024 5:14
 Operator : MA/JU
 Sample : P2897-09
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 COSL4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG061792.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.458	25	29	33	rBV2	16505	24628	1.35%	0.112%
2	3.729	71	75	81	rBV	18018	34828	1.90%	0.158%
3	3.881	98	101	108	rBV	23019	40993	2.24%	0.186%
4	4.181	149	152	154	rVB4	3496	3668	0.20%	0.017%
5	4.216	156	158	160	rVV3	5404	4358	0.24%	0.020%
6	4.363	181	183	186	rVB2	3692	3440	0.19%	0.016%
7	4.428	189	194	195	rBV5	2903	3941	0.22%	0.018%
8	4.504	205	207	212	rVB5	3299	4453	0.24%	0.020%
9	4.780	249	254	257	rBV4	5629	8816	0.48%	0.040%
10	4.892	269	273	275	rBV3	4239	5365	0.29%	0.024%
11	5.133	309	314	321	rBV2	13736	22703	1.24%	0.103%
12	5.362	351	353	357	rBV3	3926	5918	0.32%	0.027%
13	5.480	370	373	375	rVB2	2855	3501	0.19%	0.016%
14	6.114	475	481	486	rVB3	13483	23444	1.28%	0.106%
15	6.267	504	507	510	rVB3	3766	3832	0.21%	0.017%
16	6.361	519	523	525	rBV3	4003	4963	0.27%	0.023%
17	6.760	588	591	596	rBV5	2439	4214	0.23%	0.019%
18	6.907	614	616	619	rBV3	4806	6179	0.34%	0.028%
19	7.201	657	666	676	rVB	371138	627801	34.31%	2.849%
20	7.283	676	680	682	rBV3	3019	3666	0.20%	0.017%
21	7.377	689	696	707	rVB	250325	416217	22.75%	1.889%
22	7.583	724	731	737	rVV	337748	566087	30.94%	2.569%
23	7.636	737	740	743	rVB2	8425	11348	0.62%	0.052%
24	7.689	748	749	754	rVB2	3564	4915	0.27%	0.022%
25	7.736	754	757	760	rBV4	3919	5056	0.28%	0.023%
26	7.812	767	770	775	rBV5	4026	7812	0.43%	0.035%
27	8.053	803	811	818	rVV	283142	484427	26.48%	2.199%
28	8.106	818	820	826	rVV3	10300	15711	0.86%	0.071%
29	8.594	902	903	906	rBV3	3192	3394	0.19%	0.015%
30	8.752	923	930	941	rVV	431616	735381	40.19%	3.338%
31	9.216	1003	1009	1018	rBV	339867	614027	33.56%	2.787%
32	9.369	1031	1035	1040	rVB4	5385	8820	0.48%	0.040%
33	9.769	1098	1103	1109	rVB3	34574	57056	3.12%	0.259%
34	9.939	1124	1132	1140	rBV2	282539	522881	28.58%	2.373%
35	10.151	1163	1168	1169	rBV4	6489	7943	0.43%	0.036%
36	10.174	1169	1172	1174	rVB4	3844	4322	0.24%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062824\
 Data File : BG061792.D
 Acq On : 29 Jun 2024 5:14
 Operator : MA/JU
 Sample : P2897-09
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 COSL4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

37	10.480	1216	1224	1233	rVV	437336	783423	42.82%	3.556%
38	10.568	1236	1239	1242	rBV3	2275	3330	0.18%	0.015%
39	10.632	1247	1250	1257	rVB4	8902	15655	0.86%	0.071%
40	10.867	1282	1290	1298	rBV	417939	760542	41.57%	3.452%
41	10.950	1300	1304	1305	rVV4	6219	8060	0.44%	0.037%
42	10.997	1305	1312	1321	rVV	328041	606422	33.15%	2.752%
43	11.314	1361	1366	1370	rVV3	23880	37914	2.07%	0.172%
44	11.384	1373	1378	1385	rBV4	12856	22605	1.24%	0.103%
45	11.508	1395	1399	1403	rBV4	3789	5203	0.28%	0.024%
46	11.596	1406	1414	1423	rBV2	46313	94554	5.17%	0.429%
47	11.672	1426	1427	1431	rVB2	4011	3942	0.22%	0.018%
48	11.702	1431	1432	1436	rBV	3154	3749	0.20%	0.017%
49	11.790	1445	1447	1450	rVB3	3798	3400	0.19%	0.015%
50	12.330	1535	1539	1540	rBV4	3384	3819	0.21%	0.017%
51	12.395	1546	1550	1554	rBV2	4005	6259	0.34%	0.028%
52	12.436	1554	1557	1558	rBV2	7546	6288	0.34%	0.029%
53	12.947	1642	1644	1646	rVB3	4043	3544	0.19%	0.016%
54	12.988	1649	1651	1652	rBV	5526	4316	0.24%	0.020%
55	13.065	1662	1664	1666	rBV3	2863	3754	0.21%	0.017%
56	13.165	1678	1681	1682	rBV2	3450	3803	0.21%	0.017%
57	13.500	1736	1738	1742	rVB4	3633	4238	0.23%	0.019%
58	13.594	1751	1754	1758	rVB3	8562	10170	0.56%	0.046%
59	13.647	1761	1763	1768	rVB5	4667	5955	0.33%	0.027%
60	13.776	1782	1785	1788	rBV2	3043	3585	0.20%	0.016%
61	13.870	1799	1801	1805	rVB3	4452	4598	0.25%	0.021%
62	14.087	1829	1838	1845	rBV	743301	1072819	58.64%	4.869%
63	14.199	1851	1857	1860	rVB4	4181	6864	0.38%	0.031%
64	14.322	1874	1878	1881	rVV5	6604	12717	0.70%	0.058%
65	14.381	1881	1888	1894	rVB	845824	1327806	72.57%	6.026%
66	14.604	1924	1926	1929	rVB4	5333	5357	0.29%	0.024%
67	14.681	1933	1939	1947	rVB	675437	1024044	55.97%	4.648%
68	14.757	1947	1952	1954	rBV5	4277	6802	0.37%	0.031%
69	14.816	1958	1962	1963	rBV2	2981	3648	0.20%	0.017%
70	14.863	1963	1970	1980	rBV	352962	605314	33.08%	2.747%
71	14.992	1990	1992	1997	rVB3	8425	10709	0.59%	0.049%
72	15.227	2031	2032	2034	rBV2	5437	4867	0.27%	0.022%
73	15.256	2034	2037	2042	rVV5	12012	15855	0.87%	0.072%
74	15.456	2068	2071	2074	rBV3	5619	7642	0.42%	0.035%
75	15.674	2101	2108	2114	rBV	1077146	1607585	87.87%	7.296%
76	15.779	2121	2126	2132	rBV2	222197	313253	17.12%	1.422%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062824\
 Data File : BG061792.D
 Acq On : 29 Jun 2024 5:14
 Operator : MA/JU
 Sample : P2897-09
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 COSL4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

77	15.909	2144	2148	2153	rVB7	6964	12301	0.67%	0.056%
78	15.985	2157	2161	2164	rBV5	6308	9666	0.53%	0.044%
79	16.232	2201	2203	2205	rVB3	6219	5094	0.28%	0.023%
80	16.308	2214	2216	2218	rVB3	4861	4245	0.23%	0.019%
81	16.431	2234	2237	2238	rBV3	4425	4812	0.26%	0.022%
82	17.172	2360	2363	2364	rBV3	8687	10608	0.58%	0.048%
83	17.213	2367	2370	2373	rBV3	6793	7701	0.42%	0.035%
84	17.289	2381	2383	2386	rBV4	5320	4130	0.23%	0.019%
85	17.336	2387	2391	2397	rVB7	12128	18968	1.04%	0.086%
86	17.424	2400	2406	2412	rVV	804851	1209717	66.12%	5.490%
87	17.524	2416	2423	2431	rVB	1164778	1735522	94.86%	7.877%
88	17.665	2442	2447	2450	rBV5	13670	23871	1.30%	0.108%
89	17.871	2480	2482	2483	rBV2	4393	3429	0.19%	0.016%
90	18.083	2516	2518	2521	rBV4	8020	7071	0.39%	0.032%
91	18.306	2552	2556	2564	rBV4	80569	120423	6.58%	0.547%
92	18.641	2612	2613	2616	rBV3	9235	9185	0.50%	0.042%
93	18.729	2626	2628	2632	rBV5	6543	7234	0.40%	0.033%
94	19.446	2745	2750	2753	rBV4	21111	35049	1.92%	0.159%
95	19.657	2784	2786	2787	rBV2	10009	5087	0.28%	0.023%
96	19.804	2805	2811	2818	rBV	1224942	1829577	100.00%	8.304%
97	21.332	3068	3071	3082	rVB	176985	277745	15.18%	1.261%
98	21.684	3125	3131	3141	rVB	701975	1128822	61.70%	5.123%
99	24.681	3633	3641	3652	rVB3	613134	1713119	93.63%	7.775%
100	24.898	3670	3678	3686	rBV3	400718	1109109	60.62%	5.034%




Sum of corrected areas: 22033003

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062824\
Data File : BG061792.D
Acq On : 29 Jun 2024 5:14
Operator : MA/JU
Sample : P2897-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0SL4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

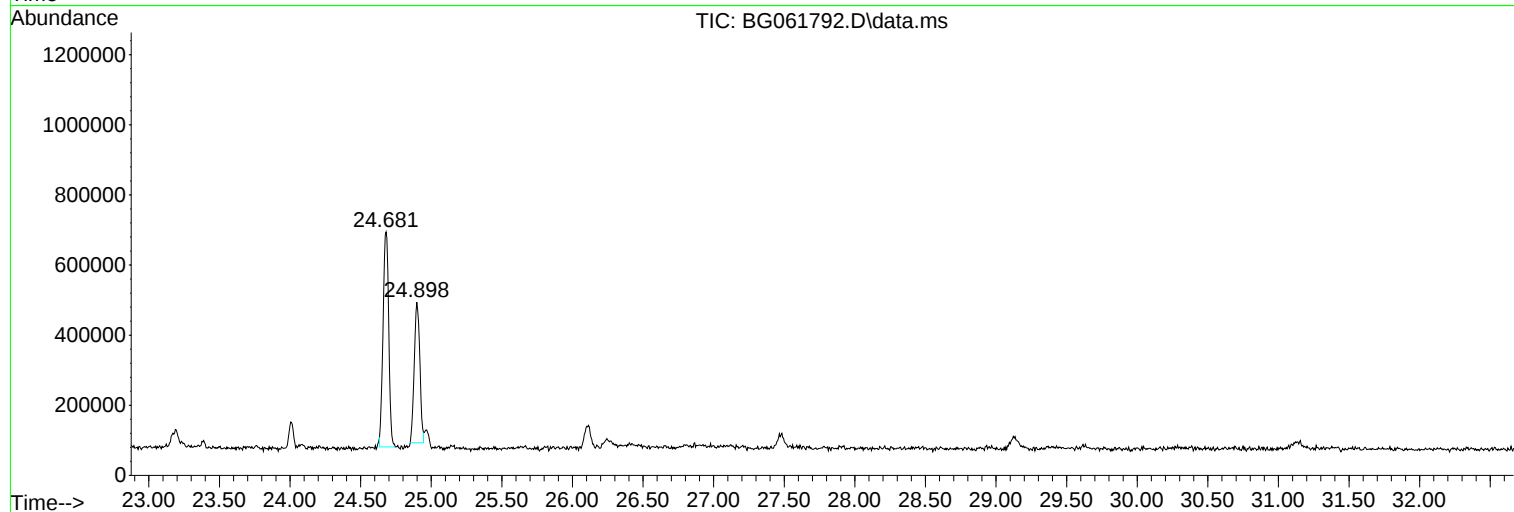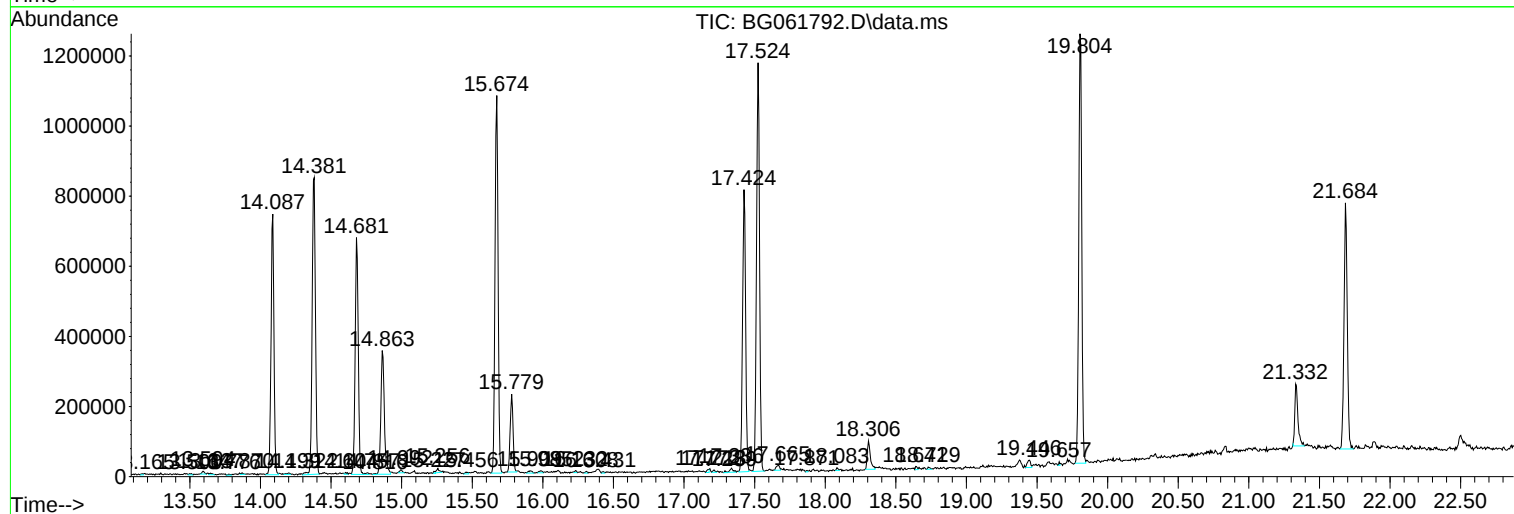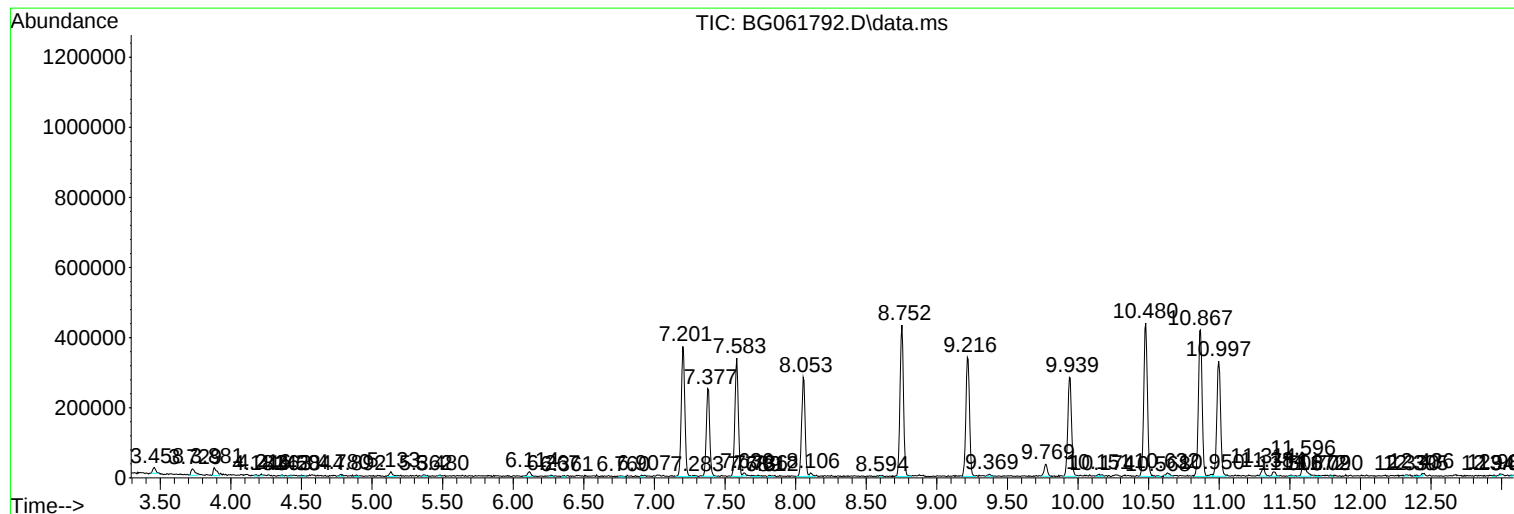

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062824\
Data File : BG061792.D
Acq On : 29 Jun 2024 5:14
Operator : MA/JU
Sample : P2897-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
COSL4










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1-Phenoxypropan-2-ol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.596	2.49 ng/ul	94554	Naphthalene-d8	10.867

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Phenoxypropan-2-ol		152	C9H12O2	000770-35-4	93	
2	1-Phenoxypropan-2-ol		152	C9H12O2	000770-35-4	90	
3	1-Phenoxypropan-2-ol		152	C9H12O2	000770-35-4	90	
4	1-Propanol, 3-phenoxy-		152	C9H12O2	006180-61-6	87	
5	1-Phenoxypropan-2-ol		152	C9H12O2	000770-35-4	81	

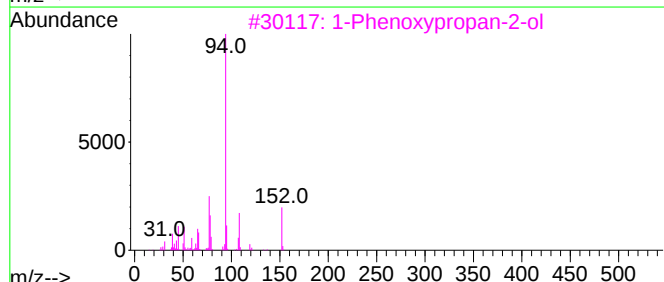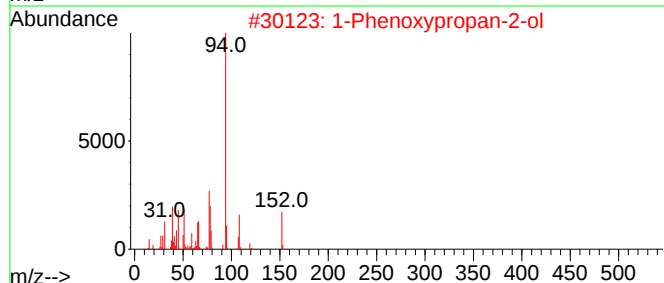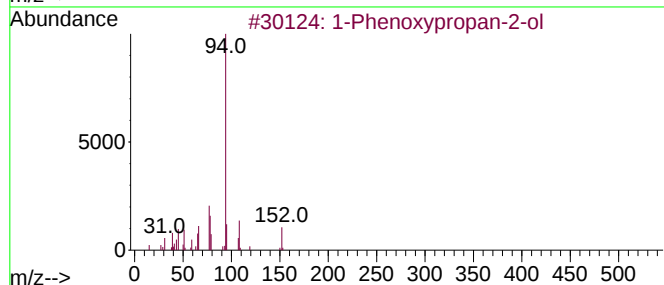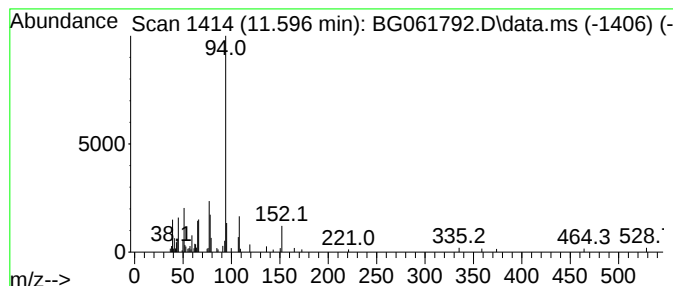

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062824\
Data File : BG061792.D
Acq On : 29 Jun 2024 5:14
Operator : MA/JU
Sample : P2897-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
COSL4










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Cyclic21.332 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.332	4.92 ng/ul	277745	Chrysene-d12	21.684

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclotetracosane	336	C24H48	000297-03-0	97
2			Z-14-Nonacosene	406	C29H58	1010131-18-9	95
3			Trichloroacetic acid, hexadecyl ...	386	C18H33Cl3O2	074339-54-1	93
4			Trichloroacetic acid, pentadecyl...	372	C17H31Cl3O2	074339-53-0	93
5			1-Docosene	308	C22H44	001599-67-3	93

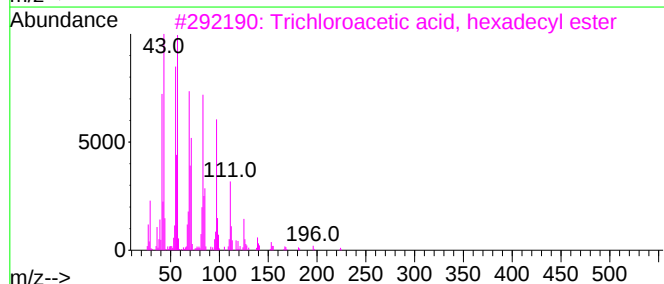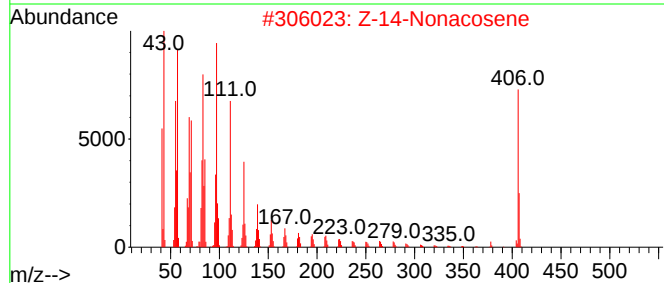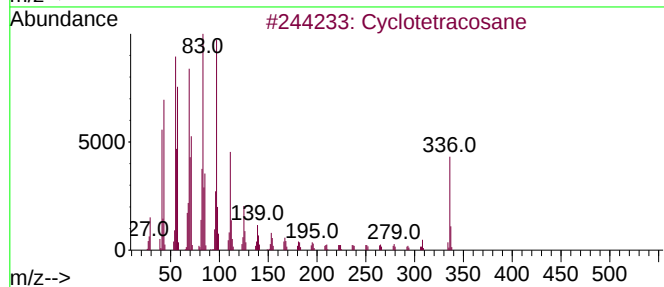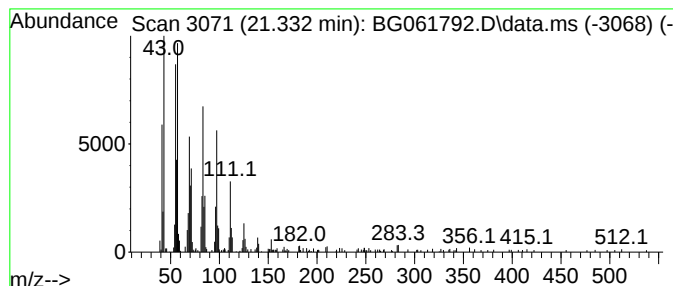

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062824\
Data File : BG061792.D
Acq On : 29 Jun 2024 5:14
Operator : MA/JU
Sample : P2897-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0SL4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Phenoxypropan...	11.596	2.5	ng/u1	94554	2	10.867	760542	20.0
(DEL) Alkane: C...	21.332	4.9	ng/u1	277745	5	21.684	1128820	20.0