
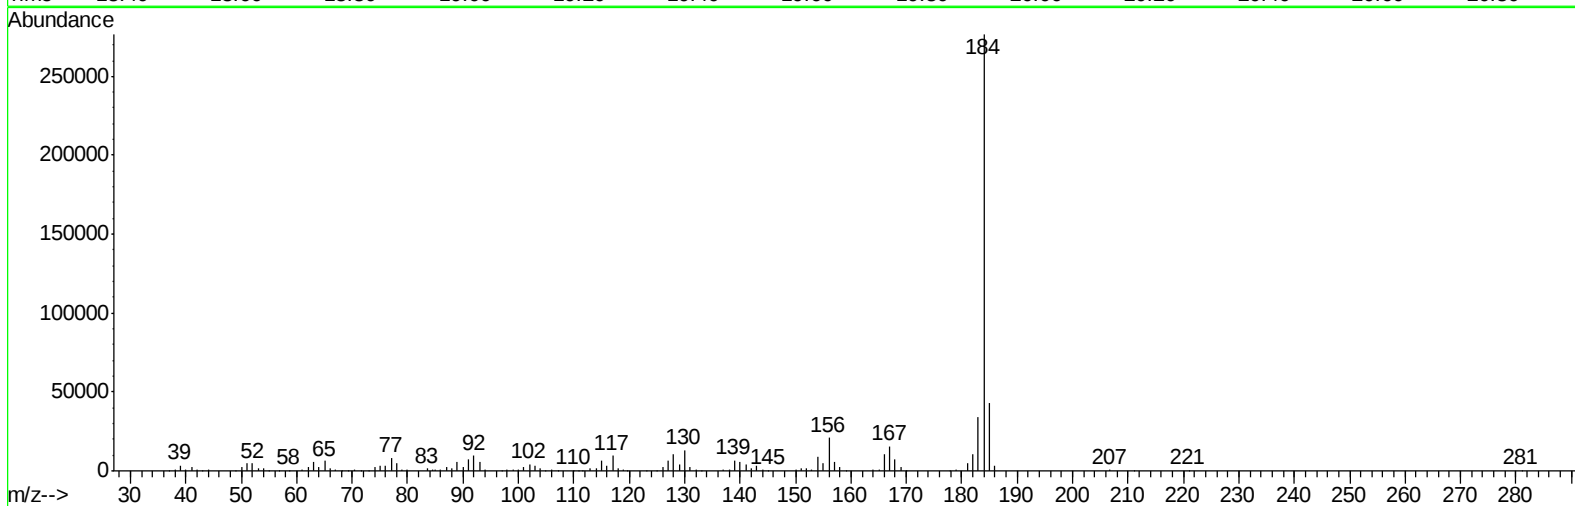


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG062919\
Data File : BG041537.D
Acq On : 29 Jun 2019 9:07
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 29 10:23:46 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG062619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 27 13:25:55 2019
Response via : Initial Calibration

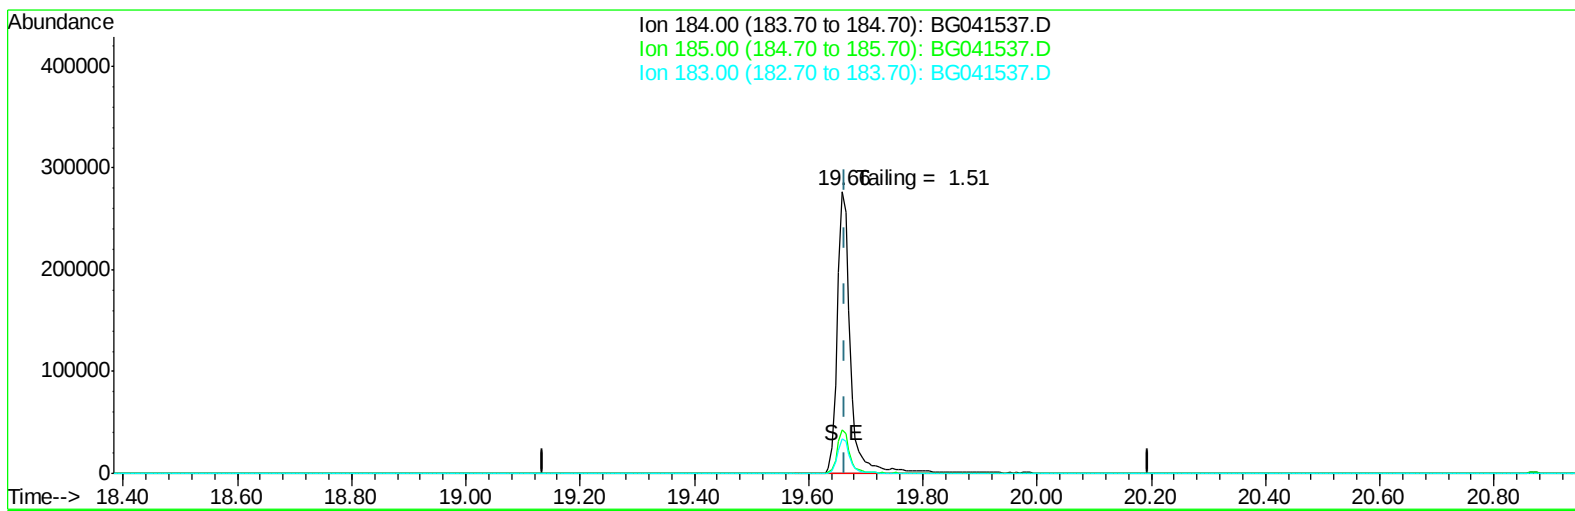

TIC: BG041537.D

(77) Benzidine



19.658min (-0.006) 0.00ng

response 435238

Ion	Exp%	Act%
184.00	100	100
185.00	15.90	15.68
183.00	11.80	12.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG062919\
Data File : BG041537.D
Acq On : 29 Jun 2019 9:07
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 29 10:23:46 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG062619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 27 13:25:55 2019
Response via : Initial Calibration

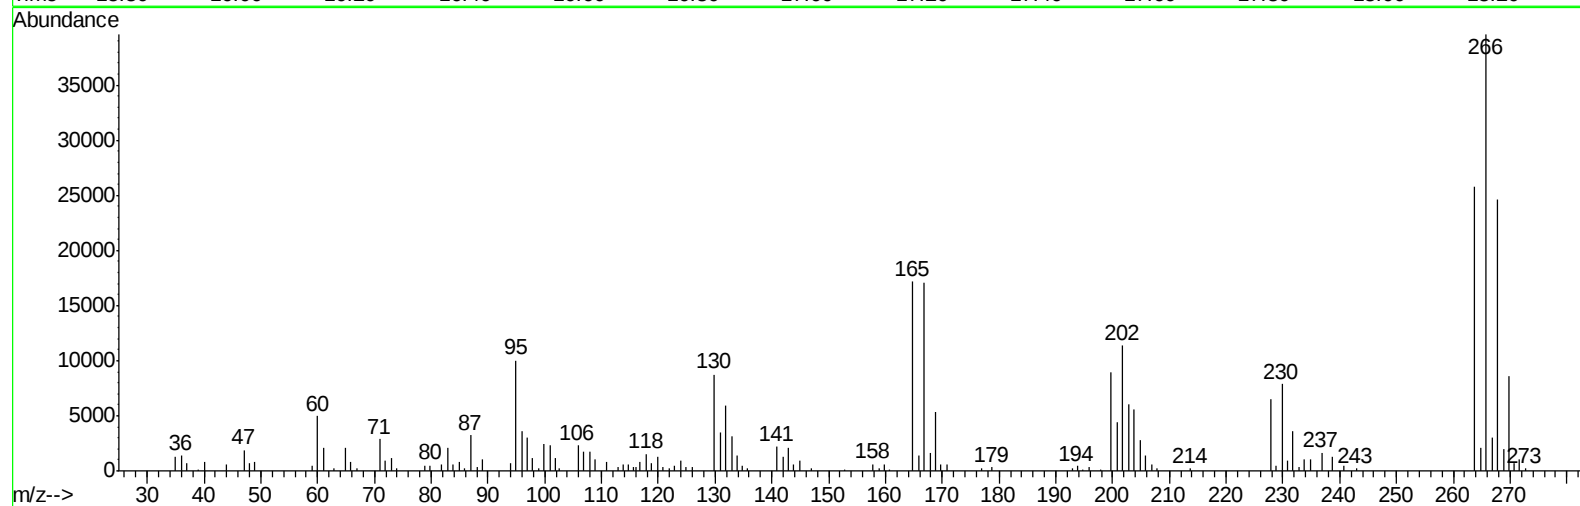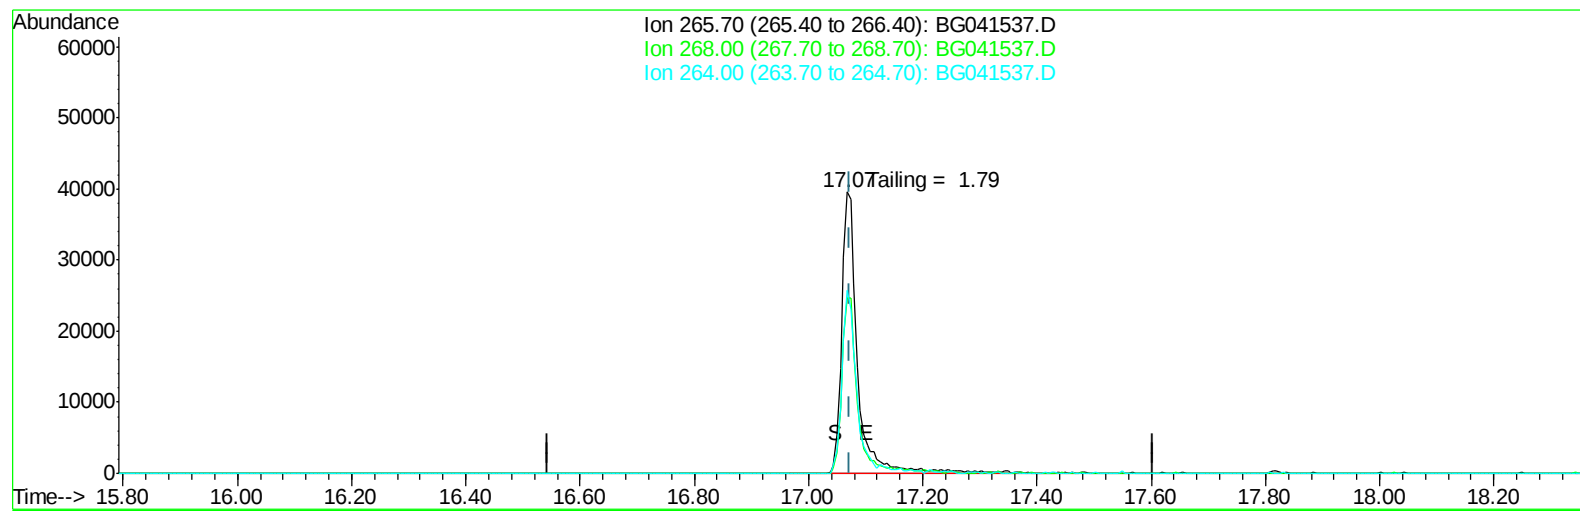

TIC: BG041537.D

(70) Pentachlorophenol (C)

17.067min (-0.006) 31039.80ng

response 74342

Ion	Exp%	Act%
265.70	100	100
268.00	58.70	62.18
264.00	59.20	65.19
0.00	0.00	0.00