


Data Path : \\74.0.250.170\TERASTORAGE\SVOASRV\HPCHEM1\BNA_G\DATA\BG062919\
Data File : BG041537.D
Acq On : 29 Jun 2019 9:07
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG062619.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jun 27 13:25:55 2019

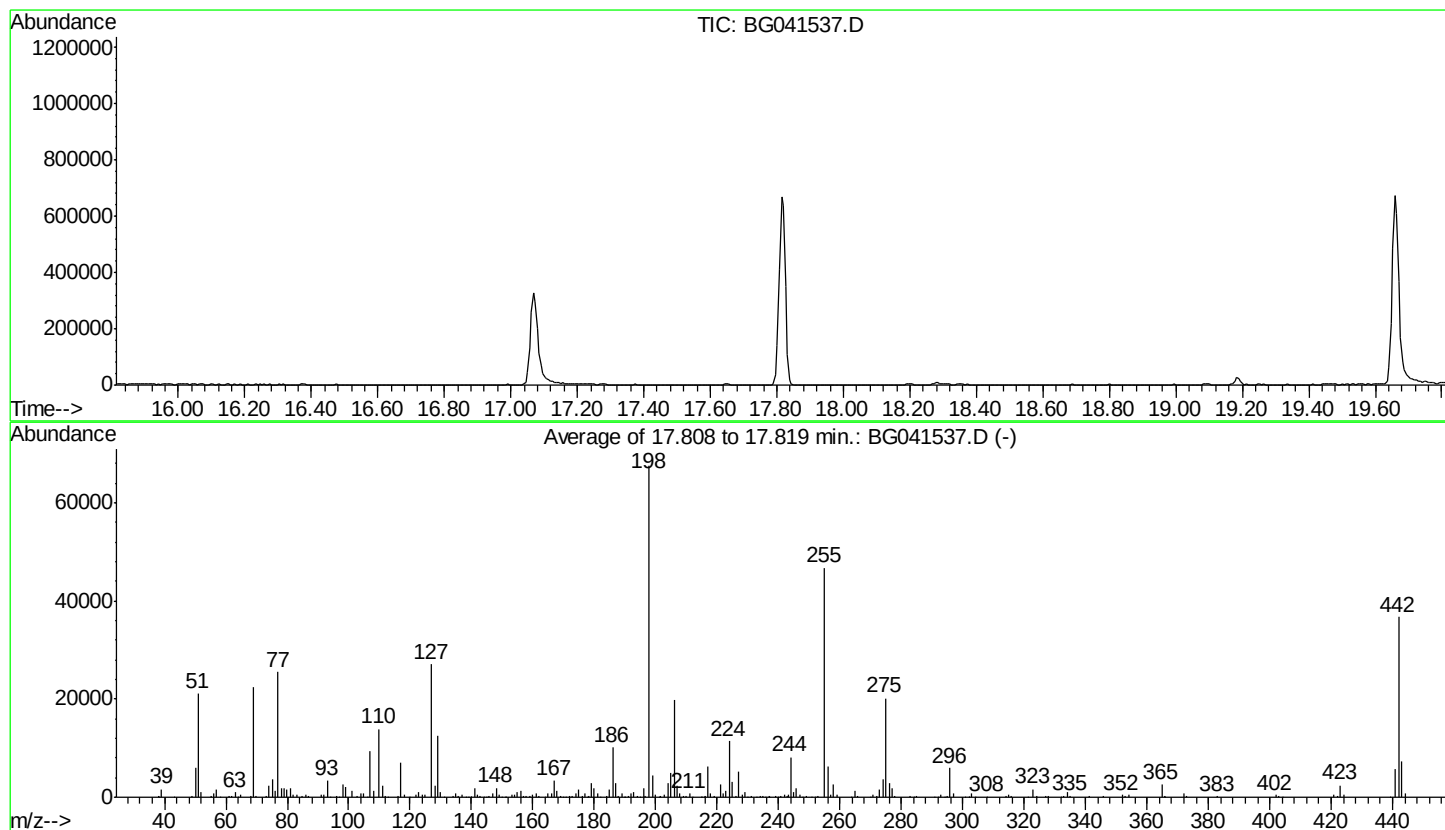

AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.1	21026	PASS
68	69	0.00	2	0.8	181	PASS
69	198	0.00	100	33.4	22549	PASS
70	69	0.00	2	0.7	152	PASS
127	198	10	80	40.1	27082	PASS
197	198	0.00	2	0.3	208	PASS
198	198	100	100	100.0	67549	PASS
199	198	5	9	6.7	4552	PASS
275	198	10	60	29.9	20183	PASS
365	198	1	100	3.7	2488	PASS
441	198	0.01	100	8.6	5778	PASS
442	198	50	100	54.3	36685	PASS
443	442	15	24	19.9	7297	PASS