
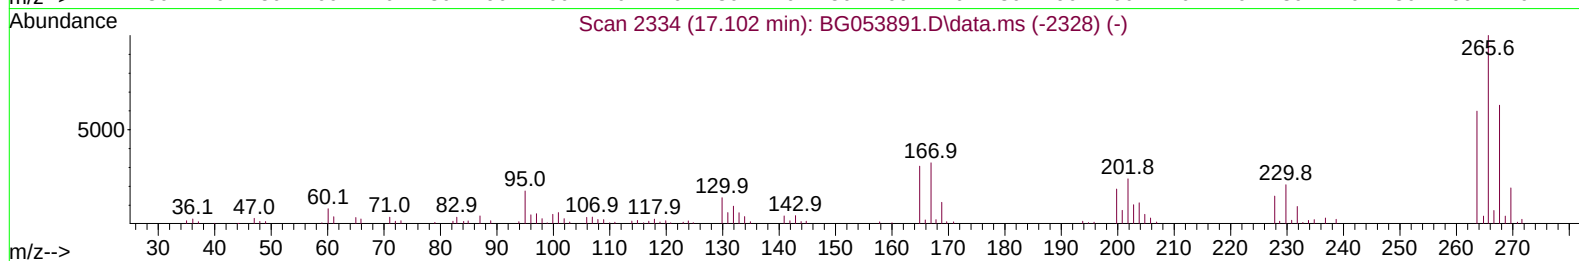
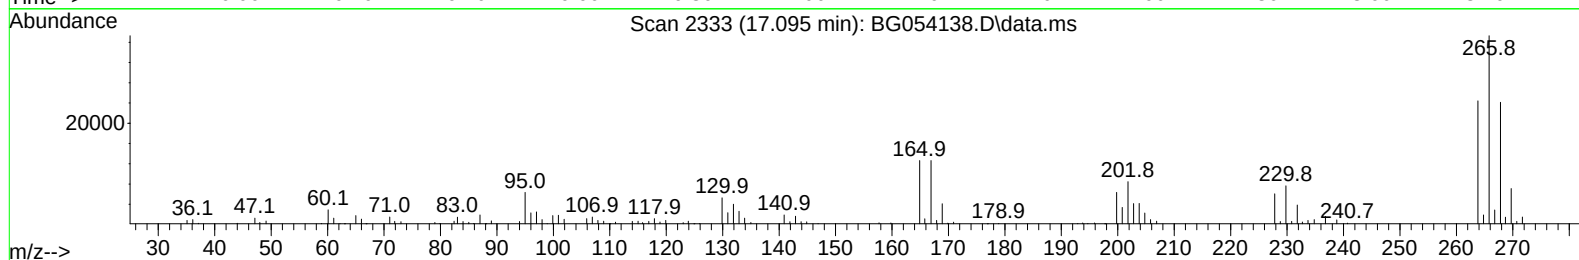


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062922\
Data File : BG054138.D
Acq On : 29 Jun 2022 10:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 29 14:18:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 00:27:54 2022
Response via : Initial Calibration

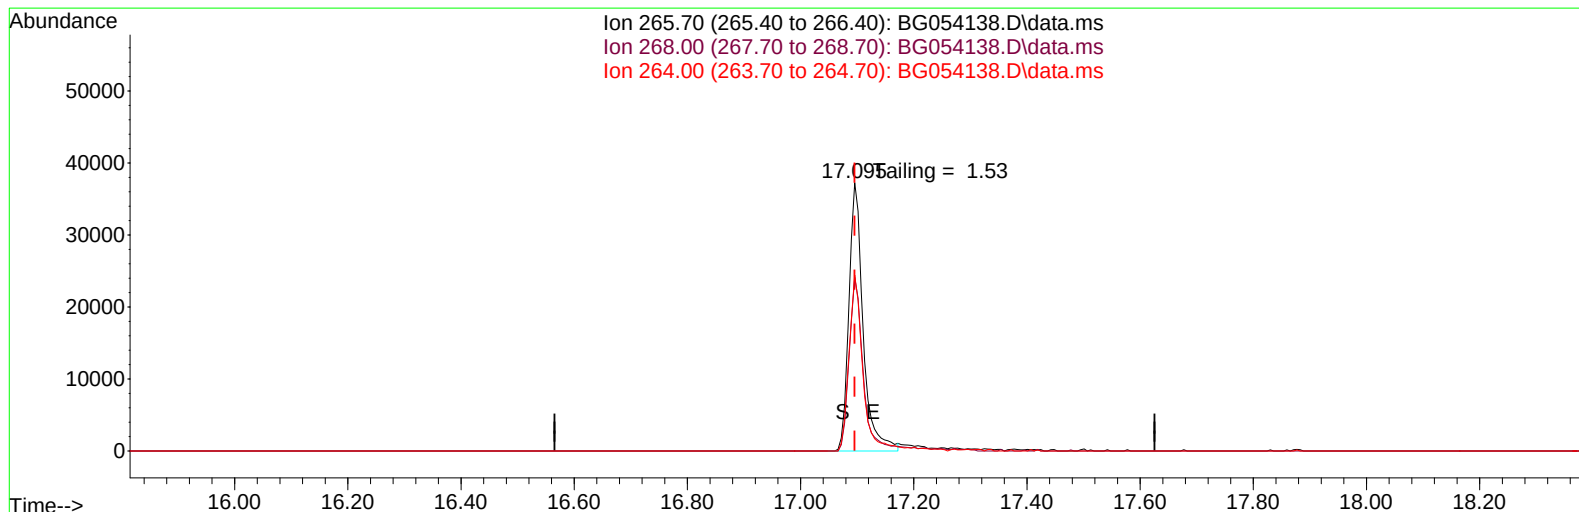

TIC: BG054138.D\data.ms

(70) Pentachlorophenol (C)




17.095min (+ 0.000) 19179.71 ng

response 67588

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	68.56
264.00	66.20	65.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062922\
Data File : BG054138.D
Acq On : 29 Jun 2022 10:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 29 14:18:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 00:27:54 2022
Response via : Initial Calibration

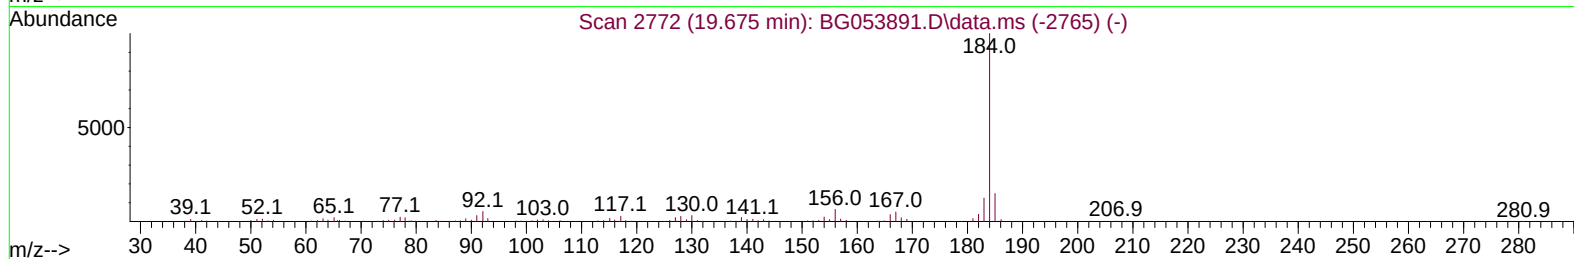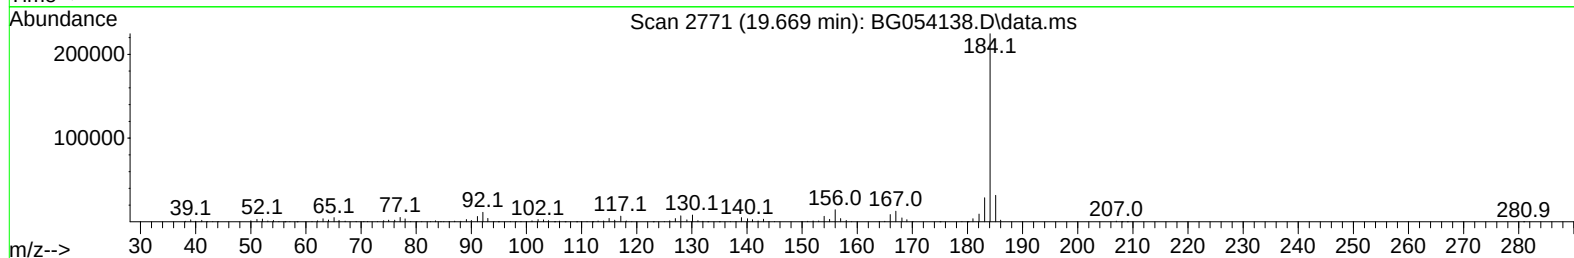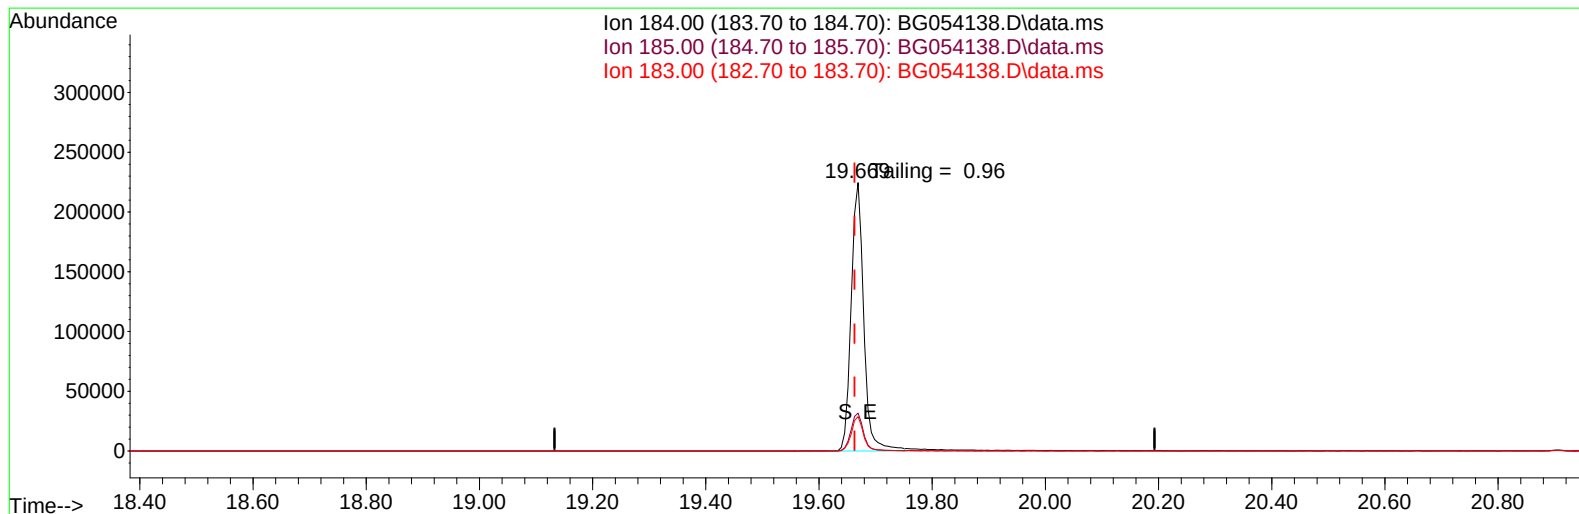

TIC: BG054138.D\data.ms

(77) Benzidine**19.669min (+ 0.006) 122952.16 ng****response 356469**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.12
183.00	11.10	12.86
0.00	0.00	0.00