
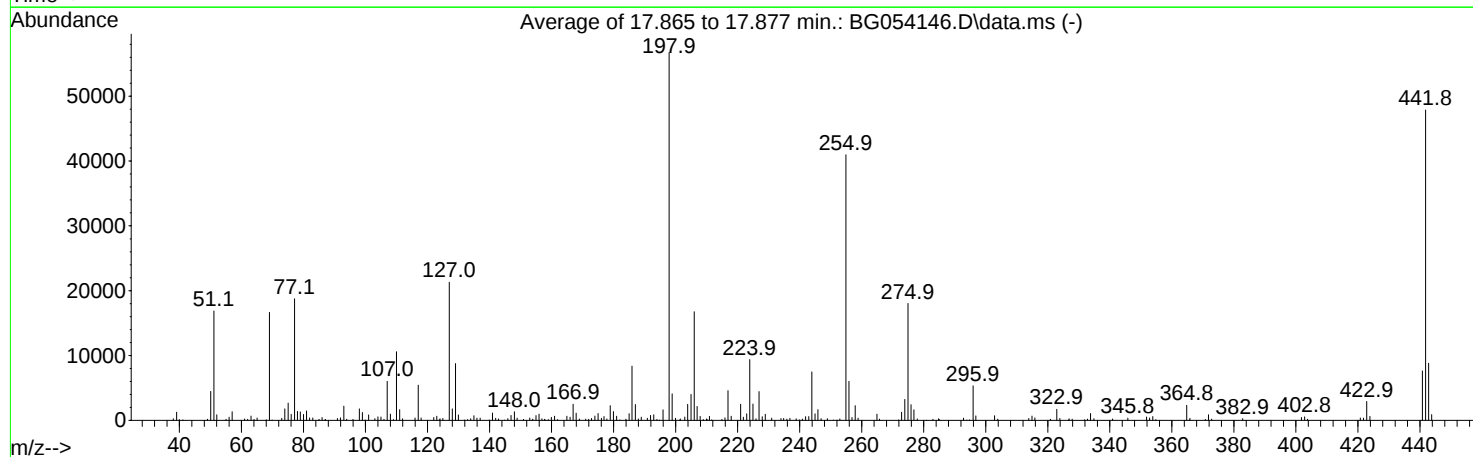


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062922\
 Data File : BG054146.D
 Acq On : 29 Jun 2022 15:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 27 00:27:54 2022

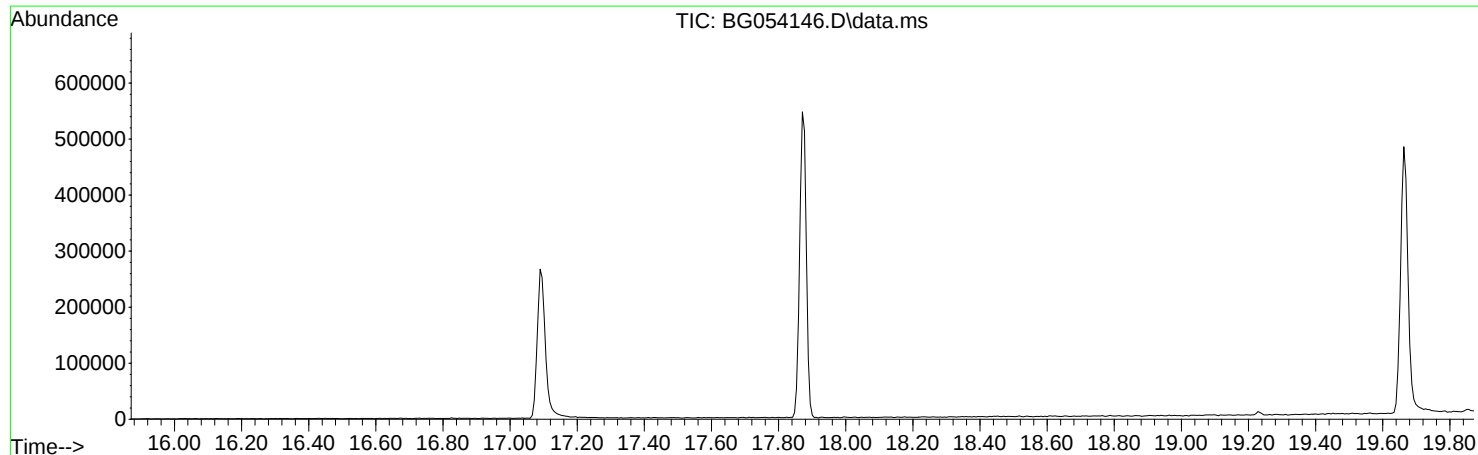




AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.8	16894	PASS
68	69	0.00	2	0.6	104	PASS
69	198	0.00	100	29.3	16648	PASS
70	69	0.00	2	0.4	63	PASS
127	198	10	80	37.5	21293	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	56741	PASS
199	198	5	9	7.2	4096	PASS
275	198	10	60	31.8	18036	PASS
365	198	1	100	4.1	2324	PASS
441	198	0.01	100	13.5	7632	PASS
442	442	50	100	100.0	47877	PASS
443	442	15	24	18.4	8821	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062922\
Data File : BG054146.D
Acq On : 29 Jun 2022 15:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 29 16:12:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 00:27:54 2022
Response via : Initial Calibration

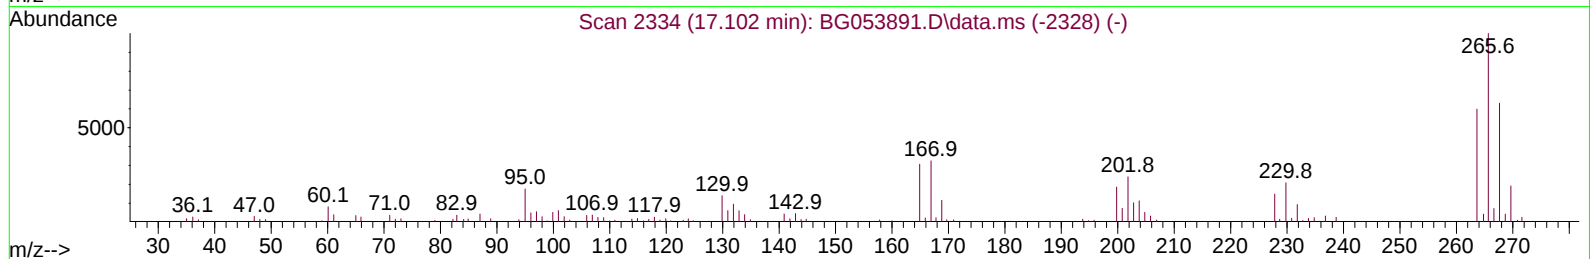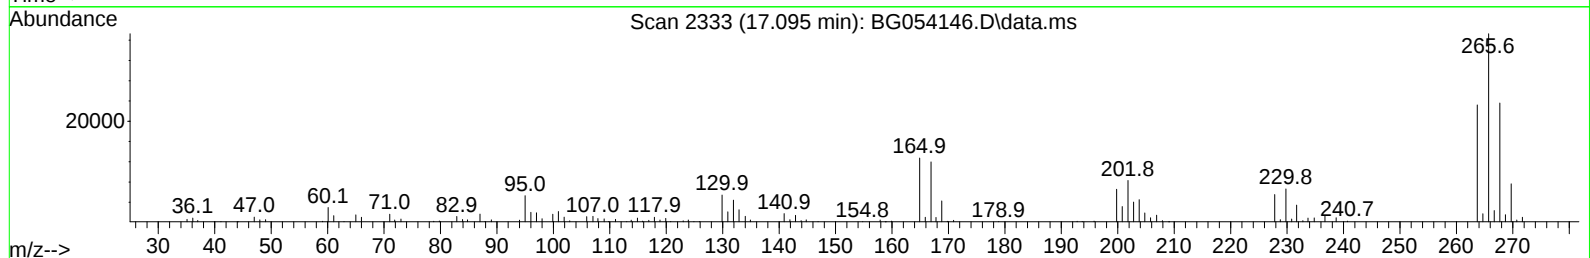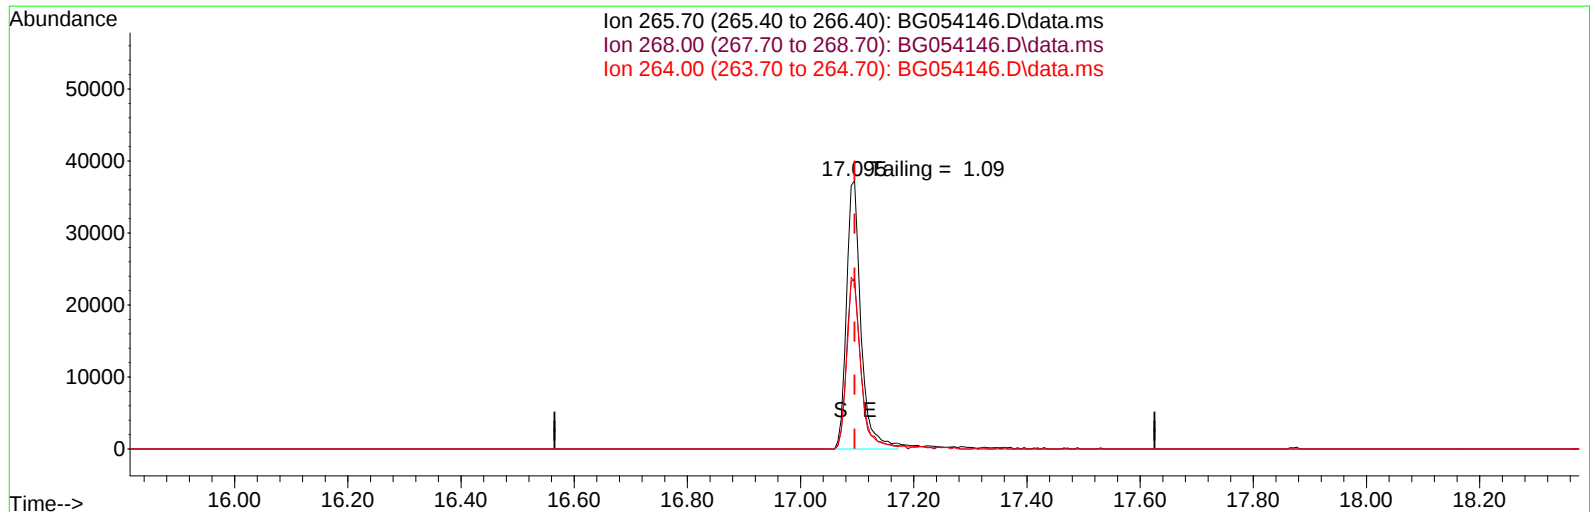

TIC: BG054146.D\data.ms

(70) Pentachlorophenol (C)

17.095min (+ 0.000) 44999.82 ng




response 67492

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	67.50
264.00	66.20	66.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062922\
Data File : BG054146.D
Acq On : 29 Jun 2022 15:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 29 16:12:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 00:27:54 2022
Response via : Initial Calibration

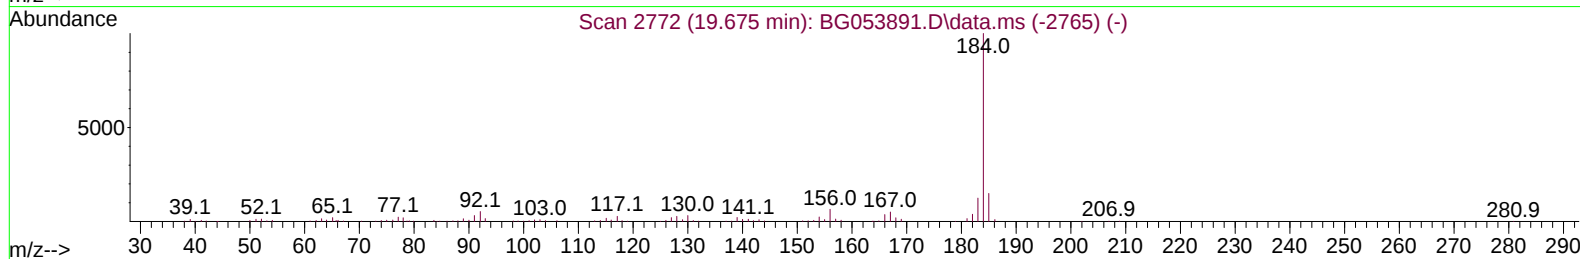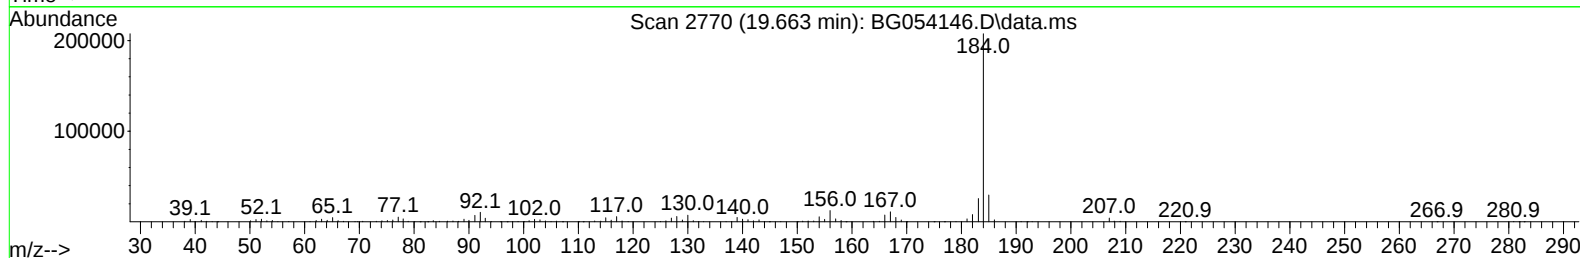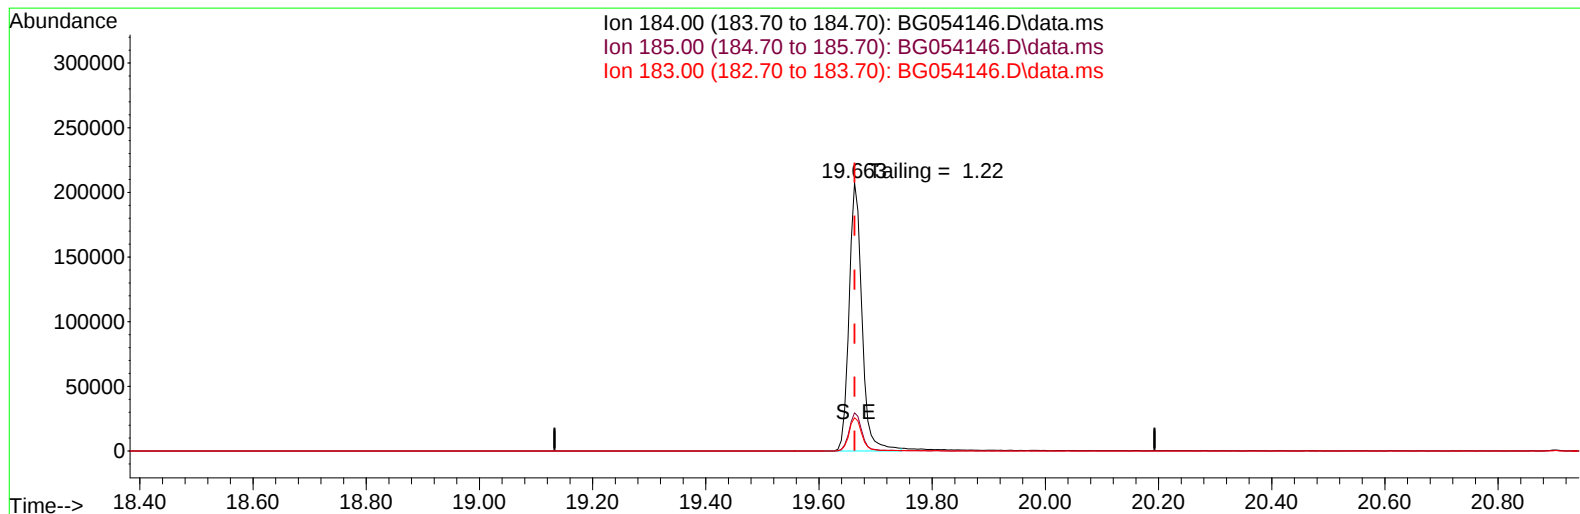

TIC: BG054146.D\data.ms

(77) Benzidine

19.663min (+ 0.000) 0.00 ng

response 334927

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.29
183.00	11.10	12.42
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/29/2022	BNA_G	<u>BG054146.D</u>
Compound Name	Response	Retention Time
DDT	192374	20.9
DDD	7167	20.45
DDE	1408	19.95
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8575	200949	4.27

Instrument :
BNA_G
ClientSampleId :
DFTPP