
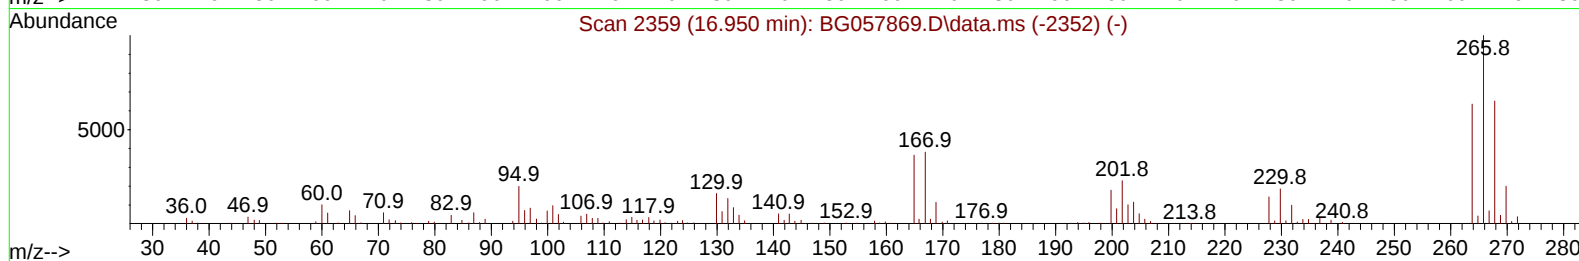
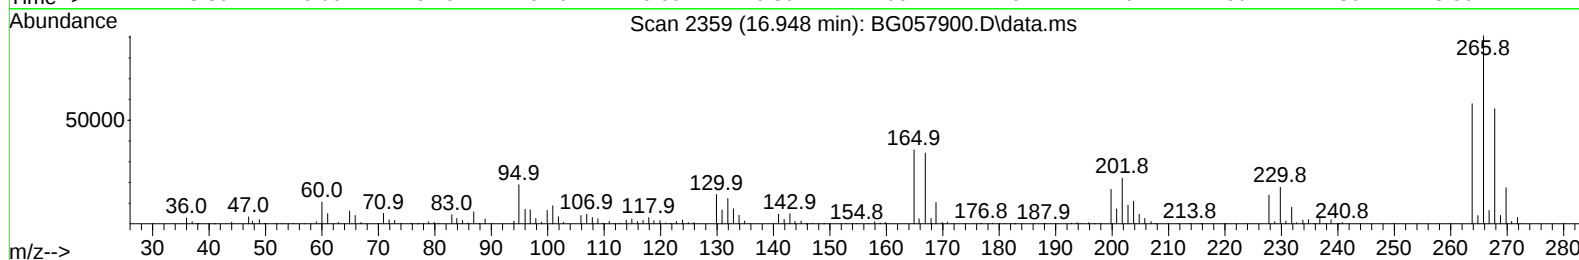


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062923\  
Data File : BG057900.D  
Acq On    : 29 Jun 2023  11:53  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Jun 29 14:25:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG062723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 28 01:12:33 2023
Response via : Initial Calibration

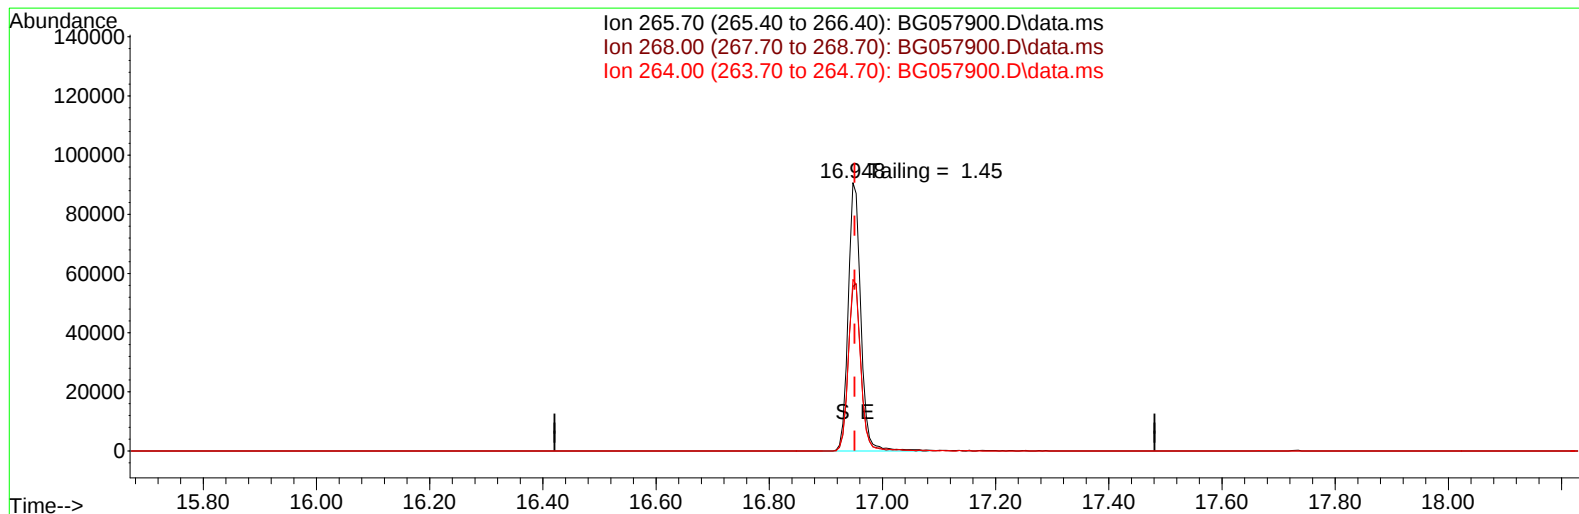

TIC: BG057900.D\data.ms

(70) Pentachlorophenol (C)




16.948min (-0.003) 6249.50 ng

response **140805**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.20	61.30
264.00	63.60	63.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062923\
Data File : BG057900.D
Acq On : 29 Jun 2023 11:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 29 14:25:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG062723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 28 01:12:33 2023
Response via : Initial Calibration

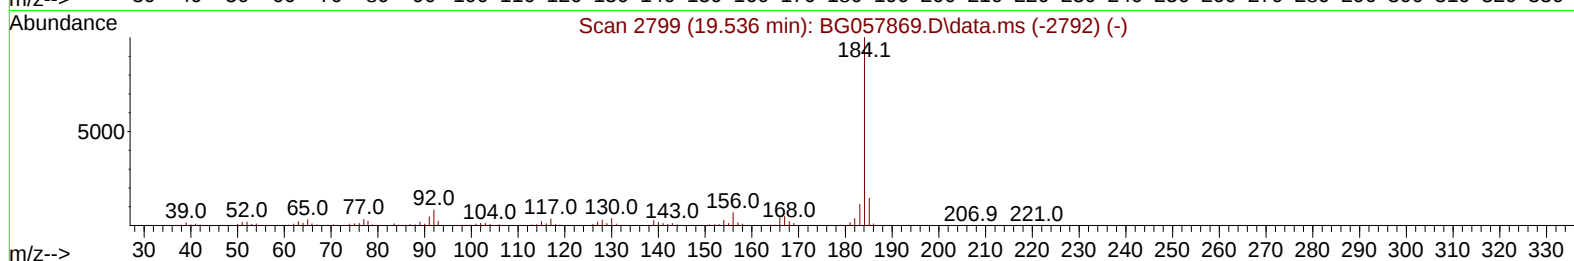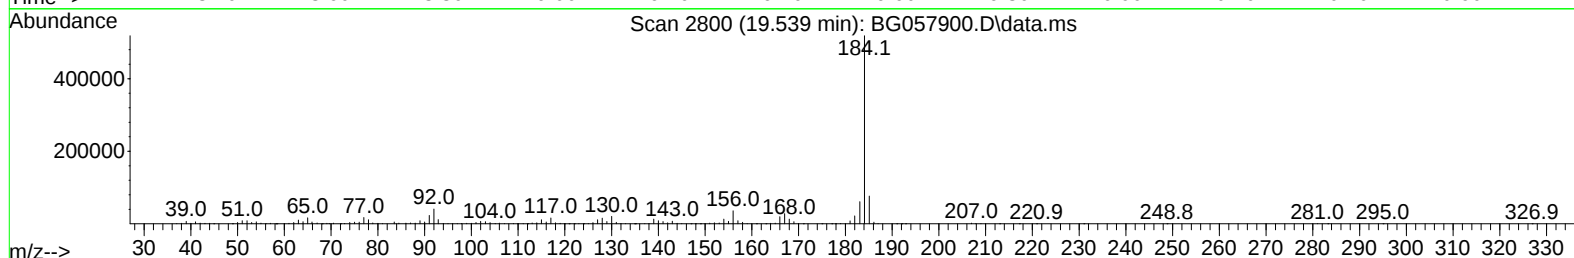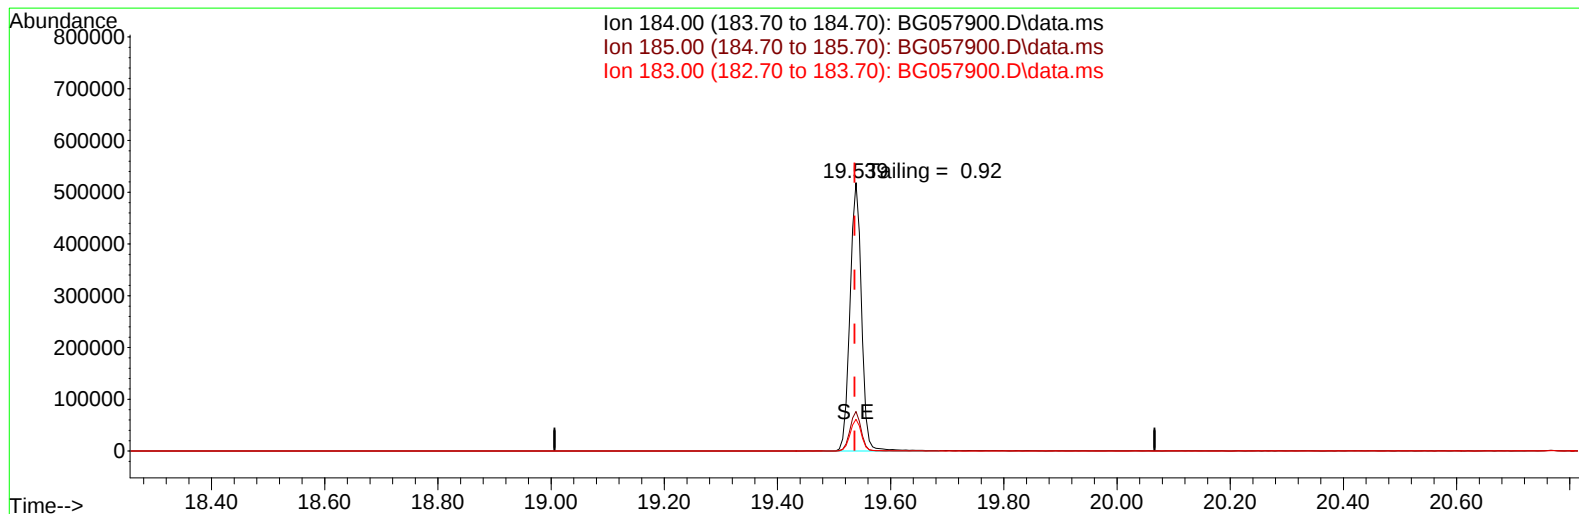

TIC: BG057900.D\data.ms

(77) Benzidine**19.539min (+ 0.003) 7564.34 ng****response 732939**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.75
183.00	11.20	11.81
0.00	0.00	0.00