

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062923\
 Data File : BG057917.D
 Acq On : 29 Jun 2023 23:44
 Operator : CG/JU
 Sample : 03403-01DL 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 ORA-1652DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG062723.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG057917.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.491	403	409	418	rBV2	78738	129919	6.21%	0.662%
2	7.084	672	680	688	rBV	76716	138720	6.63%	0.707%
3	7.912	814	821	829	rVB	210770	360930	17.24%	1.840%
4	9.075	1013	1019	1026	rBV	46745	80695	3.85%	0.411%
5	10.721	1286	1299	1305	rBV	301383	557299	26.62%	2.841%
6	10.768	1305	1307	1313	rVB	15272	22867	1.09%	0.117%
7	12.377	1576	1581	1589	rVB	14638	25603	1.22%	0.131%
8	12.595	1611	1618	1624	rBV	20019	37078	1.77%	0.189%
9	13.083	1690	1701	1707	rBV2	18923	37655	1.80%	0.192%
10	13.171	1707	1716	1722	rVV	115531	184363	8.81%	0.940%
11	13.711	1804	1808	1811	rBV4	13541	23318	1.11%	0.119%
12	13.876	1830	1836	1840	rBV2	25206	45484	2.17%	0.232%
13	13.923	1840	1844	1849	rVV2	14164	22185	1.06%	0.113%
14	14.028	1858	1862	1866	rVB2	14786	21069	1.01%	0.107%
15	14.275	1899	1904	1910	rBV2	40003	71121	3.40%	0.363%
16	14.551	1942	1951	1957	rBV	451622	706177	33.73%	3.600%
17	14.616	1957	1962	1969	rVB	96685	156506	7.48%	0.798%
18	14.763	1980	1987	1995	rBV7	12220	33227	1.59%	0.169%
19	14.857	1997	2003	2010	rVV5	12871	30006	1.43%	0.153%
20	14.945	2014	2018	2024	rVV	69854	116338	5.56%	0.593%
21	15.021	2028	2031	2035	rVB	16447	21139	1.01%	0.108%
22	15.168	2051	2056	2061	rBV5	19473	34838	1.66%	0.178%
23	15.339	2077	2085	2087	rBV7	14107	29686	1.42%	0.151%
24	15.597	2122	2129	2138	rBV2	131270	217686	10.40%	1.110%
25	15.756	2153	2156	2160	rVB3	22024	30818	1.47%	0.157%
26	15.803	2160	2164	2168	rBV3	19757	26861	1.28%	0.137%
27	15.891	2174	2179	2187	rVB2	42769	86510	4.13%	0.441%
28	16.038	2198	2204	2211	rVB3	122868	203105	9.70%	1.035%
29	16.273	2238	2244	2249	rVB3	36768	70171	3.35%	0.358%
30	16.602	2291	2300	2304	rBV4	39844	81254	3.88%	0.414%
31	16.649	2304	2308	2313	rVV3	22861	34508	1.65%	0.176%
32	16.755	2322	2326	2330	rVB3	26499	38252	1.83%	0.195%
33	16.825	2332	2338	2342	rVV3	20851	44985	2.15%	0.229%
34	16.866	2343	2345	2349	rVB4	22104	29034	1.39%	0.148%
35	16.949	2356	2359	2365	rVB4	14389	22629	1.08%	0.115%
36	17.025	2368	2372	2374	rBV2	20808	31028	1.48%	0.158%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062923\
 Data File : BG057917.D
 Acq On : 29 Jun 2023 23:44
 Operator : CG/JU
 Sample : 03403-01DL 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 ORA-1652DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG062723.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	17.113	2382	2387	2396	rVB	71105	132372	6.32%	0.675%
38	17.295	2412	2418	2422	rBV	512638	815794	38.97%	4.159%
39	17.336	2422	2425	2432	rVV	778307	1137143	54.32%	5.798%
40	17.430	2436	2441	2446	rVV	254851	372576	17.80%	1.900%
41	17.483	2446	2450	2456	rVV3	27340	53725	2.57%	0.274%
42	17.701	2483	2487	2492	rBV	36245	57535	2.75%	0.293%
43	17.818	2503	2507	2510	rBV	22110	28982	1.38%	0.148%
44	17.877	2513	2517	2524	rVB3	24240	41392	1.98%	0.211%
45	18.024	2537	2542	2548	rBV2	18016	35222	1.68%	0.180%
46	18.171	2563	2567	2571	rBV	132019	207541	9.91%	1.058%
47	18.218	2571	2575	2582	rVB	162829	246811	11.79%	1.258%
48	18.300	2584	2589	2594	rBV	77345	123376	5.89%	0.629%
49	18.370	2594	2601	2605	rBV2	272471	498408	23.81%	2.541%
50	18.670	2647	2652	2656	rBV	98112	138311	6.61%	0.705%
51	18.711	2656	2659	2665	rVB3	31821	48461	2.31%	0.247%
52	18.917	2691	2694	2698	rVB2	30616	38204	1.82%	0.195%
53	18.964	2699	2702	2705	rBV	30347	36834	1.76%	0.188%
54	19.087	2718	2723	2729	rBV	101297	186416	8.90%	0.950%
55	19.228	2743	2747	2756	rBV4	47992	117420	5.61%	0.599%
56	19.352	2762	2768	2774	rBV	1472900	2093436	100.00%	10.673%
57	19.446	2782	2784	2788	rVB2	38499	39996	1.91%	0.204%
58	19.681	2819	2824	2825	rBV	245338	295960	14.14%	1.509%
59	19.716	2825	2830	2838	rVV	1295772	2007598	95.90%	10.235%
60	19.786	2838	2842	2847	rVB2	73094	123252	5.89%	0.628%
61	19.910	2856	2863	2867	rBV2	169644	283965	13.56%	1.448%
62	20.033	2880	2884	2891	rVB4	84630	188462	9.00%	0.961%
63	20.204	2909	2913	2918	rVB	261546	376953	18.01%	1.922%
64	20.303	2926	2930	2934	rBV	233618	282523	13.50%	1.440%
65	20.503	2961	2964	2967	rBV	63175	71521	3.42%	0.365%
66	20.544	2969	2971	2975	rVB	81079	90051	4.30%	0.459%
67	21.179	3077	3079	3083	rBV	74529	82207	3.93%	0.419%
68	21.537	3134	3140	3146	rBV2	751647	1828673	87.35%	9.323%
69	21.596	3146	3150	3161	rVB	533280	921848	44.04%	4.700%
70	21.743	3171	3175	3181	rVB2	169310	255738	12.22%	1.304%
71	23.705	3503	3509	3516	rBV	325874	977078	46.67%	4.981%
72	24.557	3647	3654	3669	rVB	332374	966746	46.18%	4.929%
73	24.704	3673	3679	3687	rVV2	231976	608724	29.08%	3.103%


Sum of corrected areas: 19614318

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062923\
Data File : BG057917.D
Acq On : 29 Jun 2023 23:44
Operator : CG/JU
Sample : 03403-01DL 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
ORA-1652DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG062723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

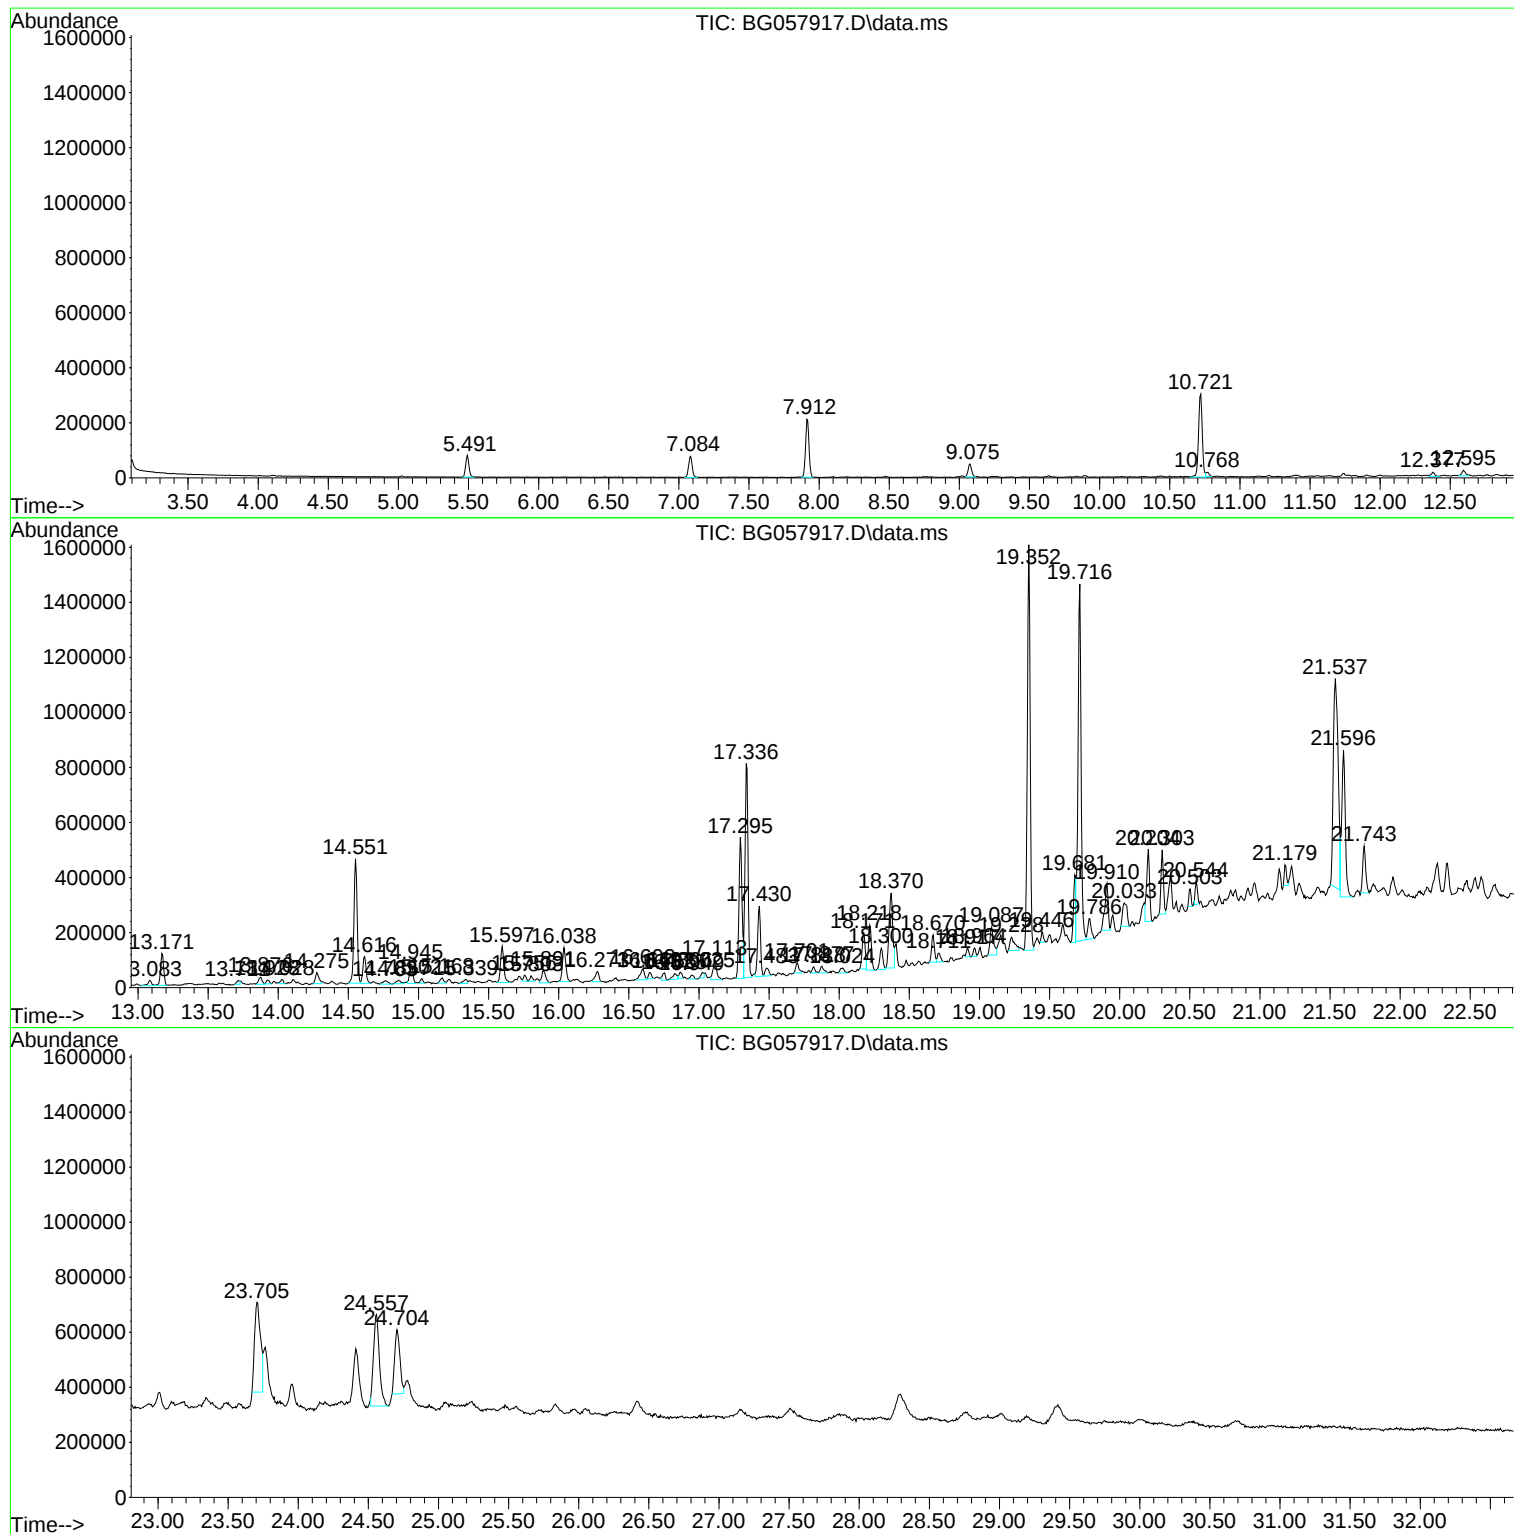

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062923\
Data File : BG057917.D
Acq On : 29 Jun 2023 23:44
Operator : CG/JU
Sample : 03403-01DL 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
ORA-1652DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG062723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062923\
Data File : BG057917.D
Acq On : 29 Jun 2023 23:44
Operator : CG/JU
Sample : 03403-01DL 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
ORA-1652DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG062723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------