


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062923\
Data File : BG057900.D
Acq On : 29 Jun 2023 11:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG062723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jun 28 01:12:33 2023

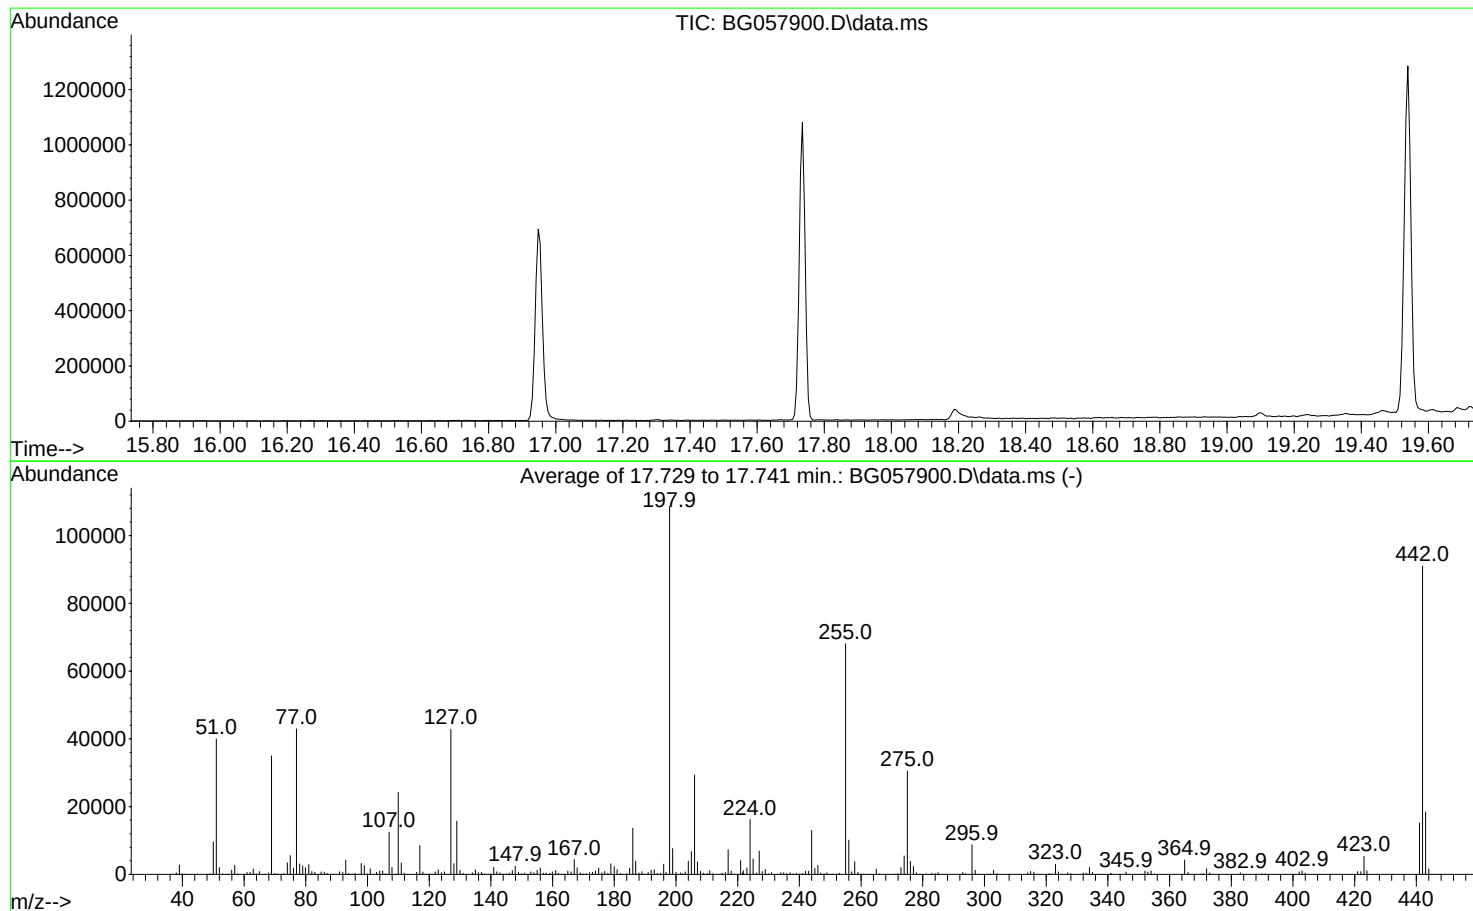

AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	39949	PASS
68	69	0.00	2	1.2	417	PASS
69	198	0.00	100	32.2	34965	PASS
70	69	0.00	2	0.8	292	PASS
127	198	10	80	39.4	42803	PASS
197	198	0.00	2	0.5	556	PASS
198	198	100	100	100.0	108589	PASS
199	198	5	9	7.0	7600	PASS
275	198	10	60	28.1	30509	PASS
365	198	1	100	3.9	4246	PASS
441	198	0.01	100	14.0	15169	PASS
442	442	50	100	100.0	91035	PASS
443	442	15	24	20.2	18405	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/29/2023	BNA_G	<u>BG057900.D</u>
Compound Name	Response	Retention Time
DDT	322028	20.767
DDD	13625	20.326
DDE	428	19.815
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14053	336081	4.18

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062923\
Data File : BG057900.D
Acq On : 29 Jun 2023 11:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 29 14:25:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG062723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 28 01:12:33 2023
Response via : Initial Calibration

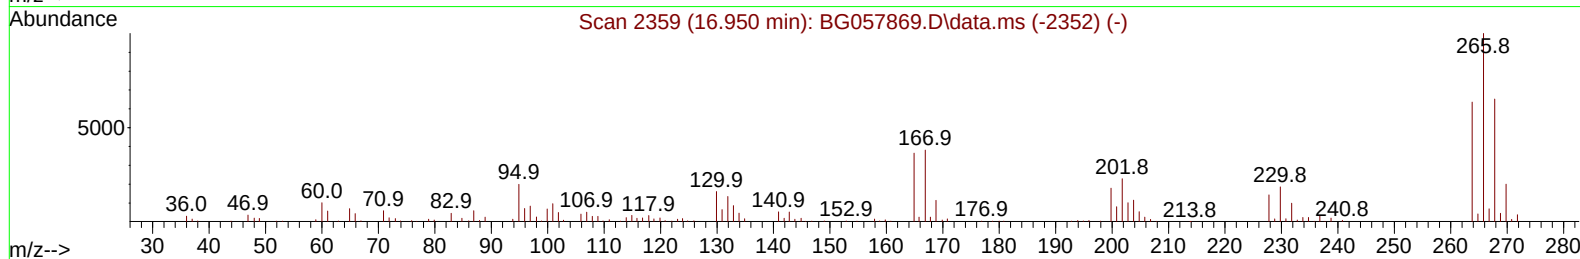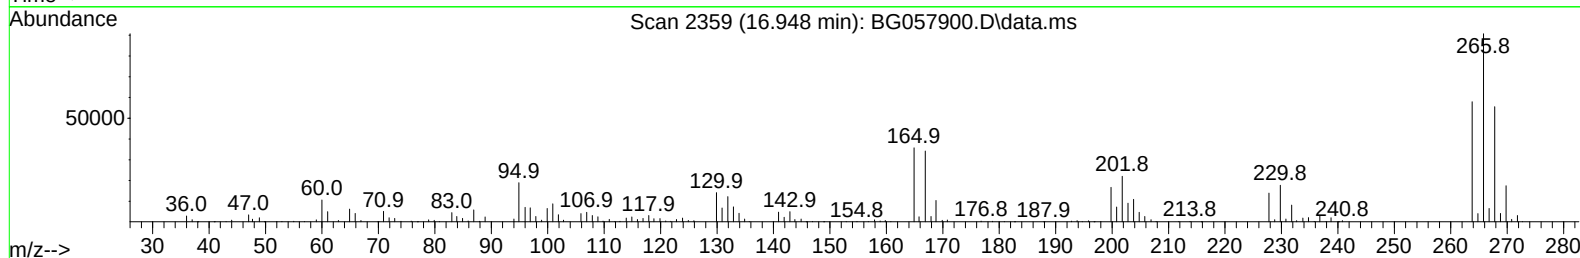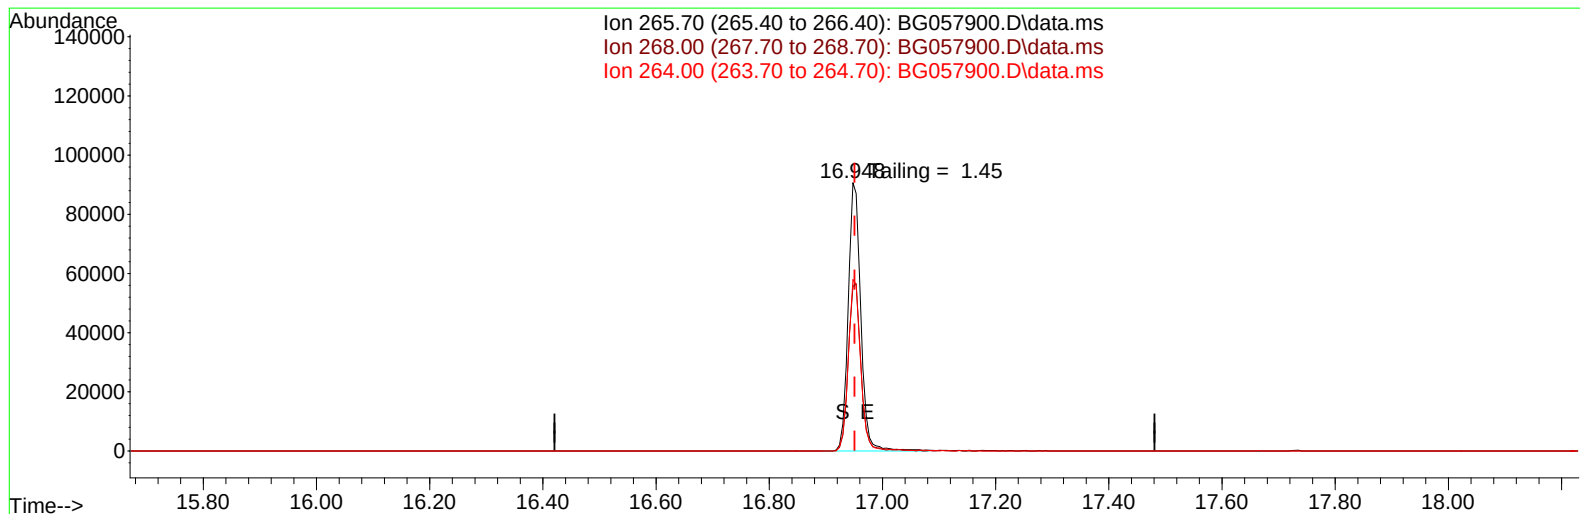

TIC: BG057900.D\data.ms

(70) Pentachlorophenol (C)

16.948min (-0.003) 6249.50 ng




response 140805

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.20	61.30
264.00	63.60	63.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062923\
Data File : BG057900.D
Acq On : 29 Jun 2023 11:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 29 14:25:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG062723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 28 01:12:33 2023
Response via : Initial Calibration

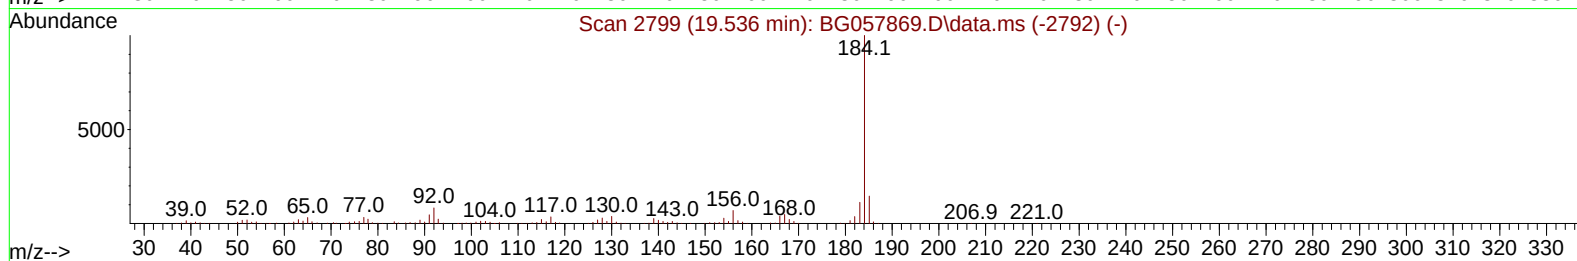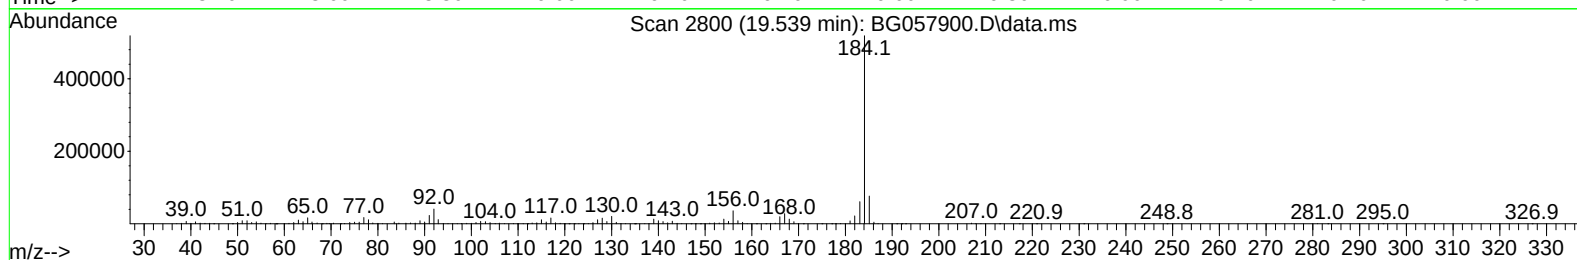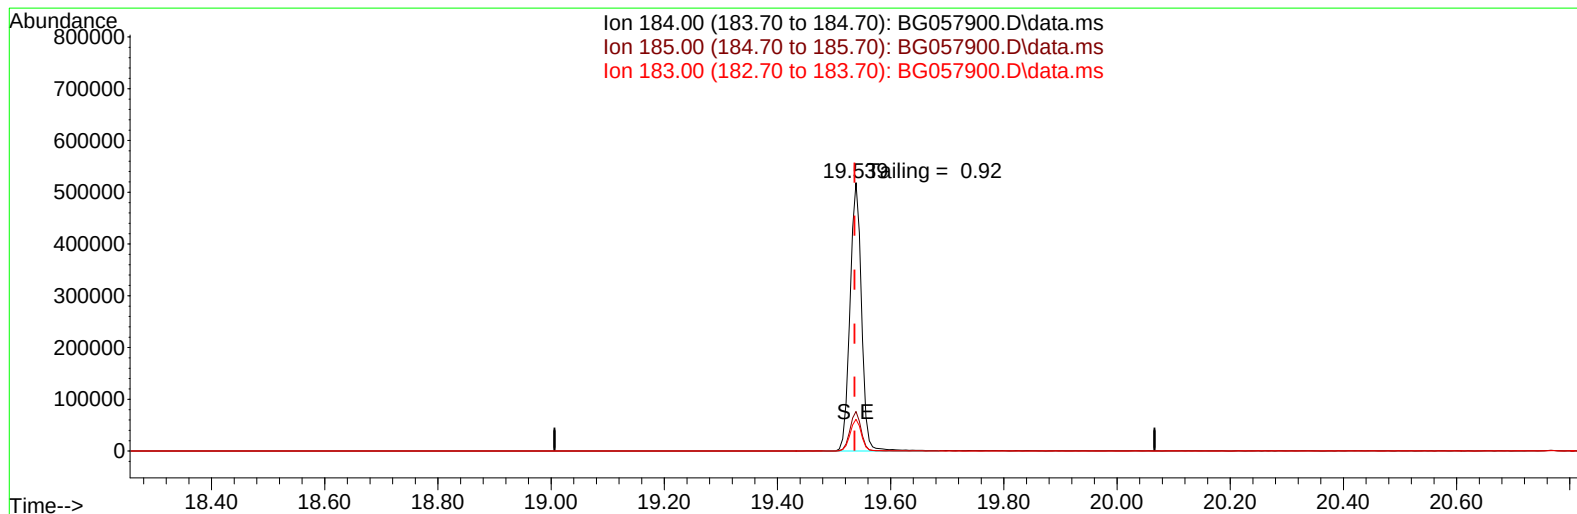

TIC: BG057900.D\data.ms

(77) Benzidine

19.539min (+ 0.003) 7564.34 ng

response 732939

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.75
183.00	11.20	11.81
0.00	0.00	0.00