
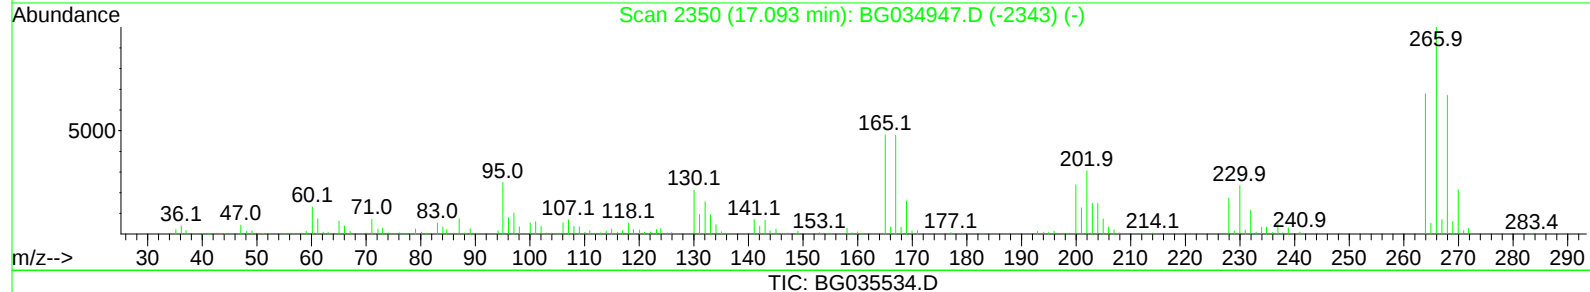
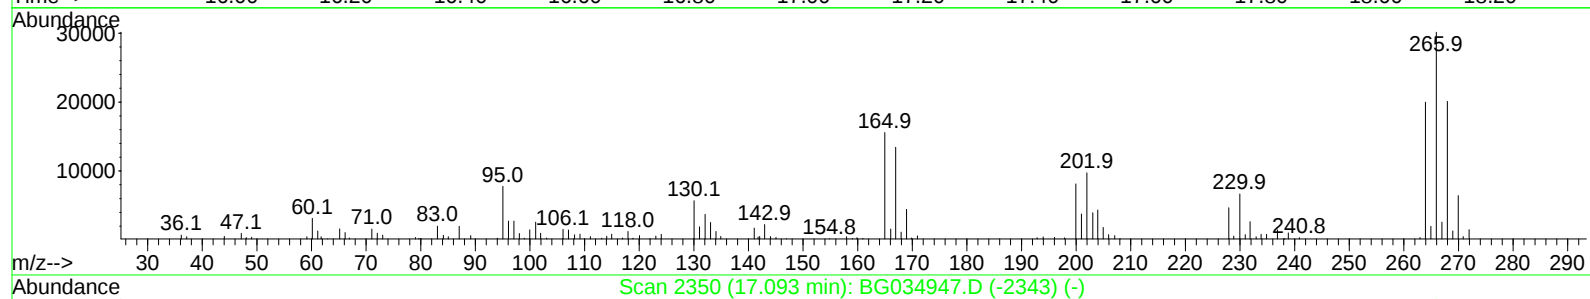


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG063018\
Data File : BG035534.D
Acq On : 30 Jun 2018 9:42
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 02 08:10:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

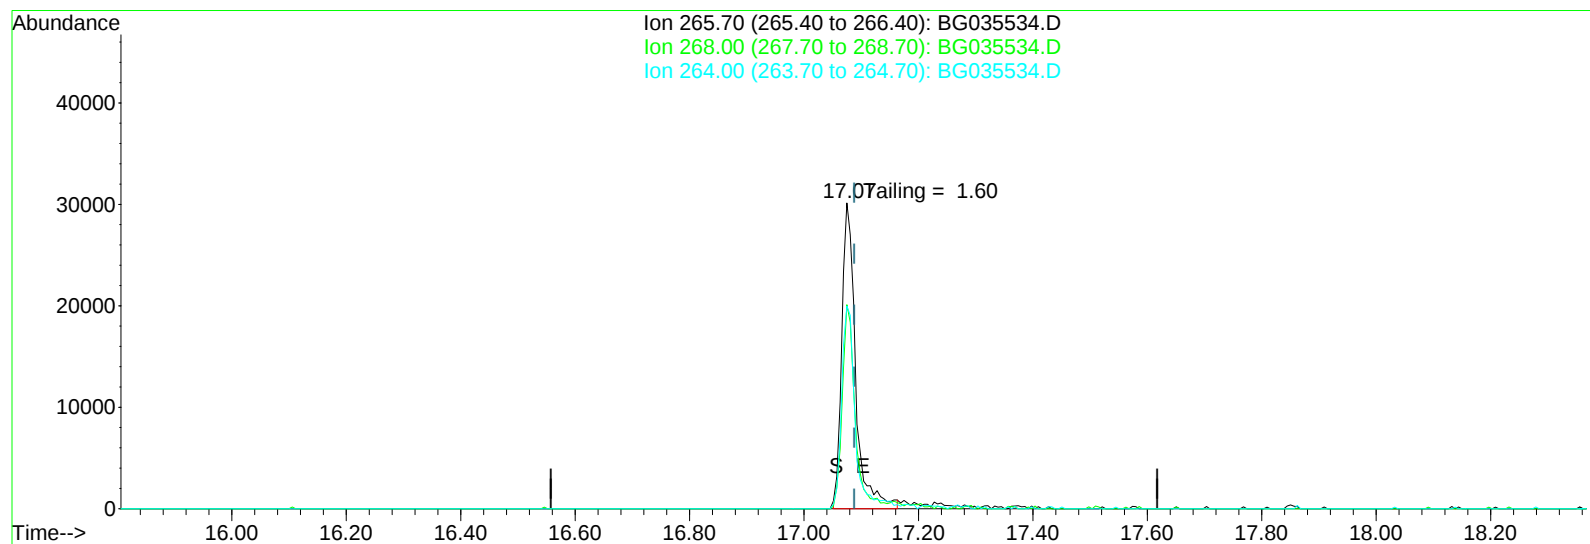

(69) Pentachlorophenol (C)




17.075min (-0.013) 47812.91ng

response 50442

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.69
264.00	62.00	66.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG063018\
Data File : BG035534.D
Acq On : 30 Jun 2018 9:42
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 02 08:10:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

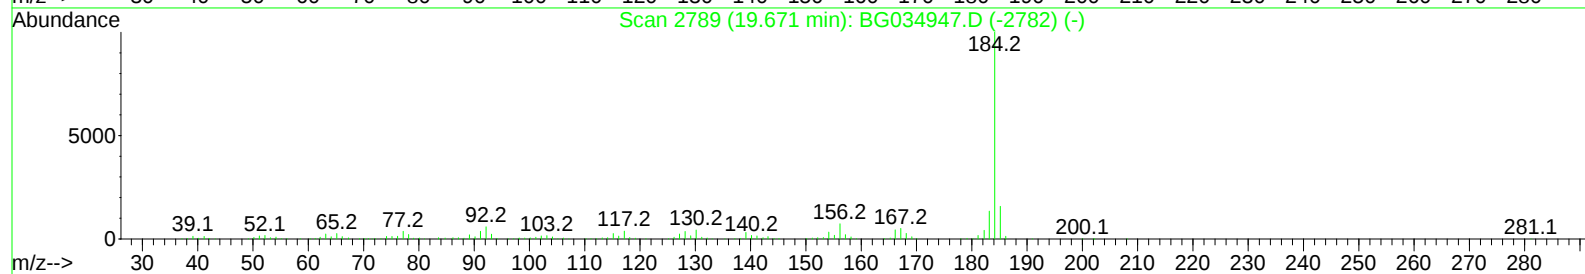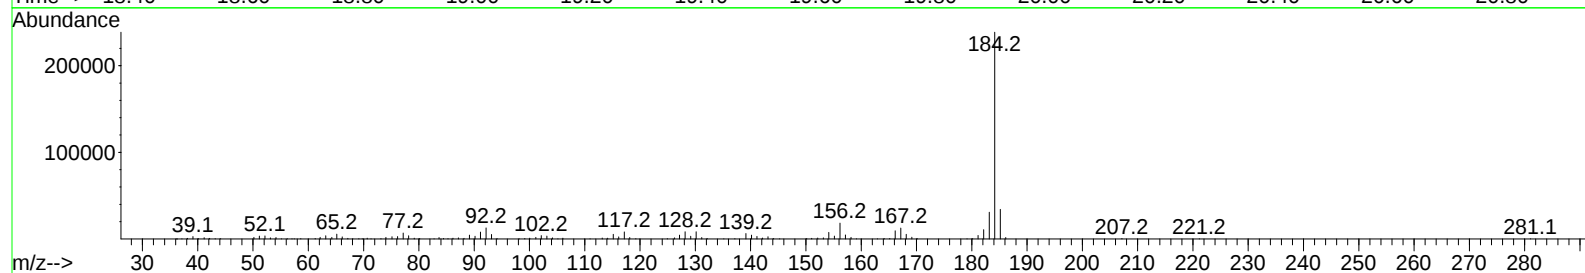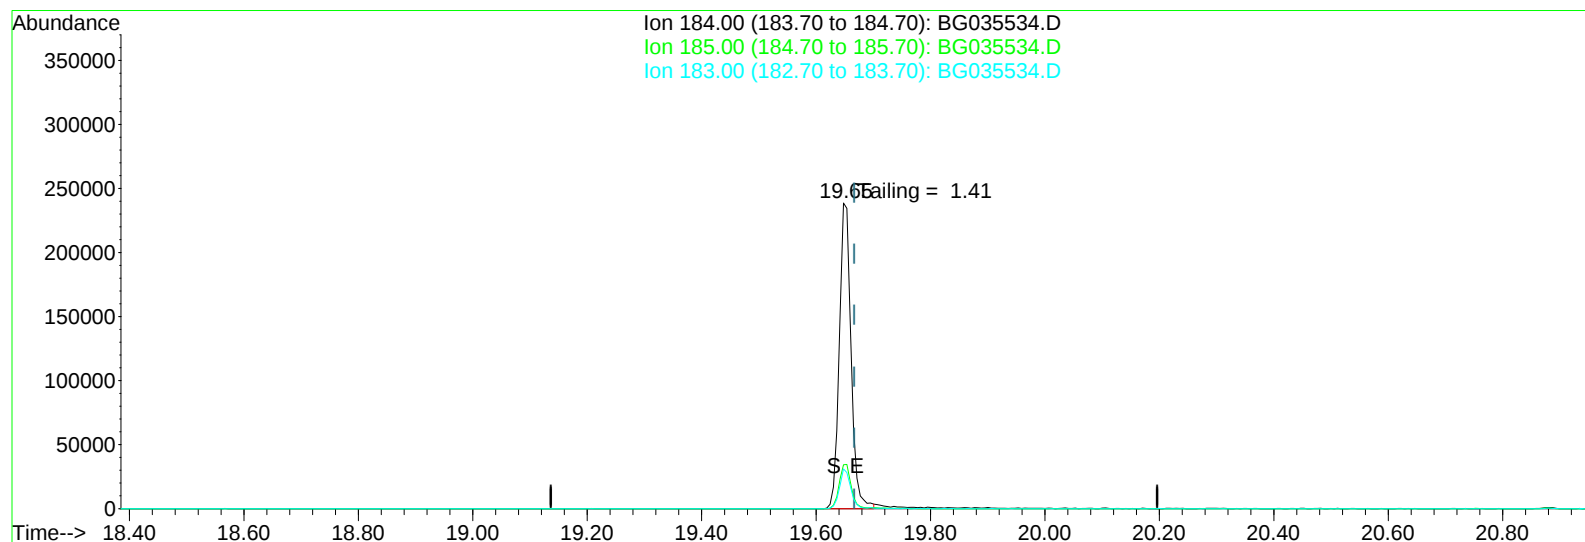

TIC: BG035534.D

(76) Benzidine

19.648min (-0.018) 0.00ng

response 344833

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.37
183.00	13.30	12.98
0.00	0.00	0.00