

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG063018\
 Data File : BG035540.D
 Acq On : 30 Jun 2018 13:34
 Operator : JU/SJ
 Sample : J3757-07
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 062618-TIPC-E-D-M

Quant Time: Jul 02 03:08:14 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 08 17:16:28 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.06	152	31373	20.00	ng	-0.01
21) Naphthalene-d8	10.87	136	121260	20.00	ng	-0.02
38) Acenaphthene-d10	14.68	164	88218	20.00	ng	-0.02
63) Phenanthrene-d10	17.42	188	251766	20.00	ng	-0.02
75) Chrysene-d12	21.69	240	271941	20.00	ng	-0.03
86) Perylene-d12	24.91	264	258569	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.64	112	74136	39.88	ng	0.00
7) Phenol-d6	7.22	99	68185	24.85	ng	0.00
23) Nitrobenzene-d5	9.22	82	250452	98.18	ng	-0.02
41) 2,4,6-Tribromophenol	16.17	330	115609	102.37	ng	-0.01
44) 2-Fluorobiphenyl	13.30	172	614777	90.59	ng	-0.02
78) Terphenyl-d14	20.03	244	1089132	83.89	ng	-0.02
Target Compounds						
10) Phenol	7.25	94	7619	2.683	ng	96
49) Dimethylphthalate	14.13	163	68651	8.924	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG063018\
Data File : BG035540.D
Acq On : 30 Jun 2018 13:34
Operator : JU/SJ
Sample : J3757-07
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
062618-TIPC-E-D-M

Quant Time: Jul 02 03:08:14 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

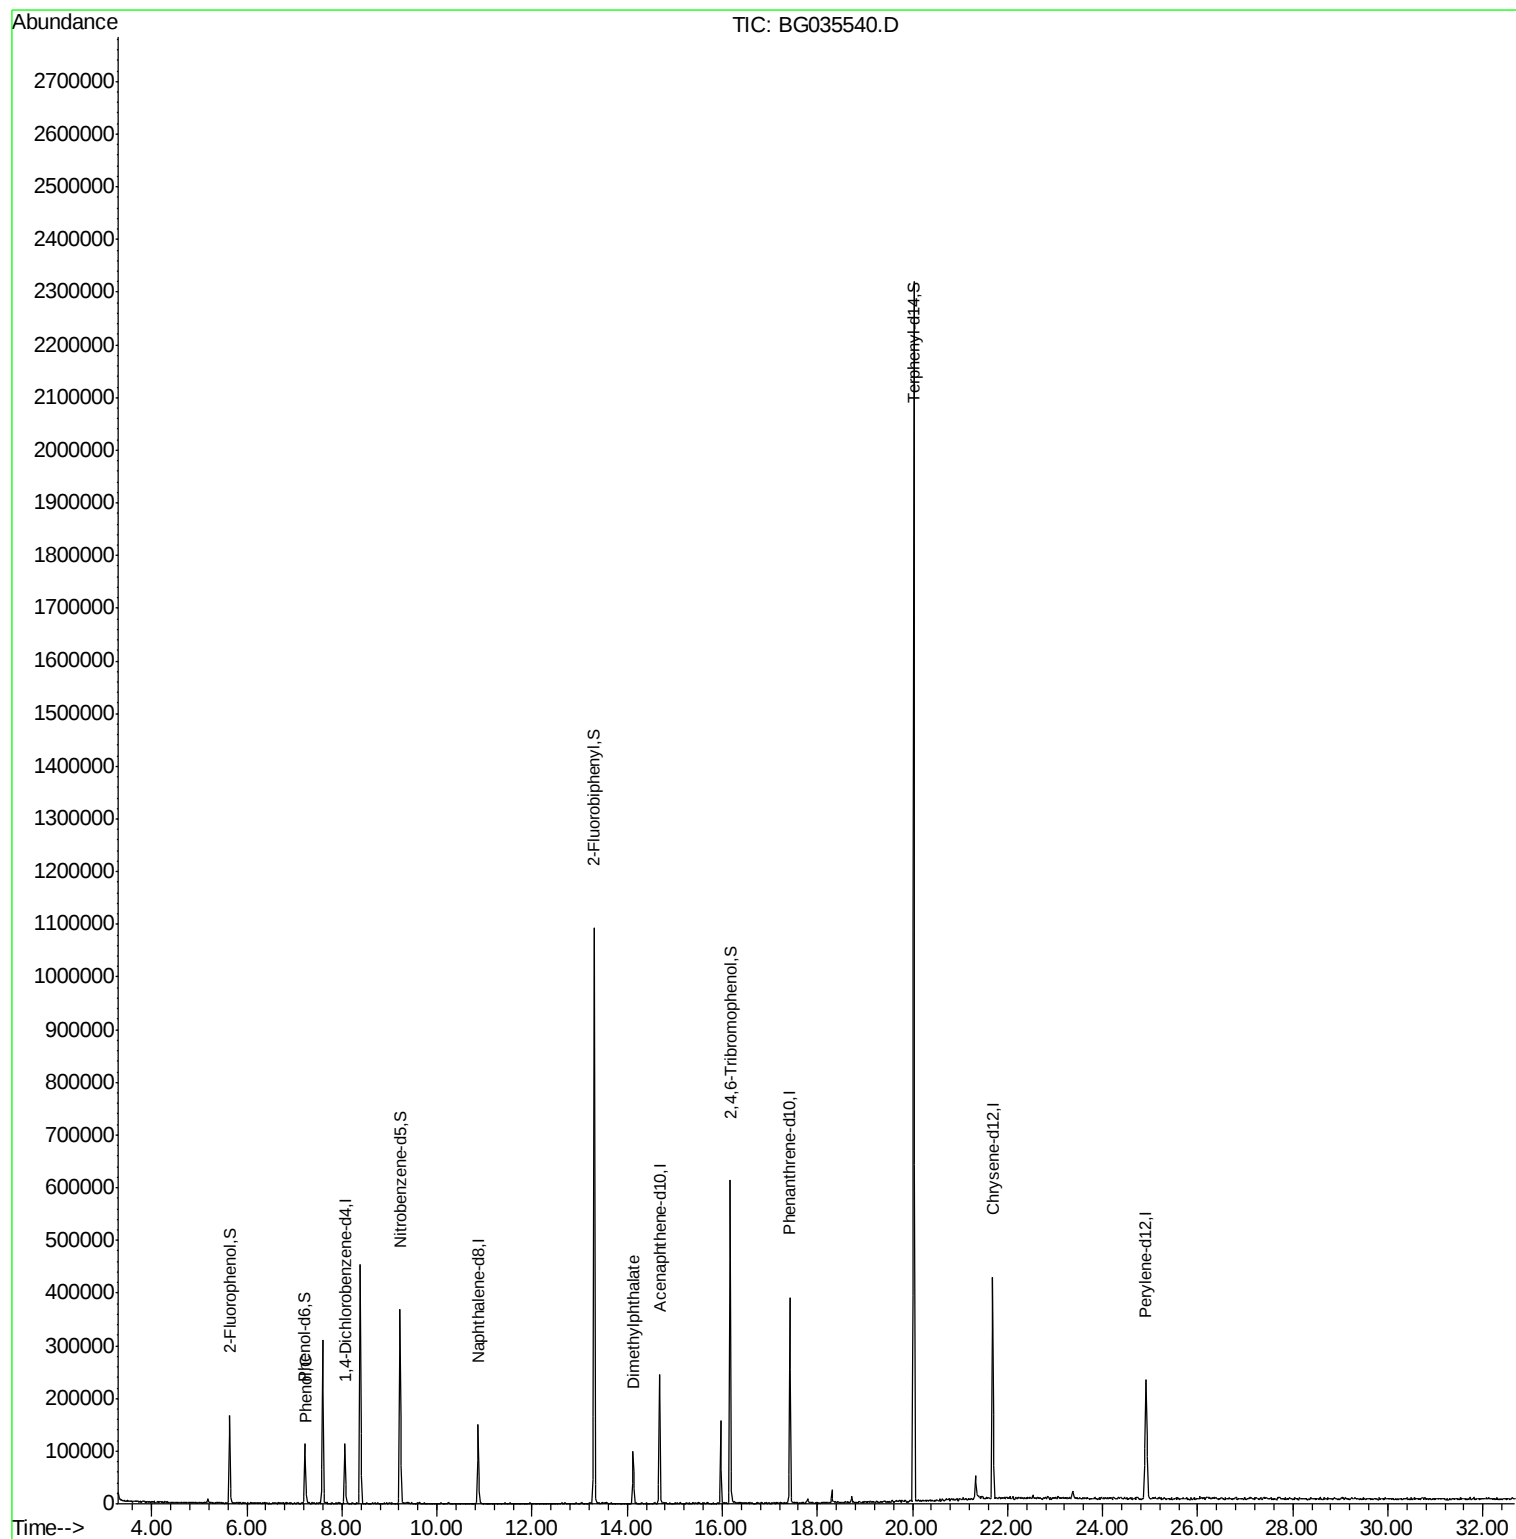




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.06 min Scan# 813
Delta R.T. -0.01 min
Lab File: BG035540.D
Acq: 30 Jun 2018 13:34

Instrument :
BNA_G
ClientSampleId :
062618-TIPC-E-D-M

Tot Ion:152 Resp: 31373
Ion Ratio Lower Upper
152 100
150 151.3 126.6 189.8
115 66.6 53.0 79.4




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

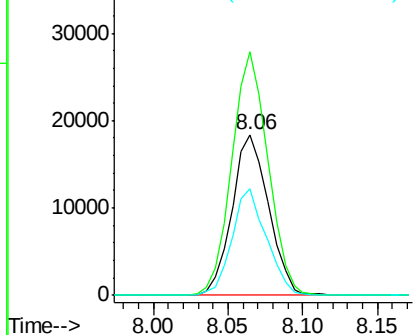



#5


2-Fluorophenol
Concen: 39.879 ng
RT: 5.64 min Scan# 400
Delta R.T. -0.01 min
Lab File: BG035540.D
Acq: 30 Jun 2018 13:34

Tgt Ion:112 Resp: 74136
Ion Ratio Lower Upper
112 100
64 67.5 56.3 84.5
63 34.0 30.1 45.1



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

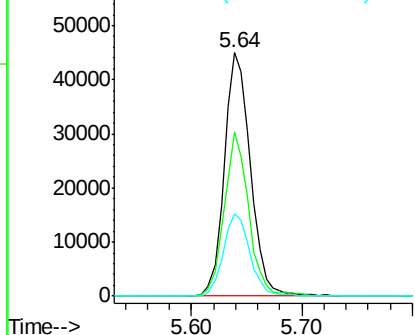

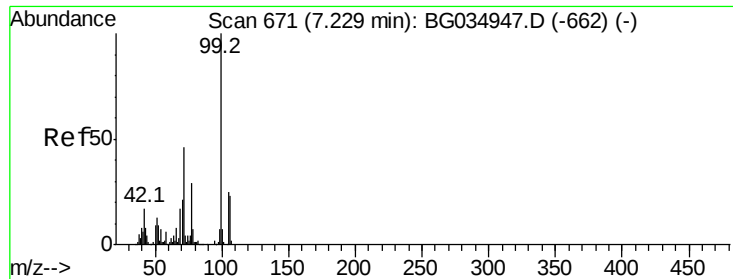

#7

Phenol-d6

Concen: 24.851 ng

RT: 7.22 min Scan# 670

Delta R.T. 0.00 min

Lab File: BG035540.D

Acq: 30 Jun 2018 13:34

Instrument :

BNA_G

ClientSampleId :

062618-TIPC-E-D-M


Tot Ion: 99 Resp: 68185

Ion Ratio Lower Upper




99 100

42 14.9 14.1 21.1

71 41.1 26.1 39.1#

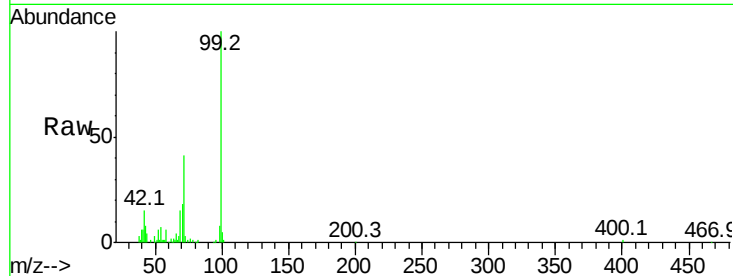

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

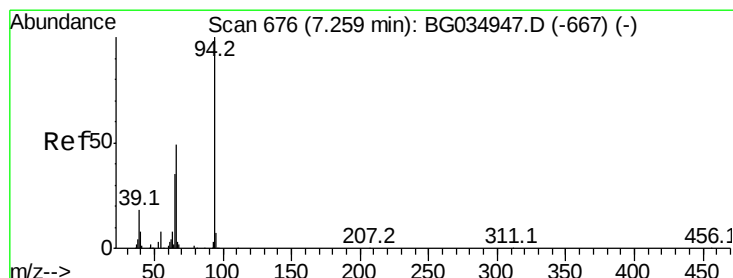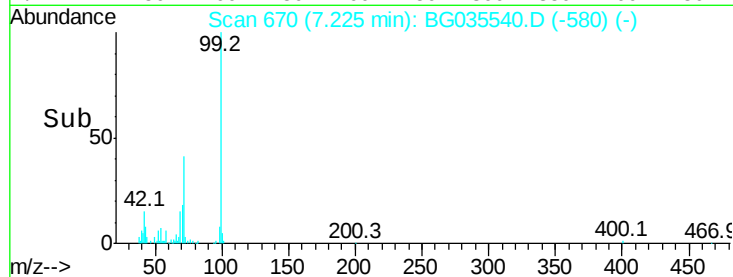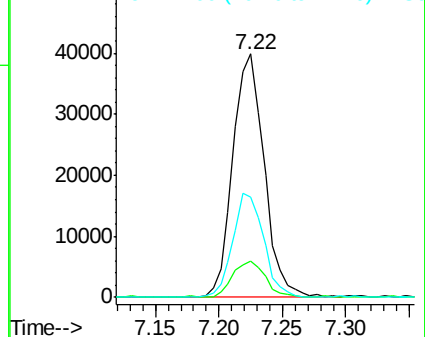

#10

Phenol

Concen: 2.683 ng

RT: 7.25 min Scan# 674

Delta R.T. -0.01 min

Lab File: BG035540.D

Acq: 30 Jun 2018 13:34


Tgt Ion: 94 Resp: 7619

Ion Ratio Lower Upper



94 100


65 28.6 11.9 51.9

66 44.0 22.2 62.2

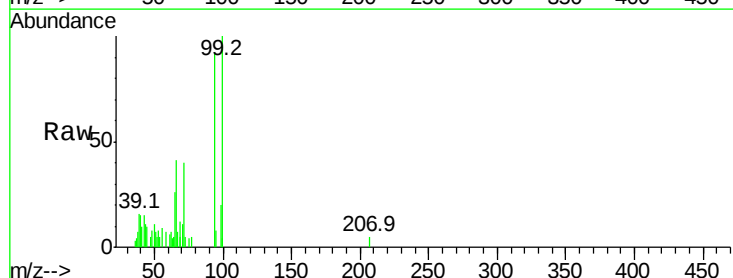

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC



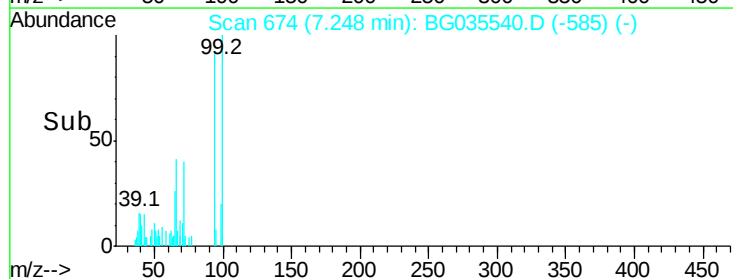
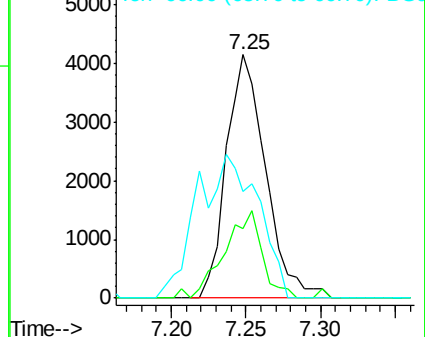


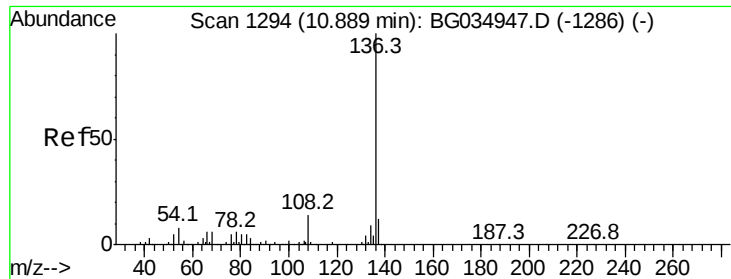

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.87 min Scan# 1290
Delta R.T. -0.02 min
Lab File: BG035540.D
Acq: 30 Jun 2018 13:34




Instrument :
BNA_G
ClientSampleId :
062618-TIPC-E-D-M


Tot Ion:	136	Resp:	121260
Ion	Ratio	Lower	Upper
136	100		
137	11.5	9.2	13.8
54	6.3	10.3	15.5#
68	4.9	4.5	6.7

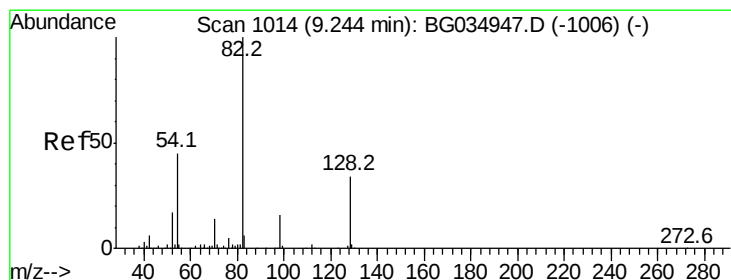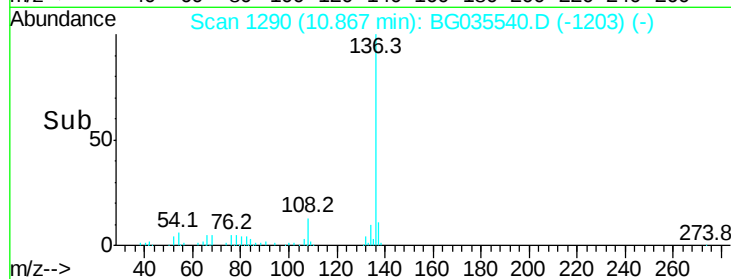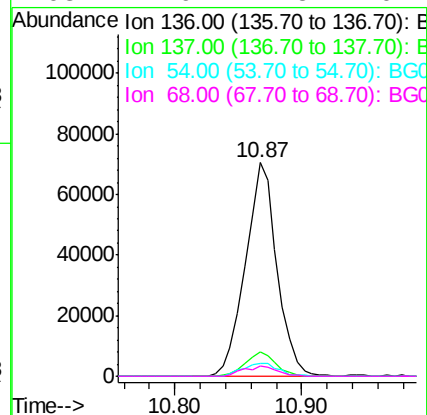

#23
Nitrobenzene-d5
Concen: 98.178 ng
RT: 9.22 min Scan# 1010
Delta R.T. -0.02 min
Lab File: BG035540.D
Acq: 30 Jun 2018 13:34

Tgt Ion:	82	Resp:	250452
Ion	Ratio	Lower	Upper
82	100		
128	32.6	29.7	44.5
54	42.4	43.1	64.7#

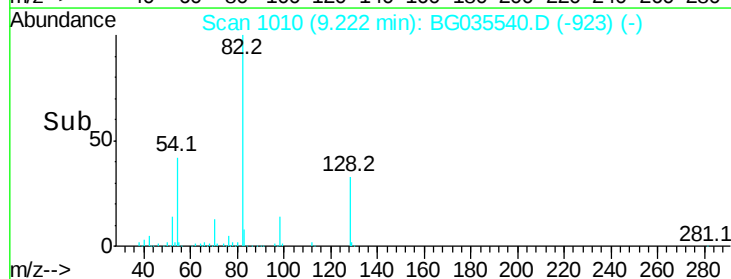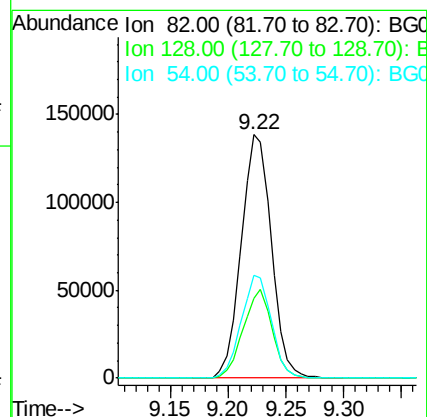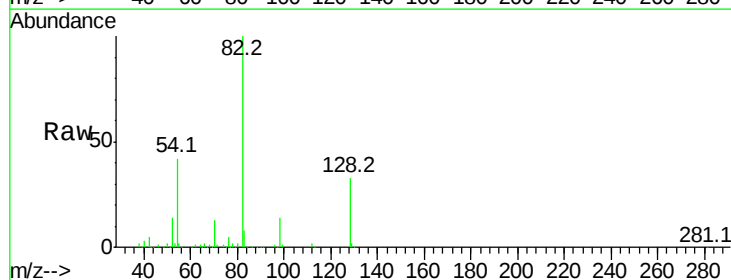

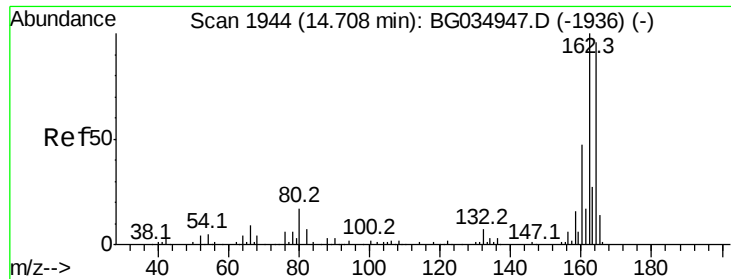

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.68 min Scan# 1939

Delta R.T. -0.02 min

Lab File: BG035540.D

Acq: 30 Jun 2018 13:34

Instrument :

BNA_G

ClientSampleId :

062618-TIPC-E-D-M


Tot Ion:164 Resp: 88218

Ion Ratio Lower Upper

164 100

162 104.8 78.8 118.2




160 45.4 35.4 53.0

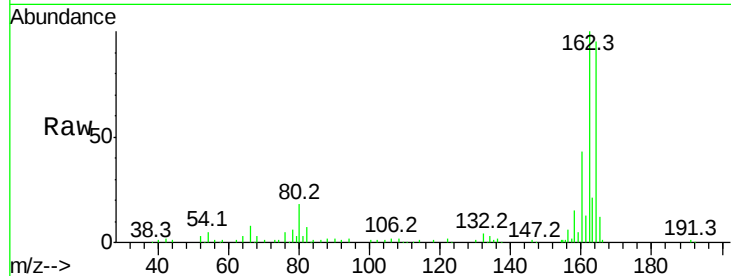

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

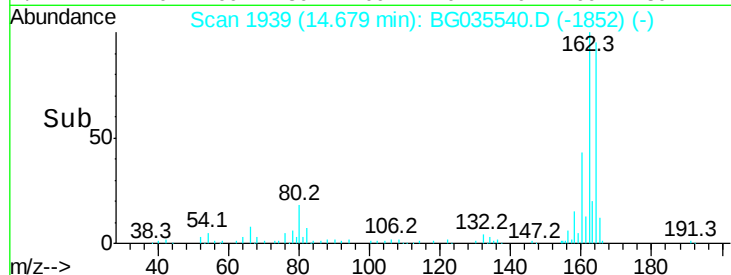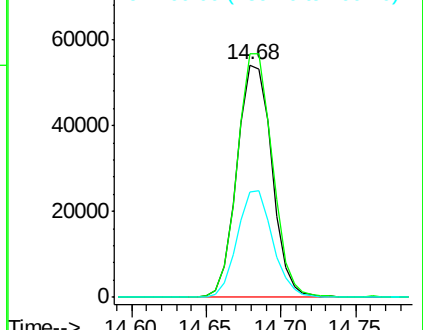

#41

2,4,6-Tribromophenol

Concen: 102.372 ng

RT: 16.17 min Scan# 2193

Delta R.T. -0.01 min

Lab File: BG035540.D

Acq: 30 Jun 2018 13:34


Tgt Ion:330 Resp: 115609

Ion Ratio Lower Upper

330 100

332 96.0 77.0 115.6



141 37.6 25.2 37.8




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E




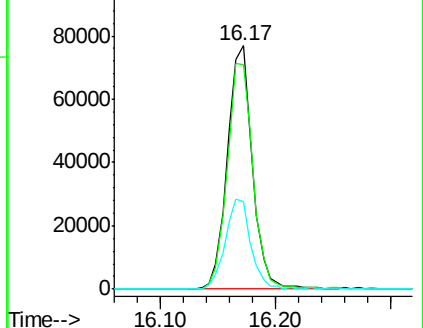




#44
2-Fluorobiphenyl
Concen: 90.595 ng
RT: 13.30 min Scan# 1705
Delta R.T. -0.02 min
Lab File: BG035540.D
Acq: 30 Jun 2018 13:34




Instrument :
BNA_G
ClientSampleId :
062618-TIPC-E-D-M


Tot Ion:172 Resp: 614777
Ion Ratio Lower Upper
172 100
171 33.5 30.0 45.0
170 23.3 19.5 29.3

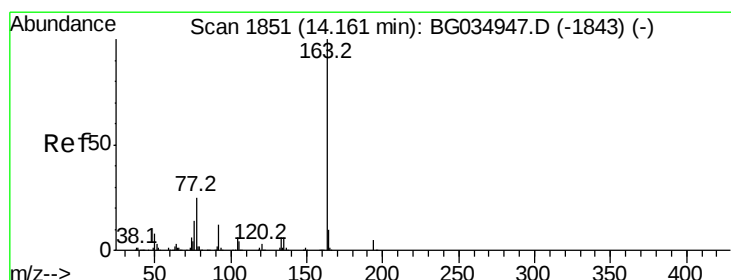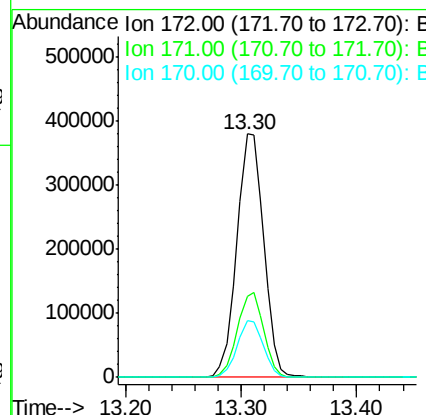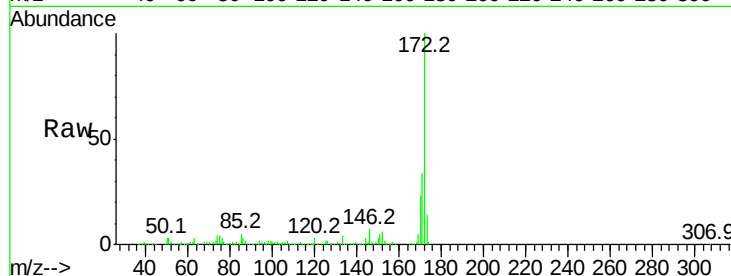

#49
Dimethylphthalate
Concen: 8.924 ng
RT: 14.13 min Scan# 1845
Delta R.T. -0.03 min
Lab File: BG035540.D
Acq: 30 Jun 2018 13:34

Tgt Ion:163 Resp: 68651
Ion Ratio Lower Upper
163 100
194 4.4 3.4 5.2
164 10.8 8.2 12.4

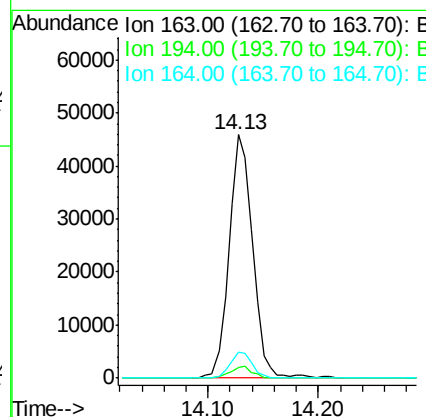



#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.42 min Scan# 2406

Delta R.T. -0.02 min

Lab File: BG035540.D

Acq: 30 Jun 2018 13:34

Instrument :

BNA_G

ClientSampleId :

062618-TIPC-E-D-M


Tot Ion:188 Resp: 251766

Ion Ratio Lower Upper

188 100

94 6.3 6.9 10.3#




80 7.9 7.7 11.5

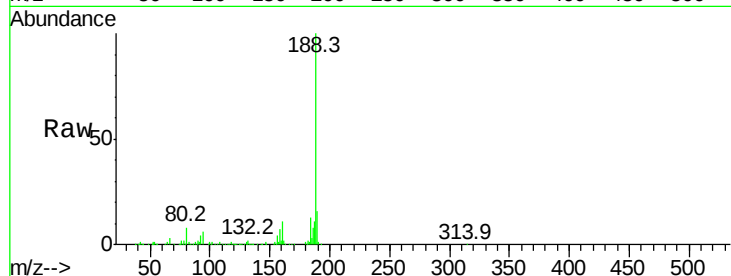

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

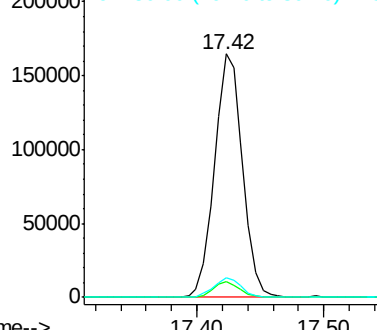

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.69 min Scan# 3132

Delta R.T. -0.03 min

Lab File: BG035540.D

Acq: 30 Jun 2018 13:34


Tgt Ion:240 Resp: 271941

Ion Ratio Lower Upper

240 100

120 4.6 6.8 10.2#



236 24.8 20.9 31.3




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

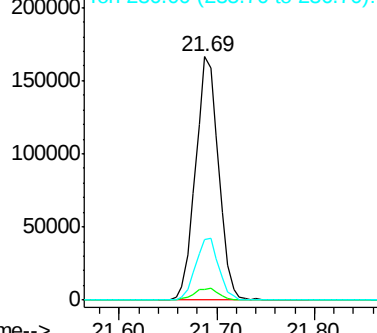

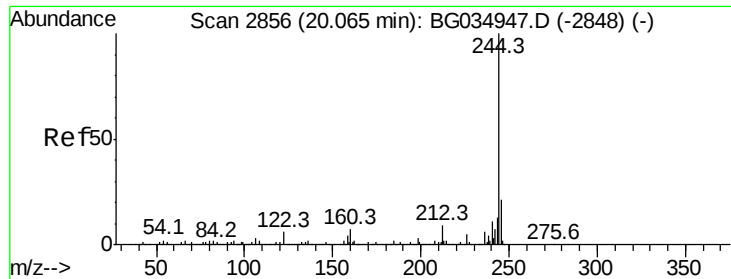

#78

Terphenyl-d14

Concen: 83.892 ng

RT: 20.03 min Scan# 2850

Delta R.T. -0.02 min

Lab File: BG035540.D

Acq: 30 Jun 2018 13:34

Instrument :

BNA_G

ClientSampleId :

062618-TIPC-E-D-M


Tot Ion:244 Resp: 1089132

Ion Ratio Lower Upper

244 100

212 8.9 5.8 8.8#




122 6.8 7.0 10.4#



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

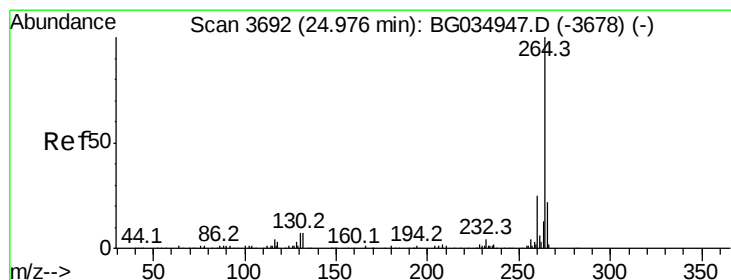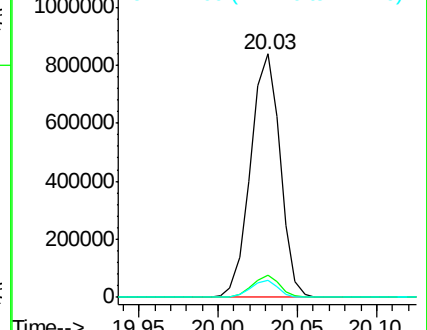

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.91 min Scan# 3681

Delta R.T. -0.04 min

Lab File: BG035540.D

Acq: 30 Jun 2018 13:34


Tgt Ion:264 Resp: 258569

Ion Ratio Lower Upper

264 100

260 24.2 17.4 26.0

265 21.1 17.7 26.5



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

