


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG063018\
 Data File : BG035534.D
 Acq On : 30 Jun 2018 9:42
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG060718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 08 17:16:28 2018

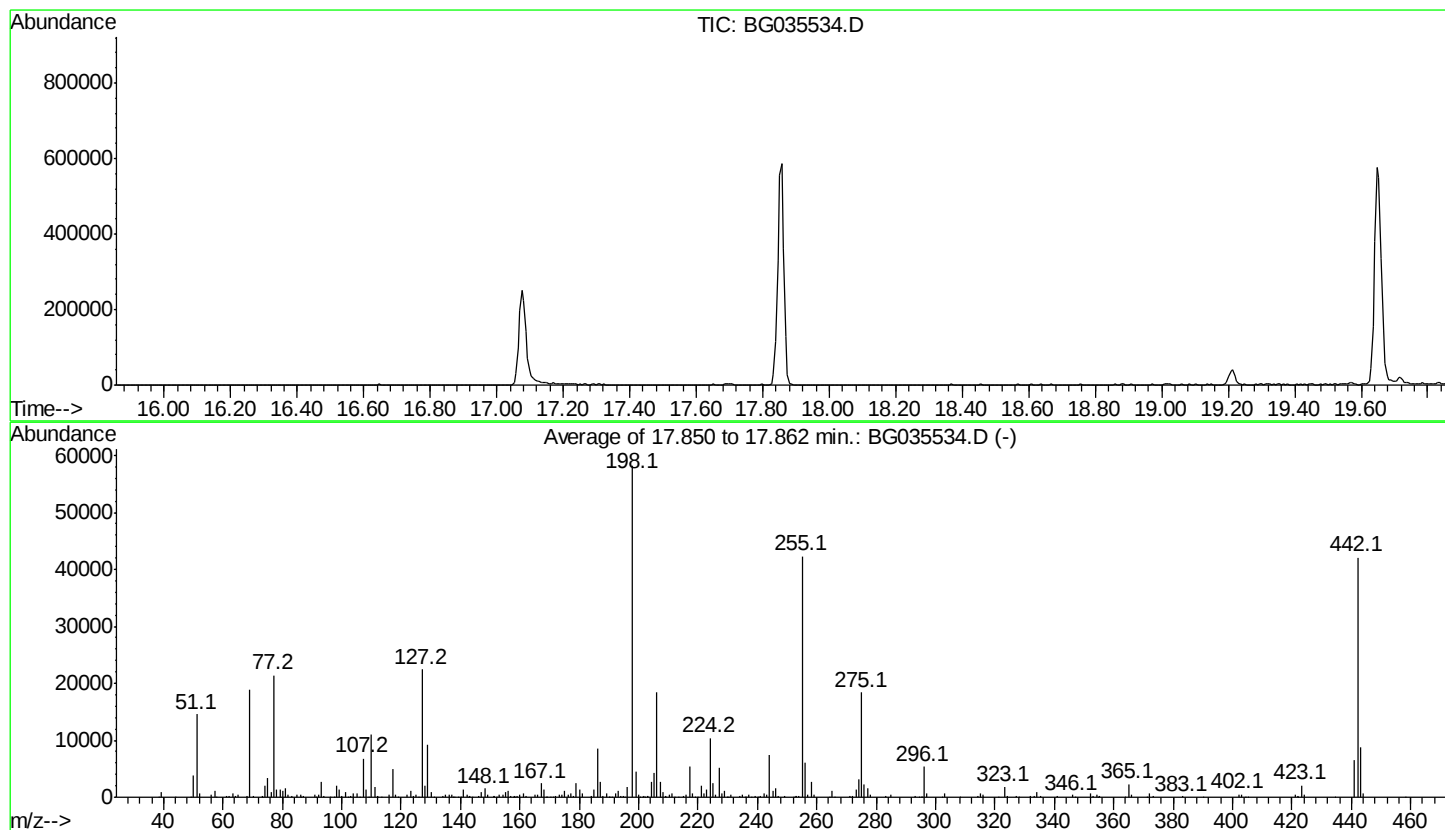

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.0	14551	PASS
68	69	0.00	2	1.2	229	PASS
69	198	0.00	100	32.4	18880	PASS
70	69	0.00	2	0.7	140	PASS
127	198	10	80	38.5	22422	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	58226	PASS
199	198	5	9	7.5	4393	PASS
275	198	10	60	31.6	18412	PASS
365	198	1	100	4.0	2300	PASS
441	443	0.01	100	74.6	6522	PASS
442	198	50	100	72.3	42096	PASS
443	442	15	24	20.8	8744	PASS