
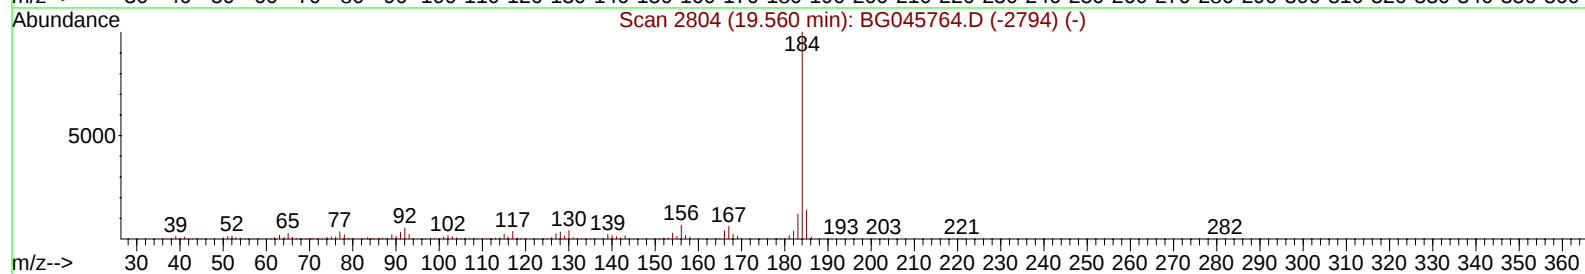
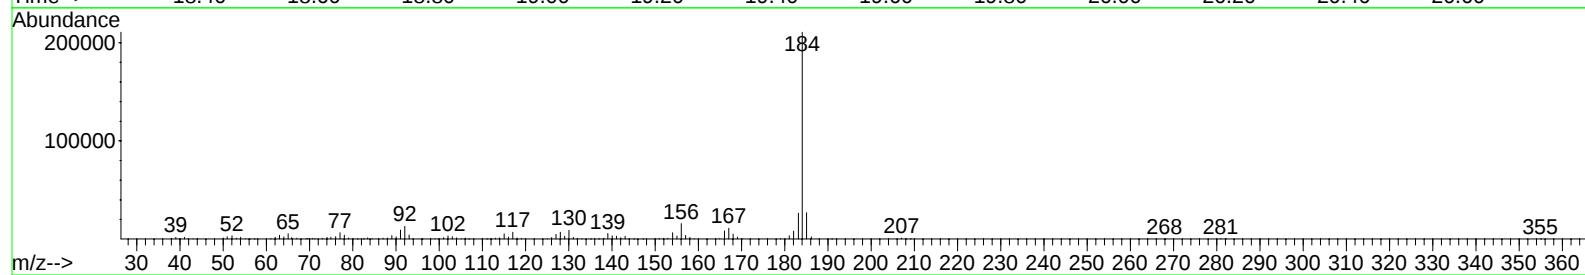


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG063020\
 Data File : BG045881.D
 Acq On : 30 Jun 2020 12:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 30 19:06:42 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 30 16:34:40 2020
 Response via : Initial Calibration

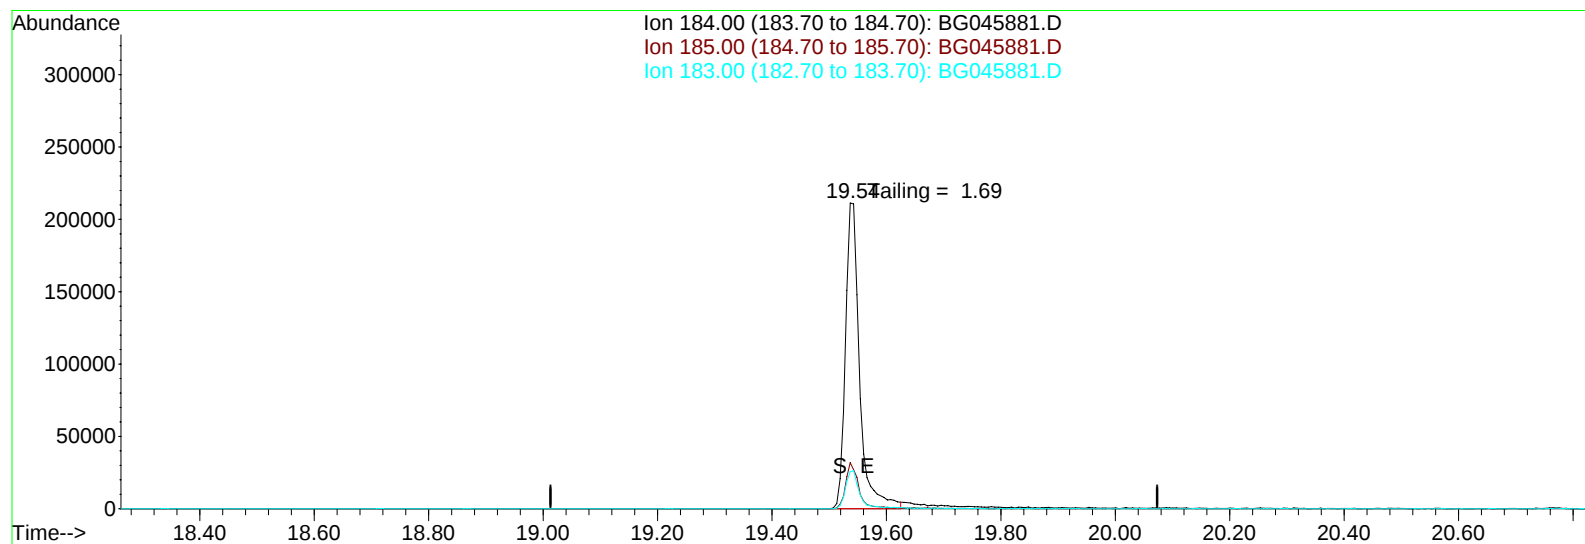

TIC: BG045881.D

(77) Benzidine




19.543min (-19.543) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	13.20	0.00#
183.00	12.60	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG063020\
Data File : BG045881.D
Acq On : 30 Jun 2020 12:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 30 19:06:42 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 30 16:34:40 2020
Response via : Initial Calibration

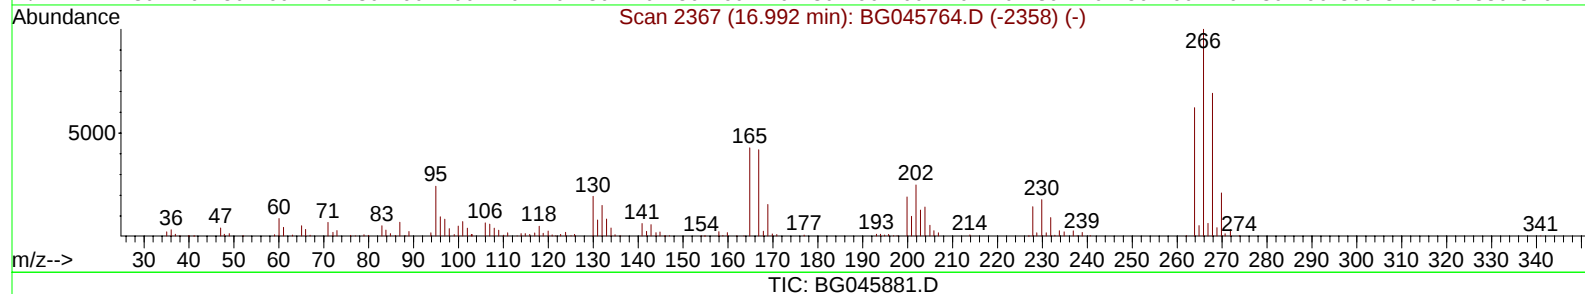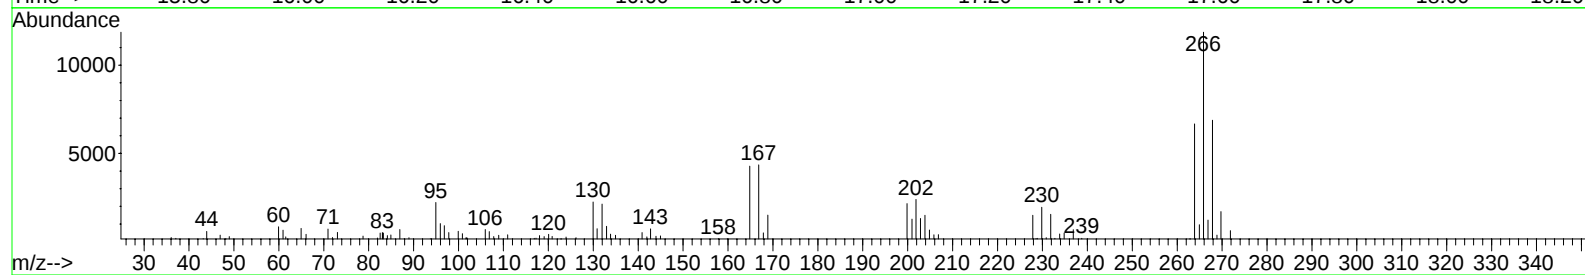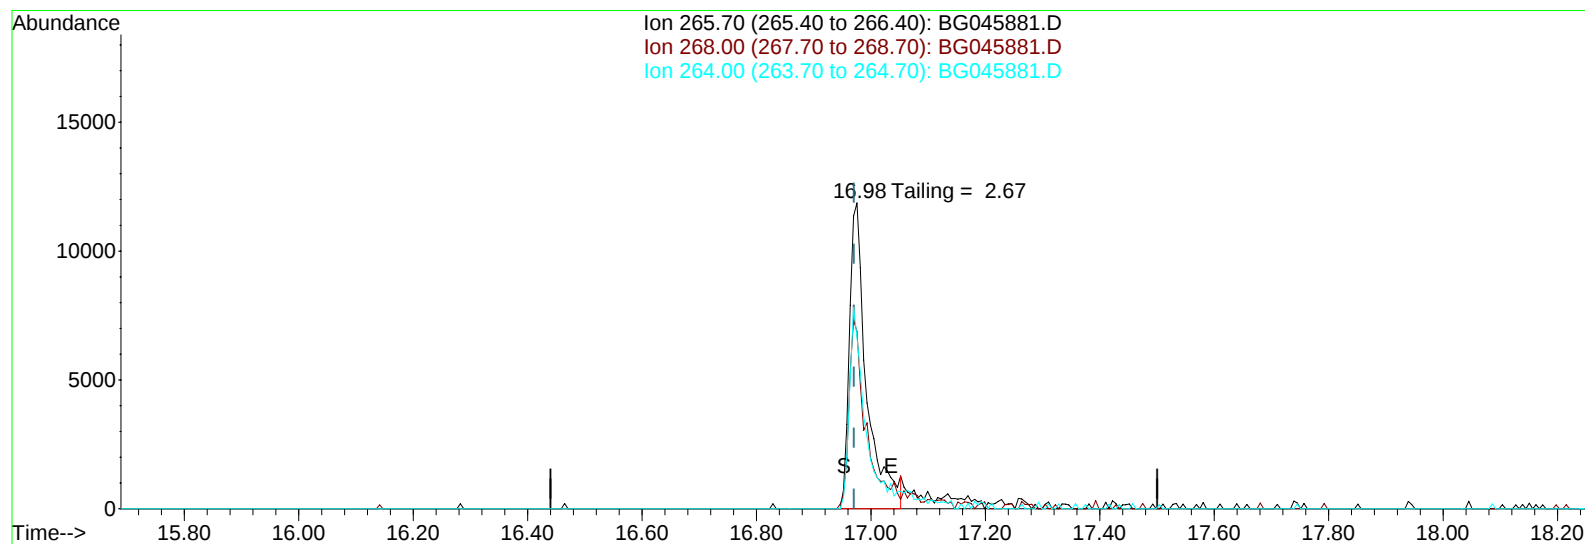

(70) Pentachlorophenol (C)

16.976min (+0.006) 9512.94ng

response 24578

Ion	Exp%	Act%
265.70	100	100
268.00	63.60	57.97
264.00	62.30	56.20
0.00	0.00	0.00