

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG063020\
 Data File : BG045896.D
 Acq On : 30 Jun 2020 22:47
 Operator : CG/JU
 Sample : L2806-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 AU-06-062620

Quant Time: Jul 01 03:29:19 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 30 16:34:40 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.89	152	60223	20.00	ng	0.00
21) Naphthalene-d8	10.70	136	235753	20.00	ng	0.00
39) Acenaphthene-d10	14.54	164	160640	20.00	ng	0.00
64) Phenanthrene-d10	17.30	188	343042	20.00	ng	0.00
76) Chrysene-d12	21.55	240	307753	20.00	ng	0.00
86) Perylene-d12	24.67	264	317516	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.50	112	466723	130.91	ng	0.00
7) Phenol-d6	7.12	99	682104	125.78	ng	0.00
23) Nitrobenzene-d5	9.06	82	455818	88.33	ng	0.00
42) 2,4,6-Tribromophenol	16.05	330	231819	95.59	ng	0.00
45) 2-Fluorobiphenyl	13.17	172	1002389	91.70	ng	0.00
79) Terphenyl-d14	19.92	244	1431903	94.29	ng	0.00
Target Compounds						
50) Dimethylphthalate	14.00	163	59814	4.753	ng	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG063020\
Data File : BG045896.D
Acq On : 30 Jun 2020 22:47
Operator : CG/JU
Sample : L2806-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
AU-06-062620

Quant Time: Jul 01 03:29:19 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 30 16:34:40 2020
Response via : Initial Calibration

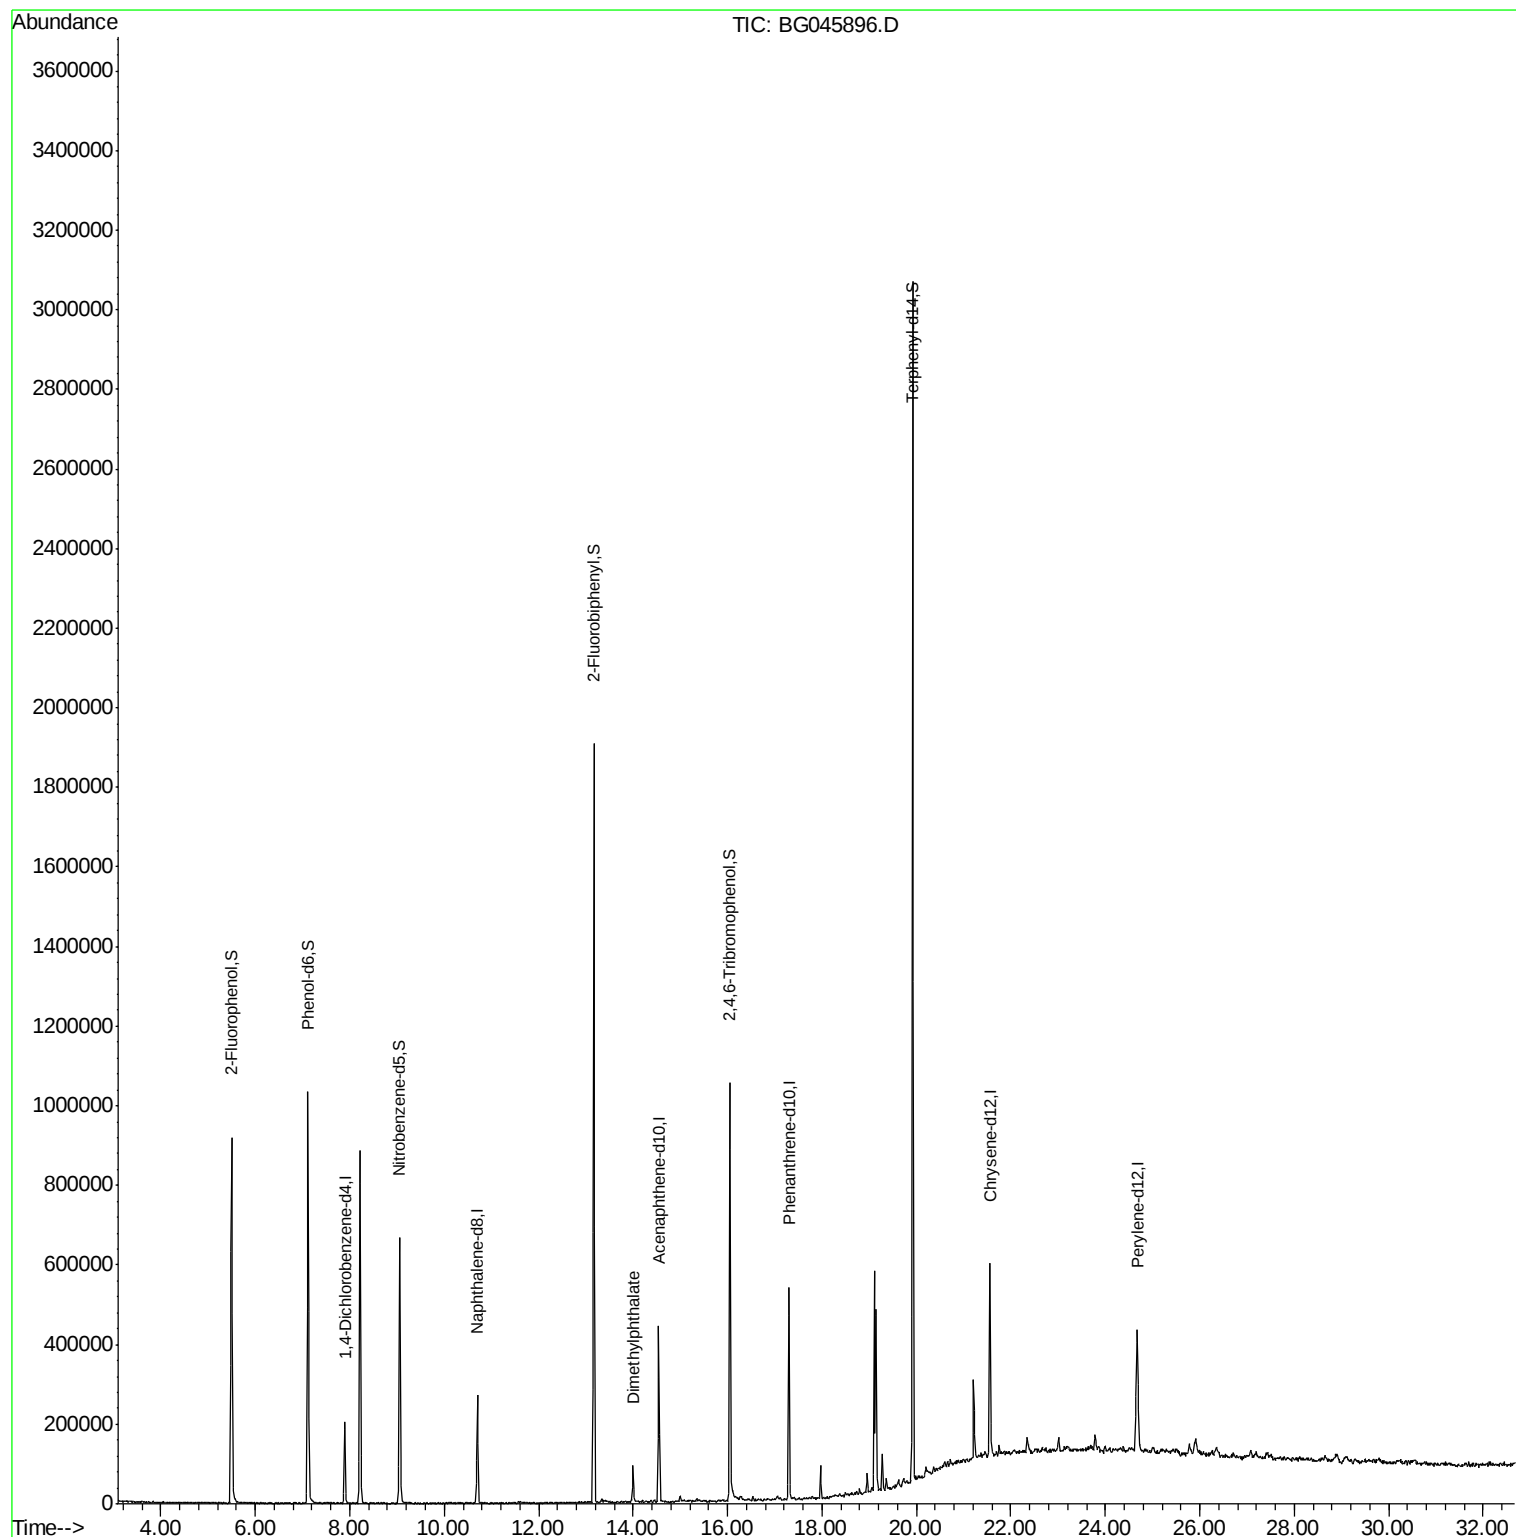




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.89 min Scan# 818
Delta R.T. 0.00 min
Lab File: BG045896.D
Acq: 30 Jun 2020 22:47

Instrument :
BNA_G
ClientSampleId :
AU-06-062620

Tot Ion	Ratio	Lower	Upper
152	100		
150	158.4	121.2	181.8
115	66.6	47.5	71.3

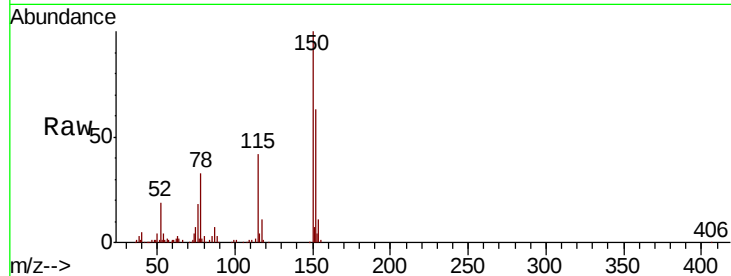


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

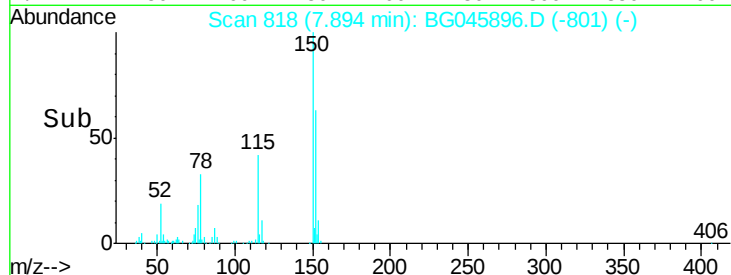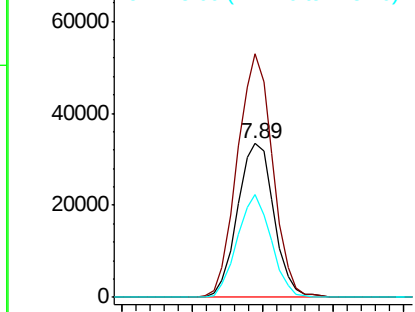



#5


2-Fluorophenol
Concen: 130.914 ng
RT: 5.50 min Scan# 410
Delta R.T. 0.01 min
Lab File: BG045896.D
Acq: 30 Jun 2020 22:47

Tgt Ion	Ratio	Lower	Upper
112	100		
64	60.7	48.5	72.7
63	34.5	26.5	39.7



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

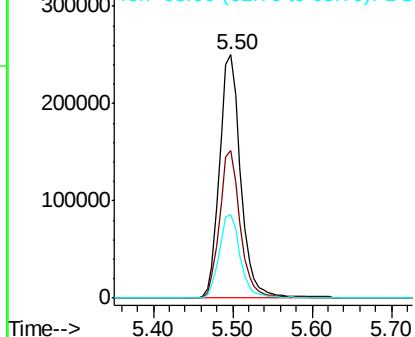

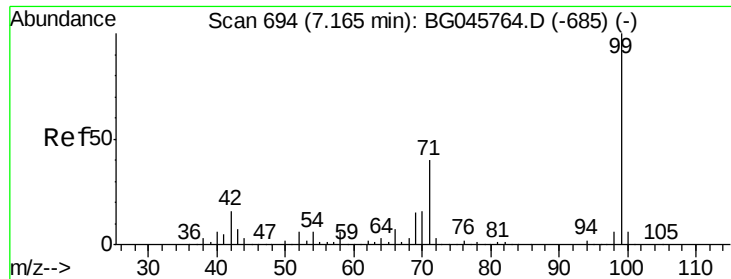

#7

Phenol-d6

Concen: 125.784 ng

RT: 7.12 min Scan# 686

Delta R.T. 0.01 min

Lab File: BG045896.D

Acq: 30 Jun 2020 22:47

Instrument :

BNA_G

ClientSampleId :

AU-06-062620


Tot Ion: 99 Resp: 682104

Ion Ratio Lower Upper




99 100

42 15.5 12.0 18.0

71 41.2 31.0 46.4

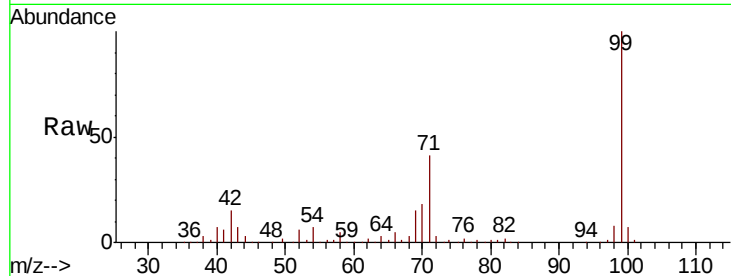

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

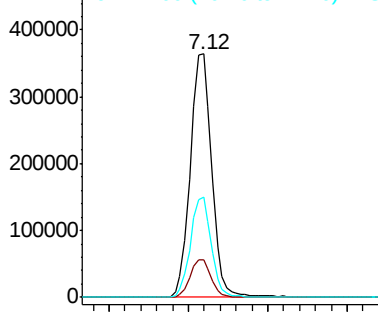

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.70 min Scan# 1296

Delta R.T. 0.00 min

Lab File: BG045896.D

Acq: 30 Jun 2020 22:47

Tgt Ion: 136 Resp: 235753


Ion Ratio Lower Upper

136 100



137 11.1 9.4 14.0


54 5.6 4.9 7.3

68 5.4 3.9 5.9



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC




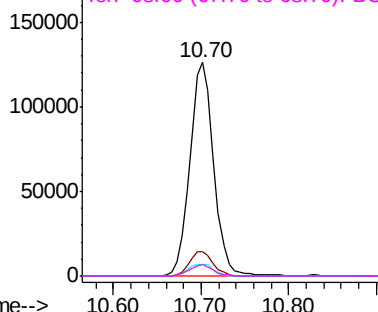


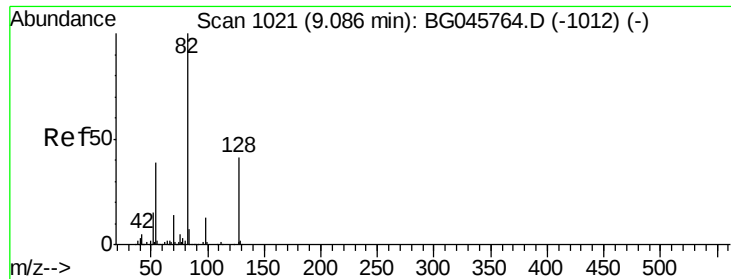

#23
Nitrobenzene-d5
Concen: 88.327 ng
RT: 9.06 min Scan# 1016
Delta R.T. 0.00 min
Lab File: BG045896.D
Acq: 30 Jun 2020 22:47




Instrument :
BNA_G
ClientSampleId :
AU-06-062620


Tot Ion	Ratio	Lower	Upper
82	100		
128	38.3	31.3	46.9
54	41.6	32.6	49.0

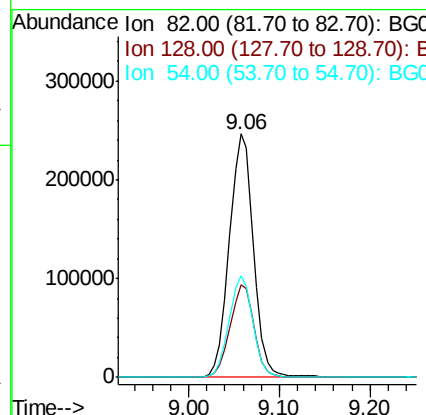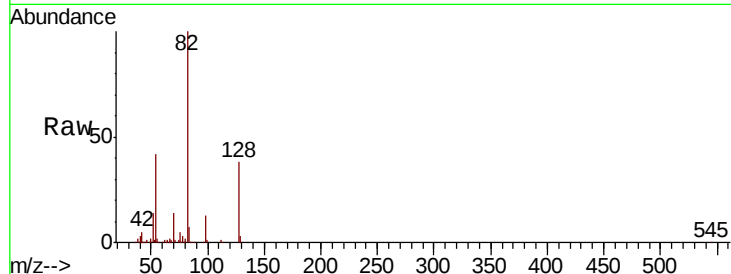

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.54 min Scan# 1950
Delta R.T. -0.01 min
Lab File: BG045896.D
Acq: 30 Jun 2020 22:47

Tgt Ion	Ratio	Lower	Upper
164	100		
162	99.4	80.6	120.8
160	43.5	35.0	52.4

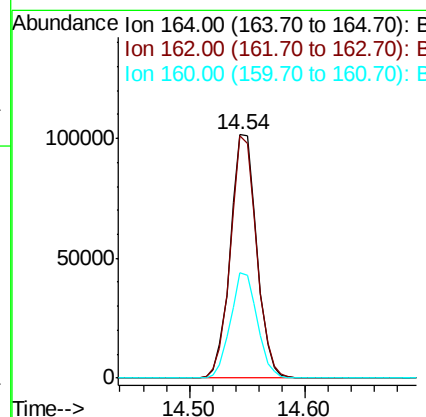



#42

2,4,6-Tribromophenol

Concen: 95.586 ng

RT: 16.05 min Scan# 2206

Delta R.T. 0.00 min

Lab File: BG045896.D

Acq: 30 Jun 2020 22:47

Instrument :

BNA_G

ClientSampleId :

AU-06-062620


Tot Ion:330 Resp: 231819

Ion Ratio Lower Upper

330 100

332 97.8 76.6 114.8




141 36.0 27.7 41.5



Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

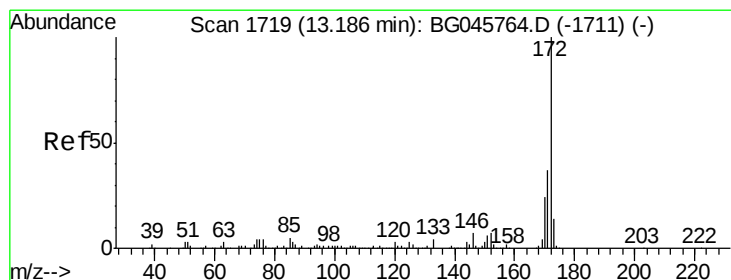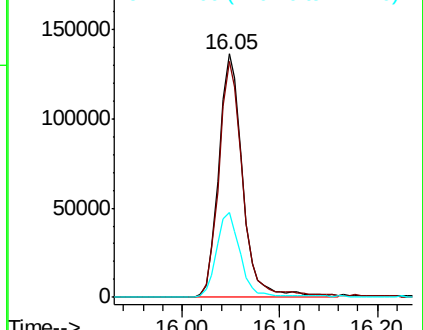

#45

2-Fluorobiphenyl

Concen: 91.700 ng

RT: 13.17 min Scan# 1716

Delta R.T. 0.00 min

Lab File: BG045896.D

Acq: 30 Jun 2020 22:47


Tgt Ion:172 Resp: 1002389

Ion Ratio Lower Upper

172 100

171 36.4 28.9 43.3



170 24.1 19.1 28.7




Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

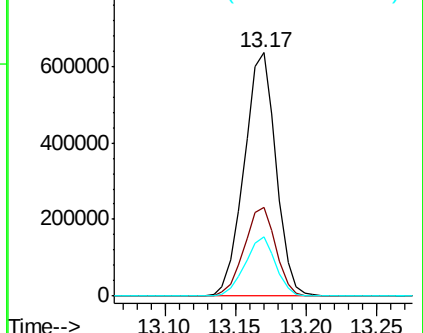

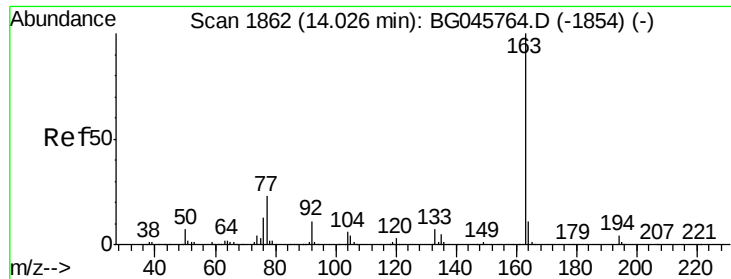

#50

Dimethylphthalate

Concen: 4.753 ng

RT: 14.00 min Scan# 1857

Delta R.T. -0.01 min

Lab File: BG045896.D

Acq: 30 Jun 2020 22:47

Instrument :

BNA_G

ClientSampleId :

AU-06-062620


Tot Ion:163 Resp: 59814

Ion Ratio Lower Upper

163 100

194 4.6 3.3 4.9




164 12.7 8.8 13.2

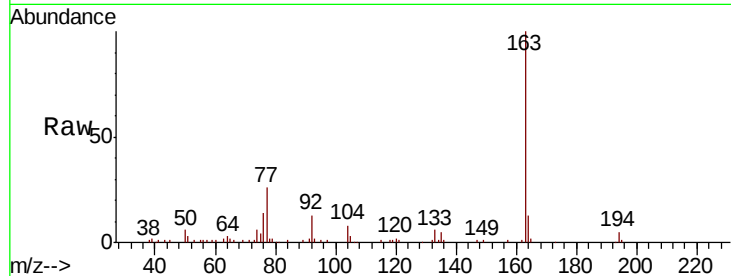

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

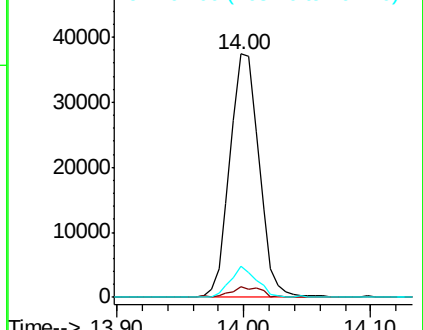

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.30 min Scan# 2419

Delta R.T. 0.00 min

Lab File: BG045896.D

Acq: 30 Jun 2020 22:47


Tgt Ion:188 Resp: 343042

Ion Ratio Lower Upper

188 100

94 6.9 5.7 8.5



80 8.5 6.6 10.0




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

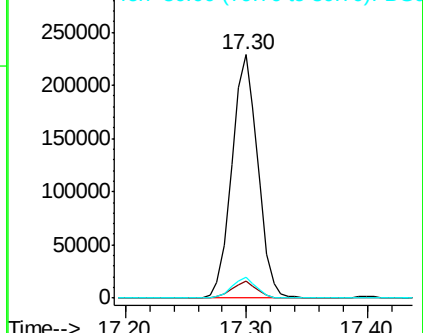



#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.55 min Scan# 3143

Delta R.T. -0.01 min

Lab File: BG045896.D

Acq: 30 Jun 2020 22:47

Instrument :

BNA_G

ClientSampleId :

AU-06-062620


Tot Ion:240 Resp: 307753

Ion Ratio Lower Upper

240 100

120 6.0 5.6 8.4




236 25.9 21.3 31.9

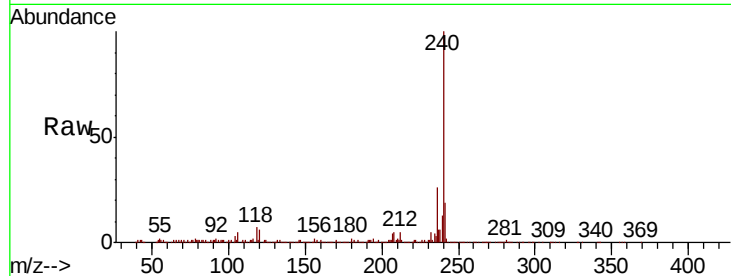

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

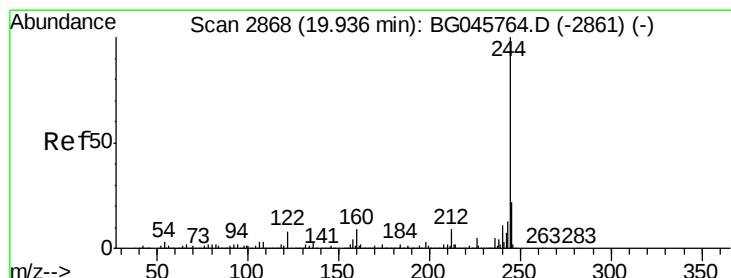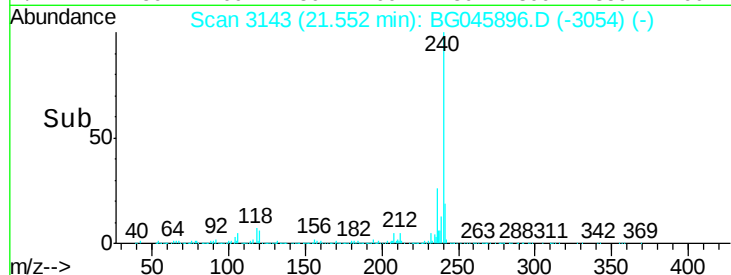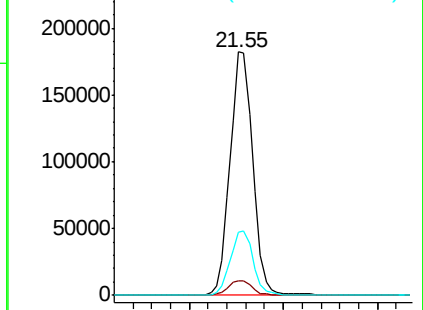

#79

Terphenyl-d14

Concen: 94.293 ng

RT: 19.92 min Scan# 2865

Delta R.T. 0.00 min

Lab File: BG045896.D

Acq: 30 Jun 2020 22:47


Tgt Ion:244 Resp: 1431903

Ion Ratio Lower Upper

244 100

212 9.1 7.2 10.8



122 7.8 6.9 10.3




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

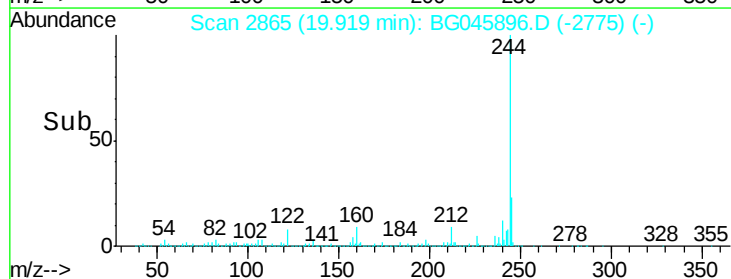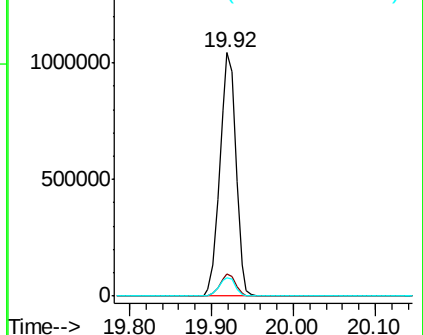

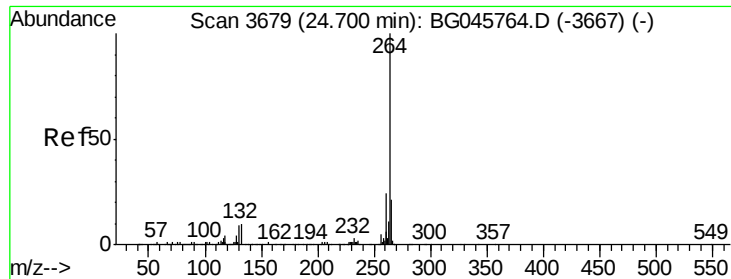

#86
Pervlene-d12
Concen: 20.000 ng
RT: 24.67 min Scan# 3674
Delta R.T. 0.00 min
Lab File: BG045896.D
Acq: 30 Jun 2020 22:47

Instrument :
BNA_G
ClientSampleId :
AU-06-062620

Tot Ion:	264	Resp:	317516
Ion	Ratio	Lower	Upper
264	100		
260	23.2	19.5	29.3
265	22.6	17.4	26.0

