


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG063020\
 Data File : BG045881.D
 Acq On : 30 Jun 2020 12:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 30 16:34:40 2020

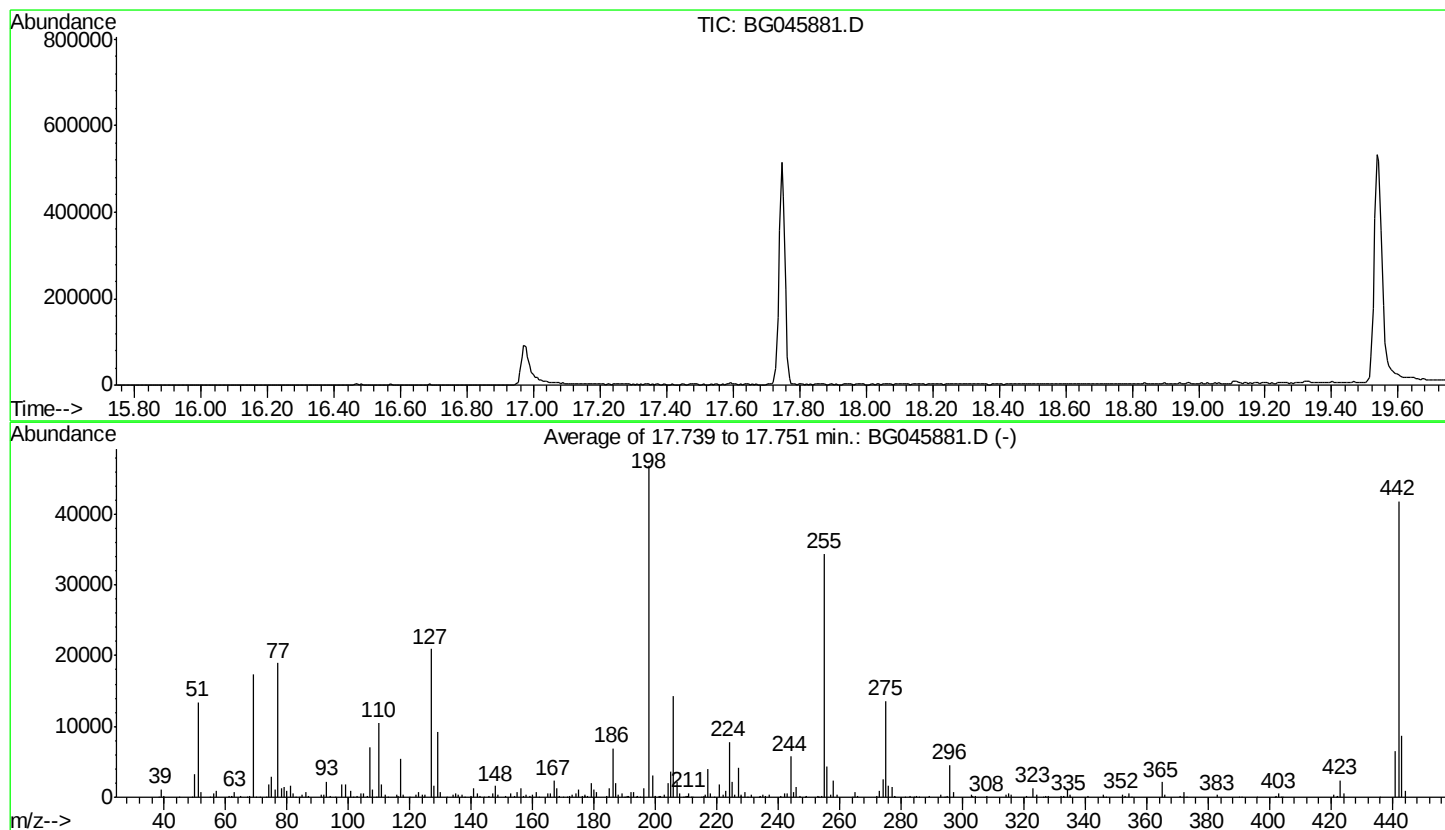

AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.7	13460	PASS
68	69	0.00	2	1.3	219	PASS
69	198	0.00	100	37.1	17357	PASS
70	69	0.00	2	0.4	68	PASS
127	198	10	80	44.7	20912	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	46834	PASS
199	198	5	9	6.4	2996	PASS
275	198	10	60	29.0	13576	PASS
365	198	1	100	4.6	2132	PASS
441	198	0.01	100	14.1	6604	PASS
442	198	50	100	89.3	41800	PASS
443	442	15	24	20.7	8632	PASS