


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG070119\
 Data File : BG041550.D
 Acq On : 1 Jul 2019 9:00
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG062619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 27 13:25:55 2019

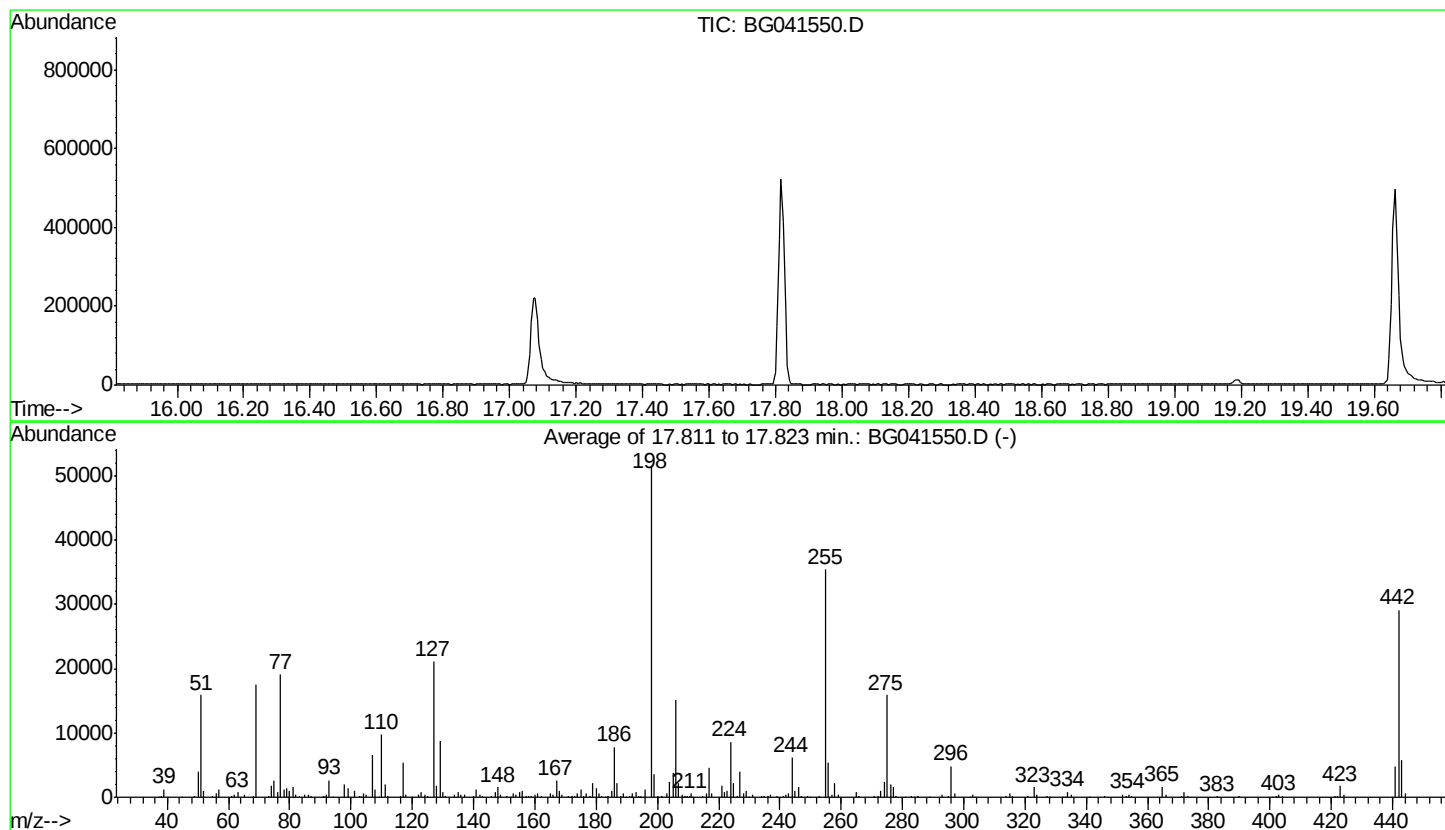

AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2500

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.8	15861	PASS
68	69	0.00	2	0.8	133	PASS
69	198	0.00	100	34.2	17607	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.9	21072	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	51546	PASS
199	198	5	9	7.1	3641	PASS
275	198	10	60	30.8	15869	PASS
365	198	1	100	3.2	1657	PASS
441	198	0.01	100	9.1	4698	PASS
442	198	50	100	56.5	29133	PASS
443	442	15	24	19.9	5812	PASS