
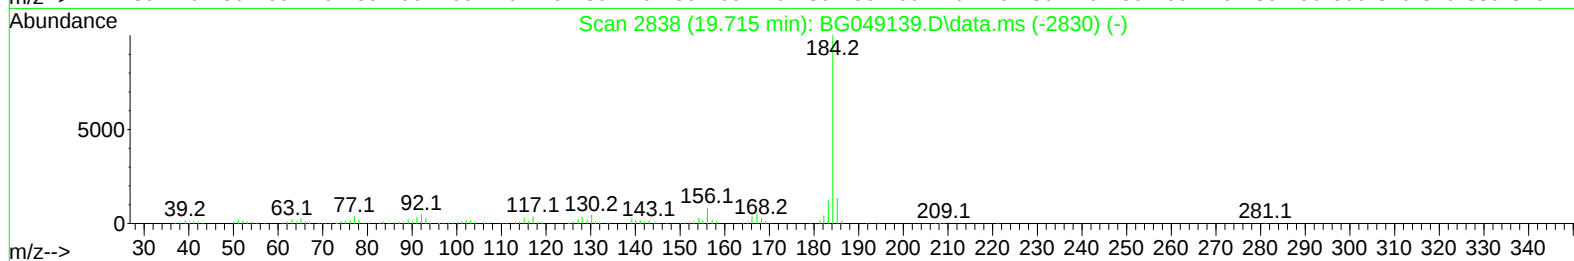
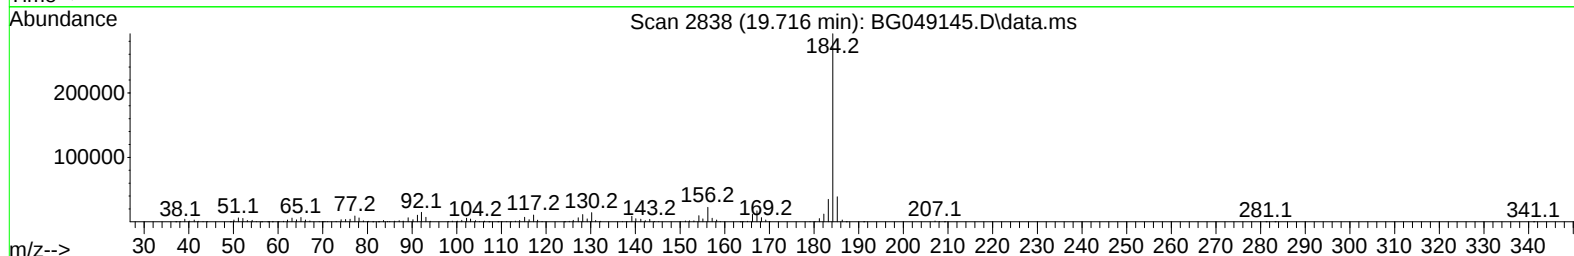


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070121\
 Data File : BG049145.D
 Acq On : 1 Jul 2021 8:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 01 13:36:27 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG063021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 30 15:39:12 2021
 Response via : Initial Calibration

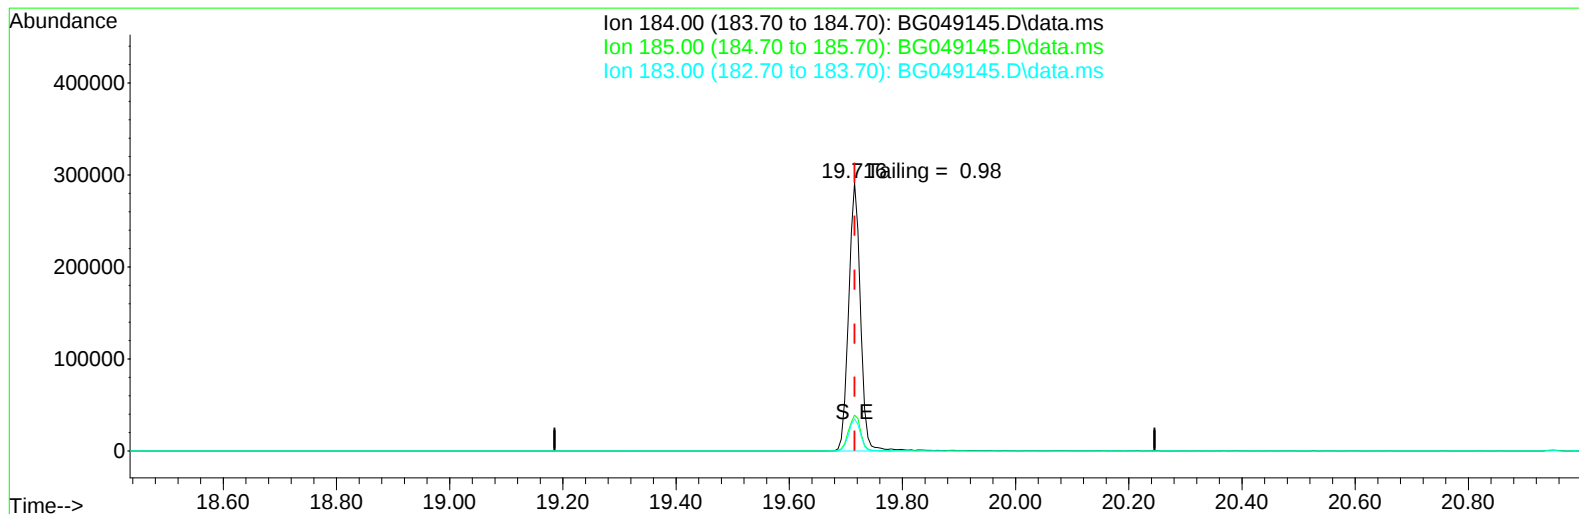

TIC: BG049145.D\data.ms

(77) Benzidine




19.716min (+ 0.000) 0.00 ng

response 421799

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.37
183.00	11.70	11.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070121\
Data File : BG049145.D
Acq On : 1 Jul 2021 8:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 01 13:36:27 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG063021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 30 15:39:12 2021
Response via : Initial Calibration

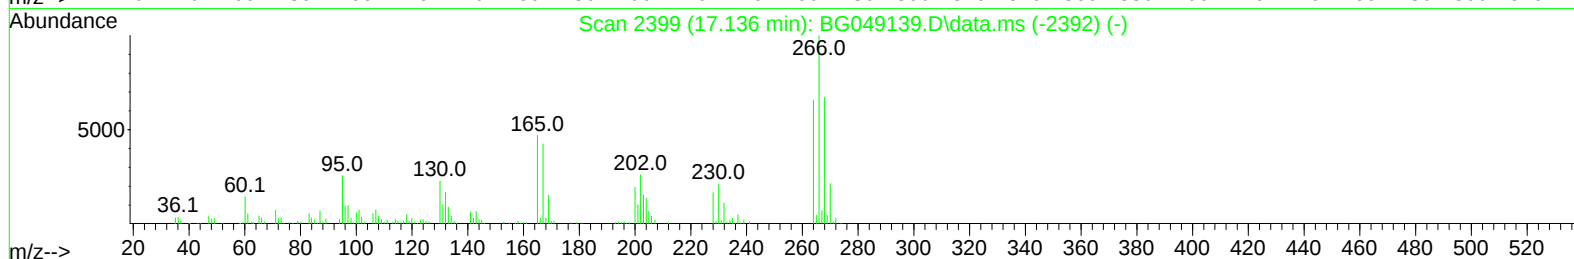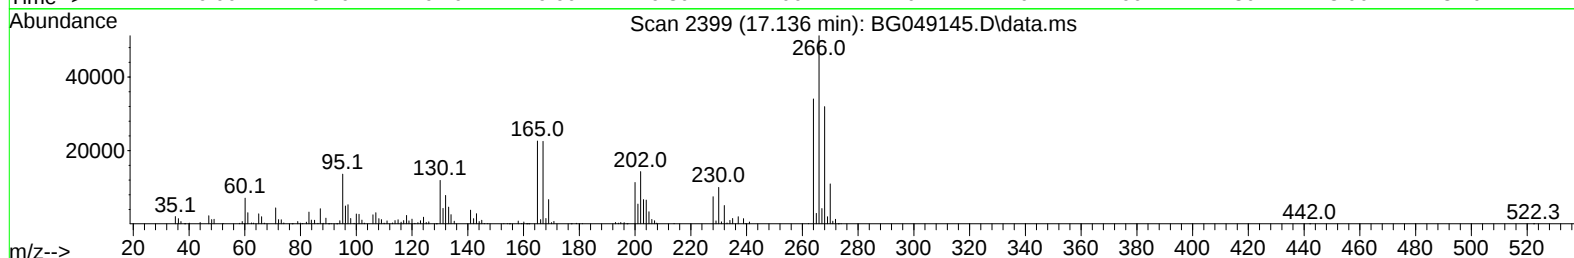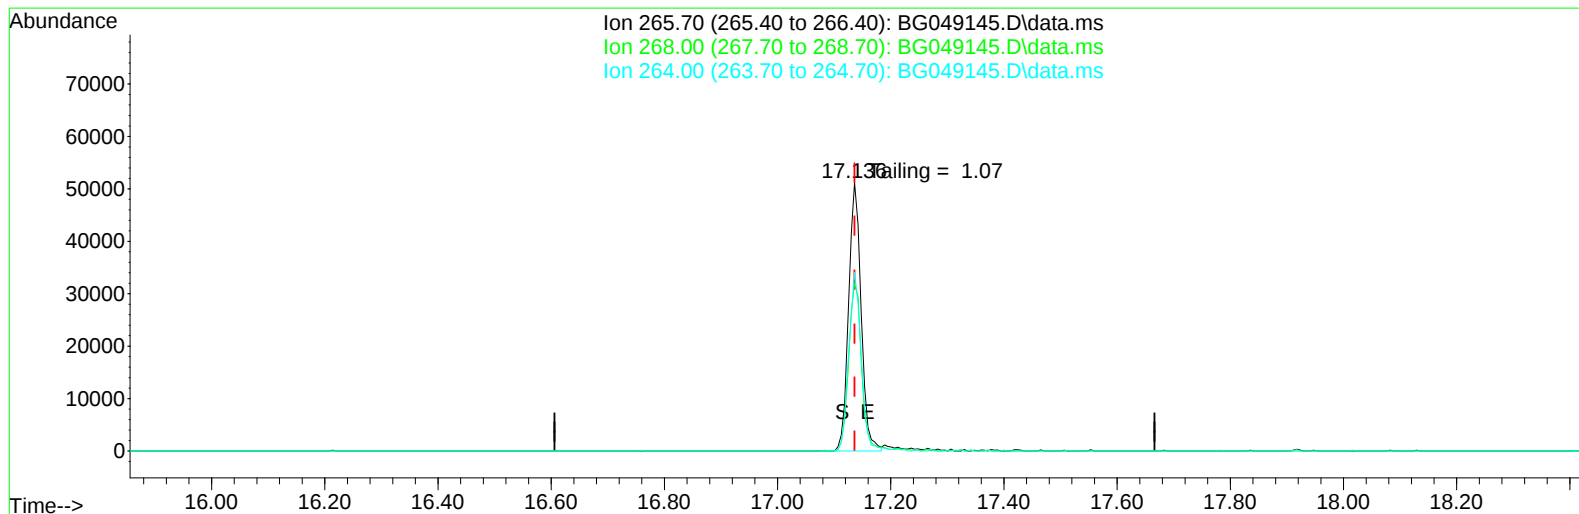

TIC: BG049145.D\data.ms

(70) Pentachlorophenol (C)

17.136min (+ 0.000) 21989.28 ng

response 78460

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	62.38
264.00	61.30	66.46
0.00	0.00	0.00