


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070121\
 Data File : BG049145.D
 Acq On : 1 Jul 2021 8:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG063021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 30 15:39:12 2021

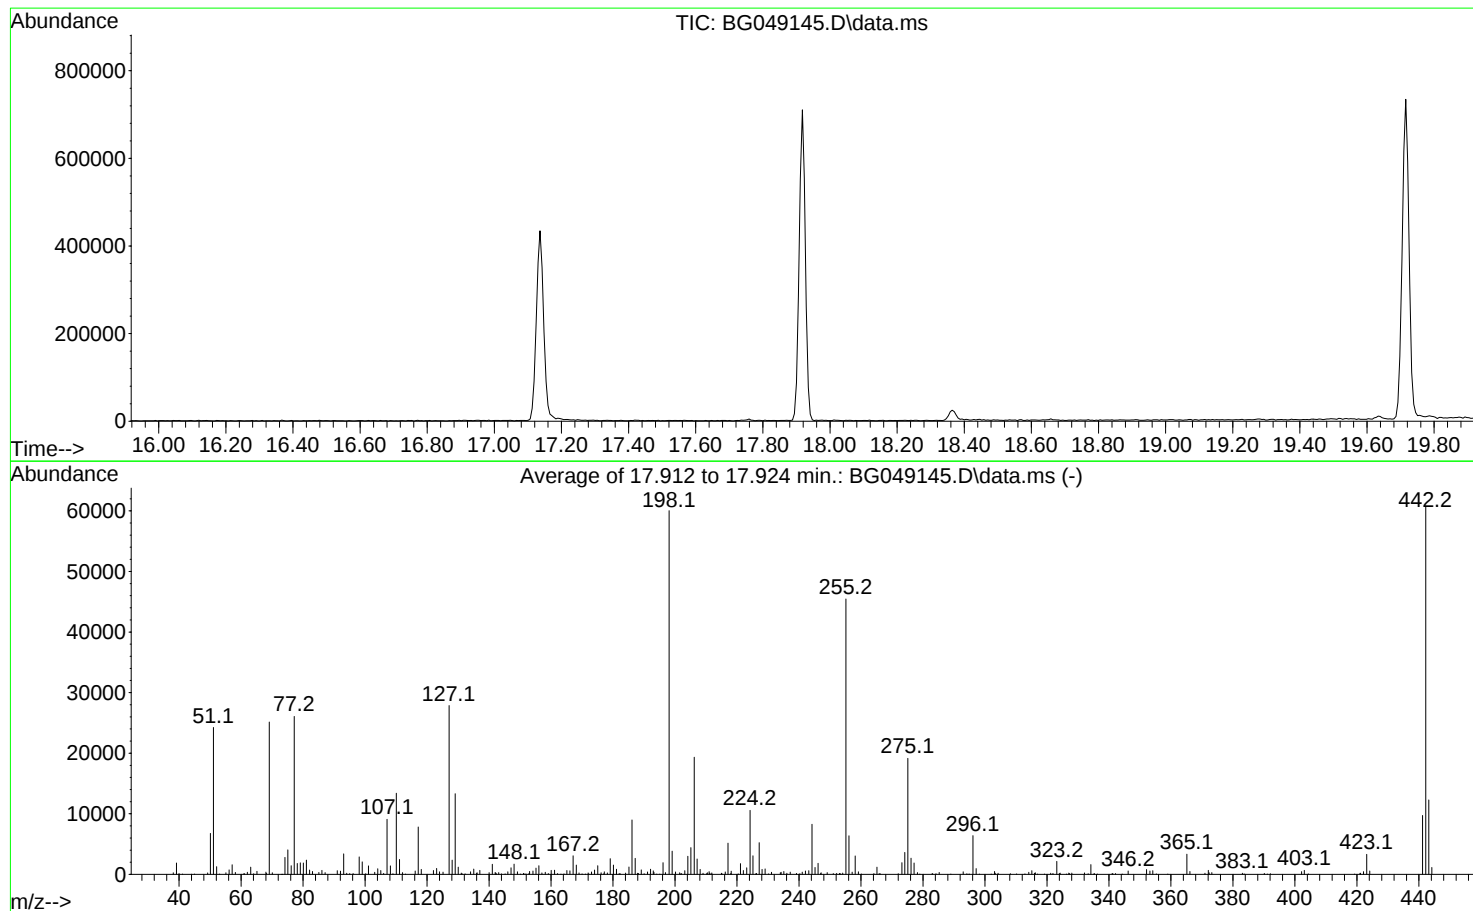




AutoFind: Scans 2531, 2532, 2533; Background Corrected with Scan 2524

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.4	24240	PASS
68	69	0.00	2	1.5	373	PASS
69	198	0.00	100	41.9	25139	PASS
70	69	0.00	2	1.0	253	PASS
127	198	10	80	46.4	27867	PASS
197	198	0.00	2	0.5	284	PASS
198	198	100	100	100.0	60043	PASS
199	198	5	9	6.4	3825	PASS
275	198	10	60	31.9	19160	PASS
365	198	1	100	5.5	3332	PASS
441	198	0.01	100	16.2	9709	PASS
442	442	100	100	100.0	60723	PASS
443	442	15	24	20.2	12277	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070121\
 Data File : BG049145.D
 Acq On : 1 Jul 2021 8:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jul 01 13:36:27 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG063021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 30 15:39:12 2021
 Response via : Initial Calibration

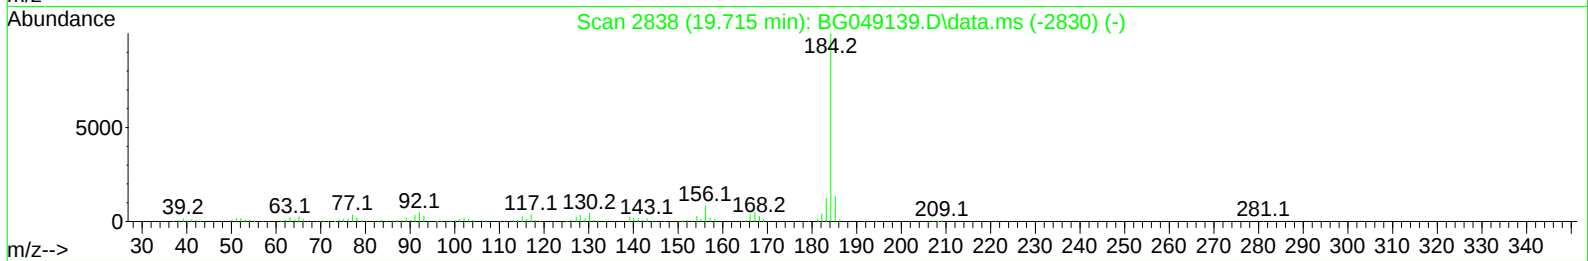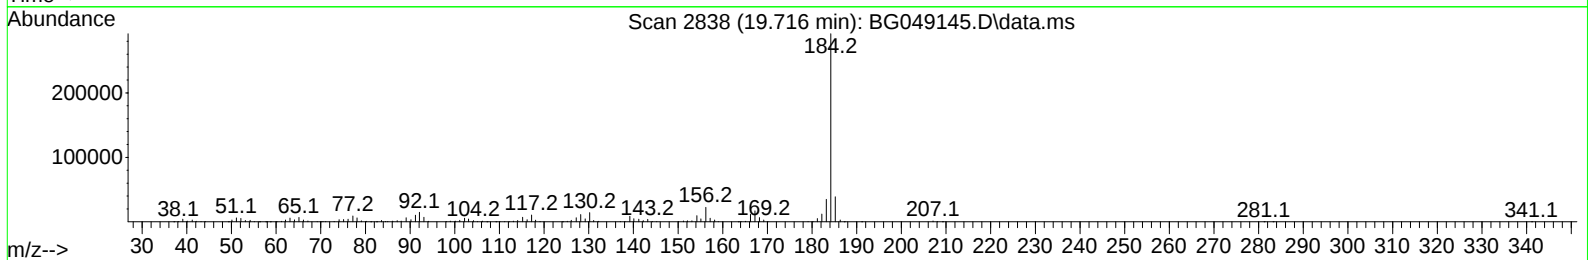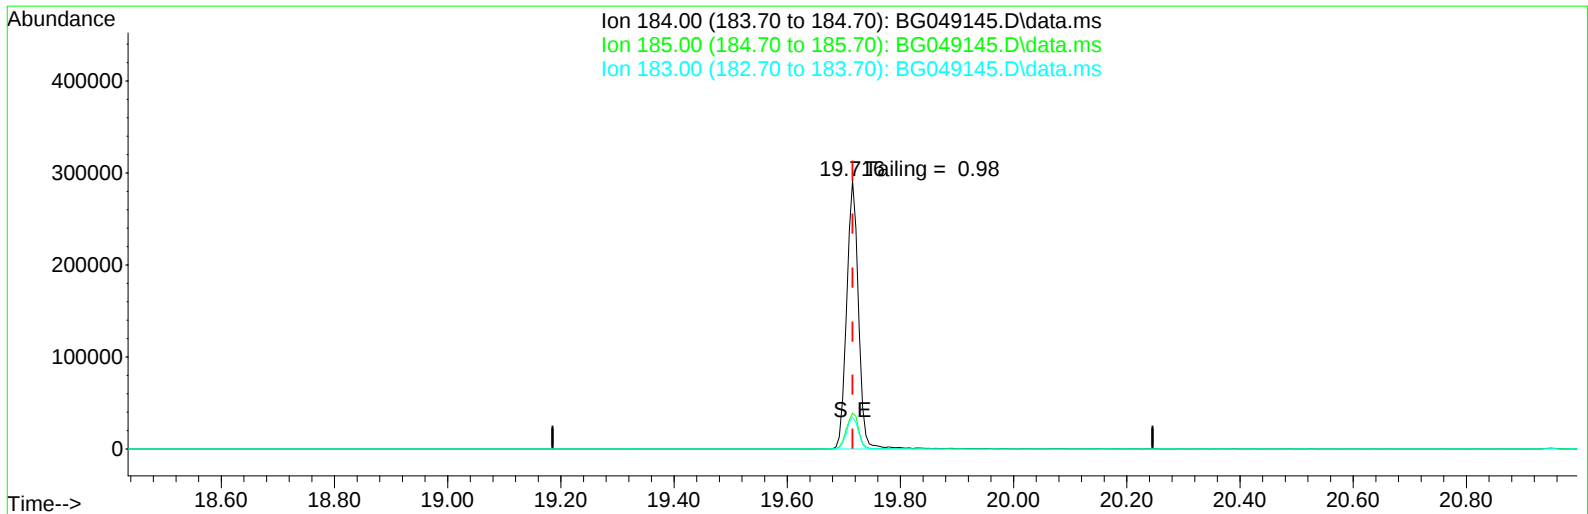

TIC: BG049145.D\data.ms

(77) Benzidine

19.716min (+ 0.000) 0.00 ng




response 421799

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.37
183.00	11.70	11.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070121\
Data File : BG049145.D
Acq On : 1 Jul 2021 8:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 01 13:36:27 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG063021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 30 15:39:12 2021
Response via : Initial Calibration

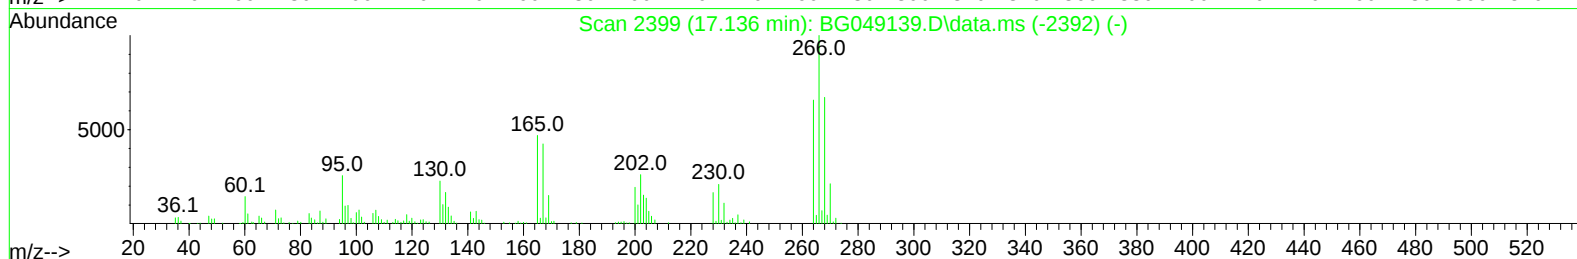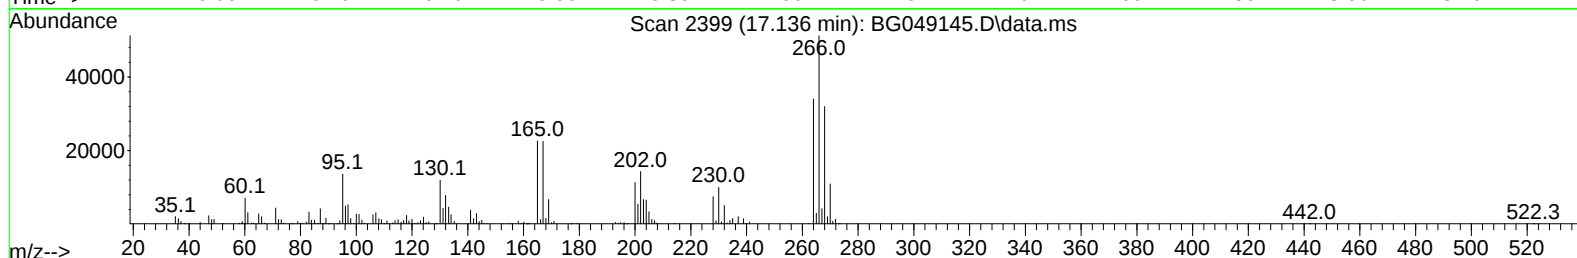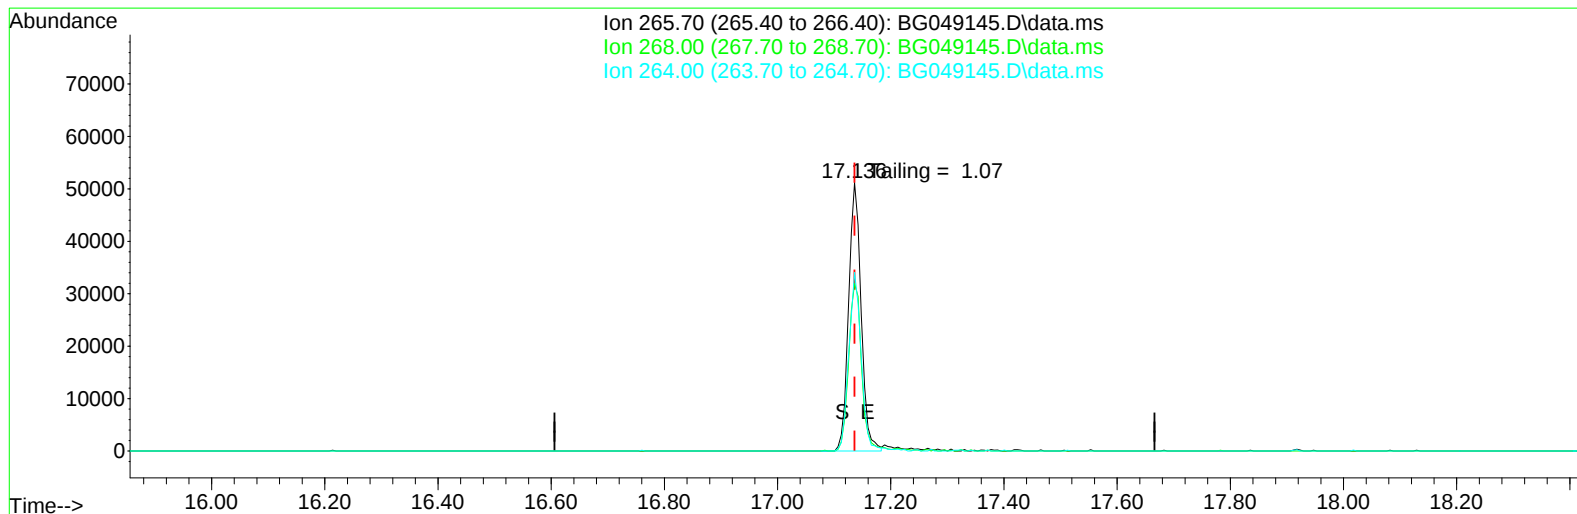

TIC: BG049145.D\data.ms

(70) Pentachlorophenol (C)

17.136min (+ 0.000) 21989.28 ng

response 78460

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	62.38
264.00	61.30	66.46
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/1/2021	BNA_G	<u>BG049145.D</u>
Compound Name	Response	Retention Time
DDT	219423	20.94
DDD	3466	20.5
DDE	136	19.99
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3602	223025	1.62