
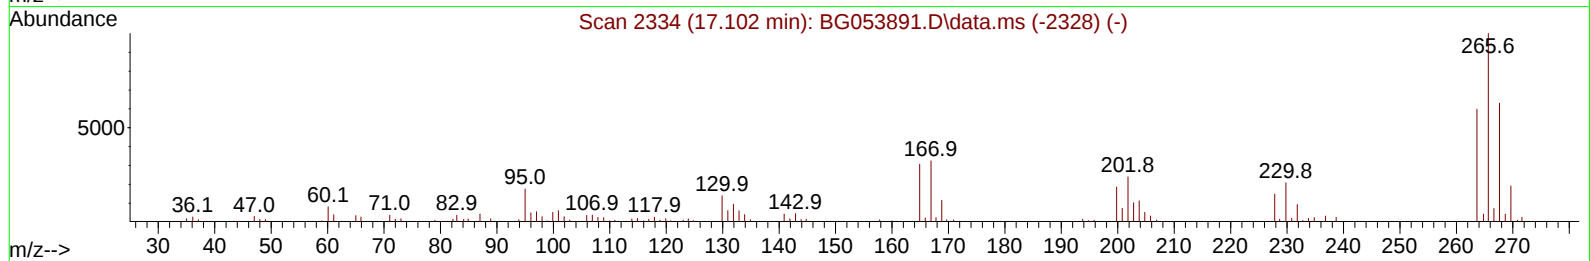
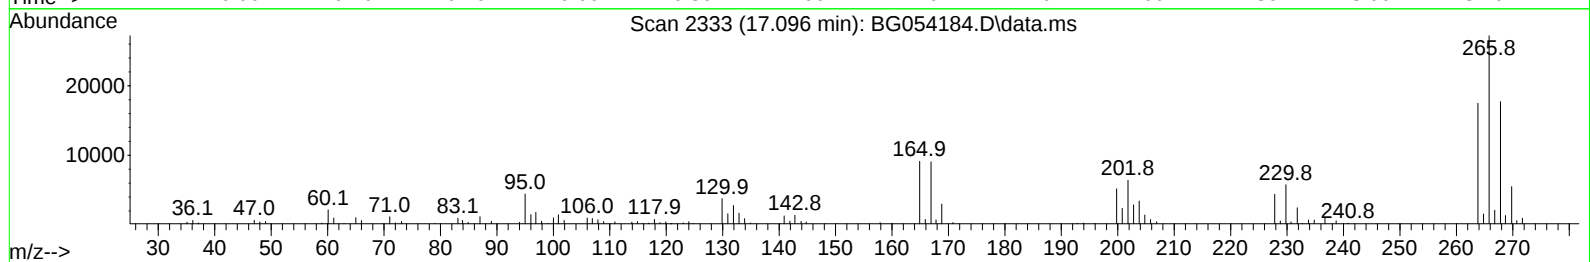


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070122\
Data File : BG054184.D
Acq On : 1 Jul 2022 10:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 02 04:10:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 00:27:54 2022
Response via : Initial Calibration

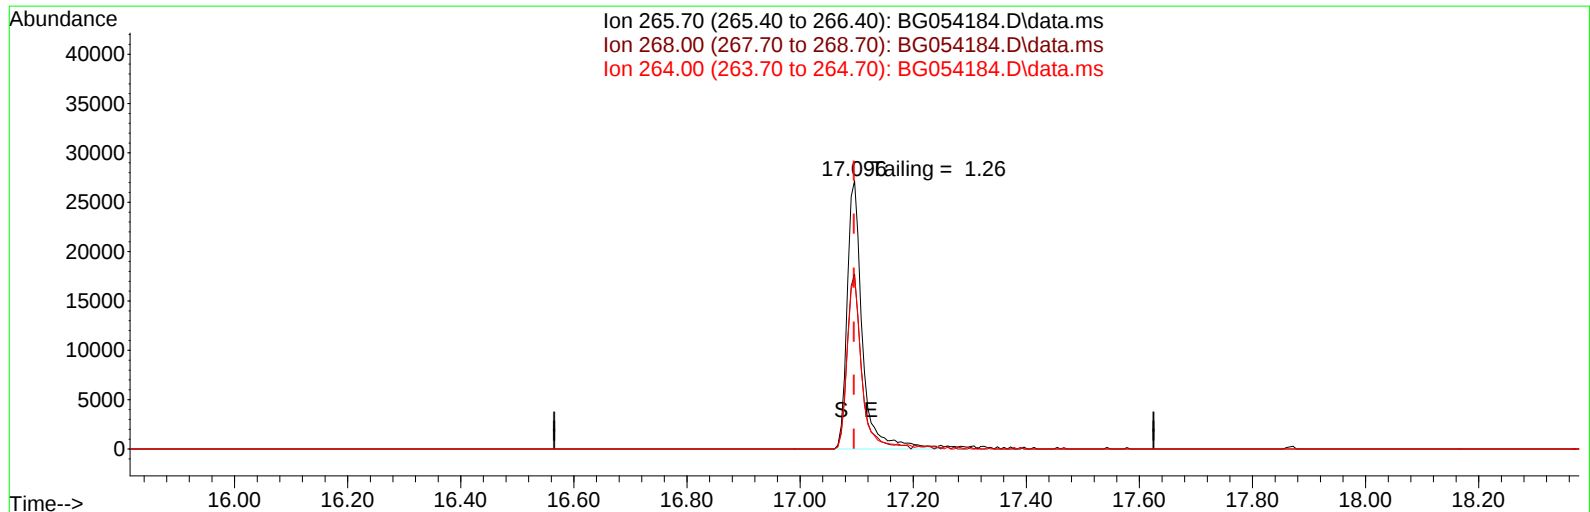

TIC: BG054184.D\data.ms

(70) Pentachlorophenol (C)




17.096min (+ 0.001) 29775.97 ng

response 50587

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	70.09
264.00	66.20	64.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070122\
Data File : BG054184.D
Acq On : 1 Jul 2022 10:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 02 04:10:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 00:27:54 2022
Response via : Initial Calibration

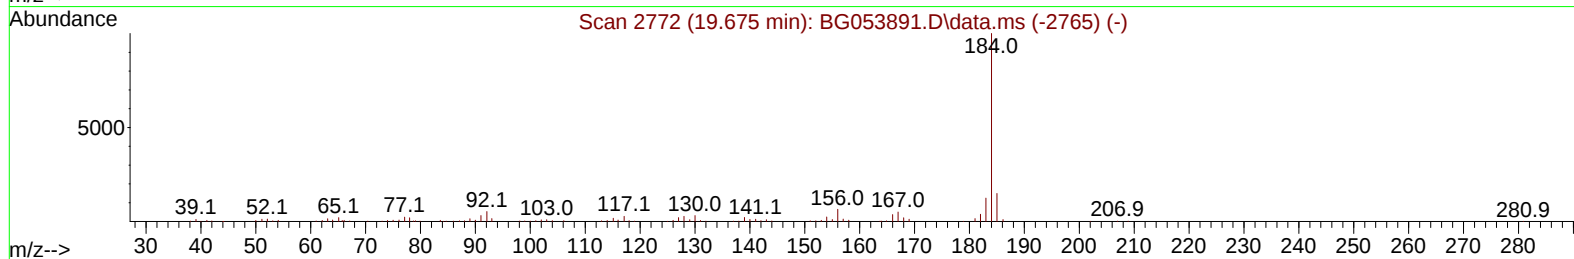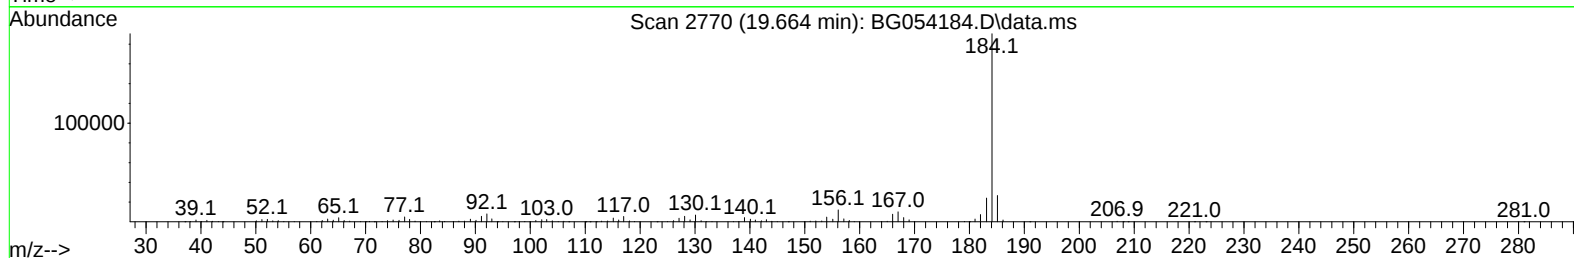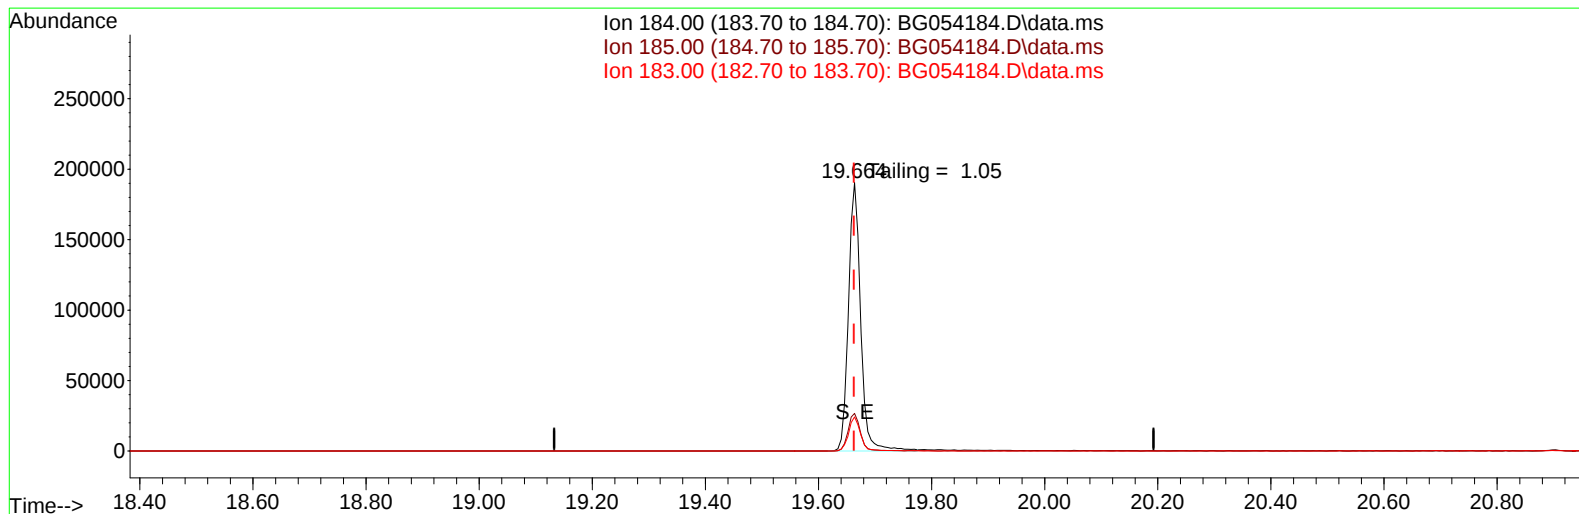

TIC: BG054184.D\data.ms

(77) Benzidine

19.664min (+ 0.001) 246936.32 ng

response 286372

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.01
183.00	11.10	12.71
0.00	0.00	0.00