

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070122\
 Data File : BG054192.D
 Acq On : 1 Jul 2022 15:37
 Operator : CG/JU
 Sample : N3561-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 S-3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG054192.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.635	375	382	391	rVB	161517	274513	21.99%	5.873%
2	7.228	645	653	663	rBV	169824	305354	24.46%	6.533%
3	8.062	789	795	804	rVB	42931	75521	6.05%	1.616%
4	9.225	984	993	1003	rBB	104910	197905	15.86%	4.234%
5	10.876	1267	1274	1282	rVB	57171	105477	8.45%	2.257%
6	13.315	1682	1689	1698	rBB	333761	539936	43.26%	11.552%
7	14.689	1916	1923	1930	rBB	110422	179176	14.36%	3.834%
8	16.176	2169	2176	2189	rBV3	362824	582222	46.65%	12.457%
9	17.433	2384	2390	2398	rVB	173820	274510	21.99%	5.873%
10	18.320	2537	2541	2549	rBV3	11699	21779	1.74%	0.466%
11	20.042	2828	2834	2840	rBV	944503	1248176	100.00%	26.706%
12	21.340	3051	3055	3062	rBV2	55567	88462	7.09%	1.893%
13	21.711	3112	3118	3126	rVB	225395	377636	30.26%	8.080%
14	22.892	3315	3319	3328	rVB8	11615	21917	1.76%	0.469%
15	24.966	3662	3672	3684	rVB3	127295	381208	30.54%	8.156%




Sum of corrected areas: 4673792

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070122\
Data File : BG054192.D
Acq On : 1 Jul 2022 15:37
Operator : CG/JU
Sample : N3561-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
S-3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

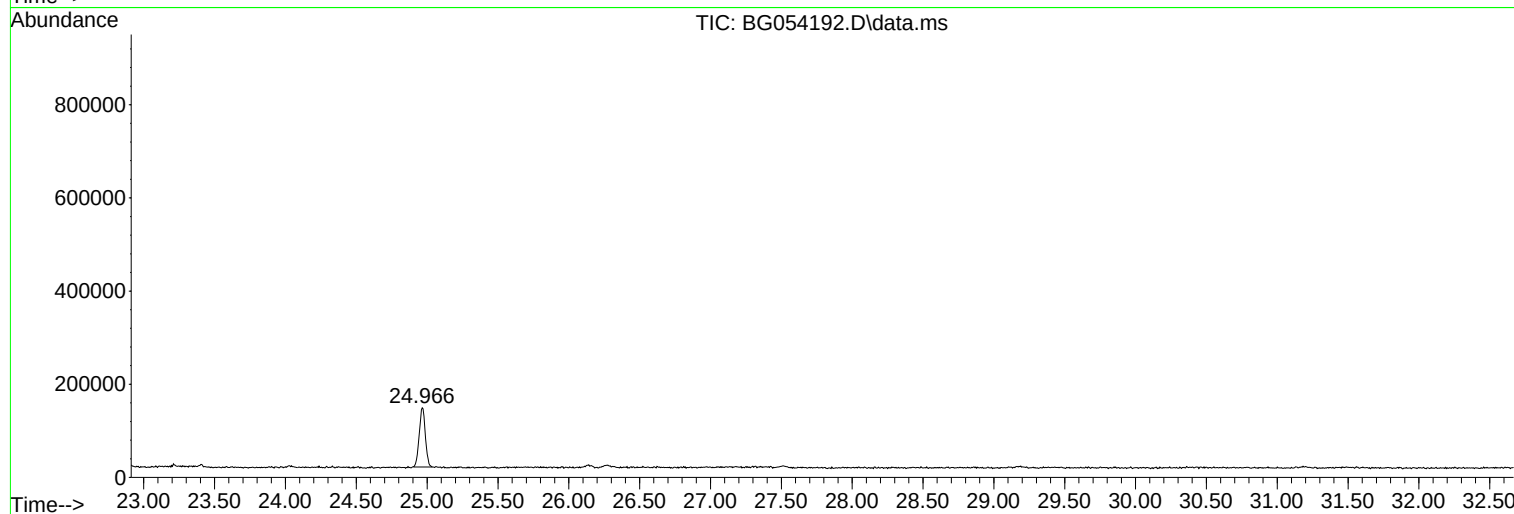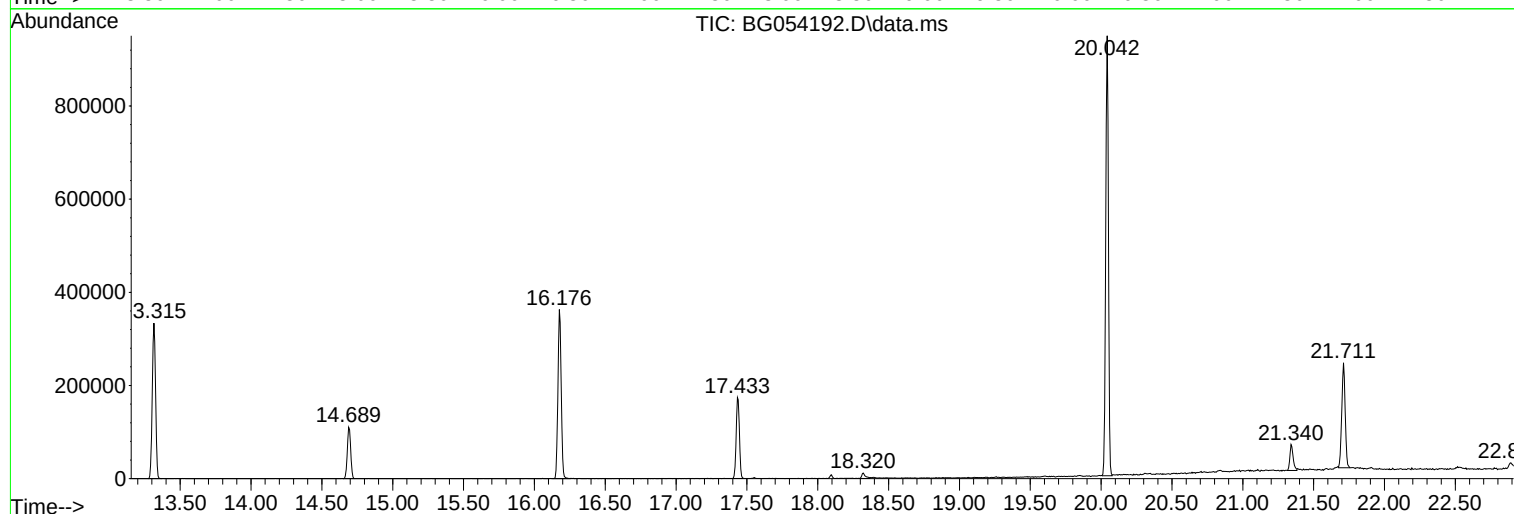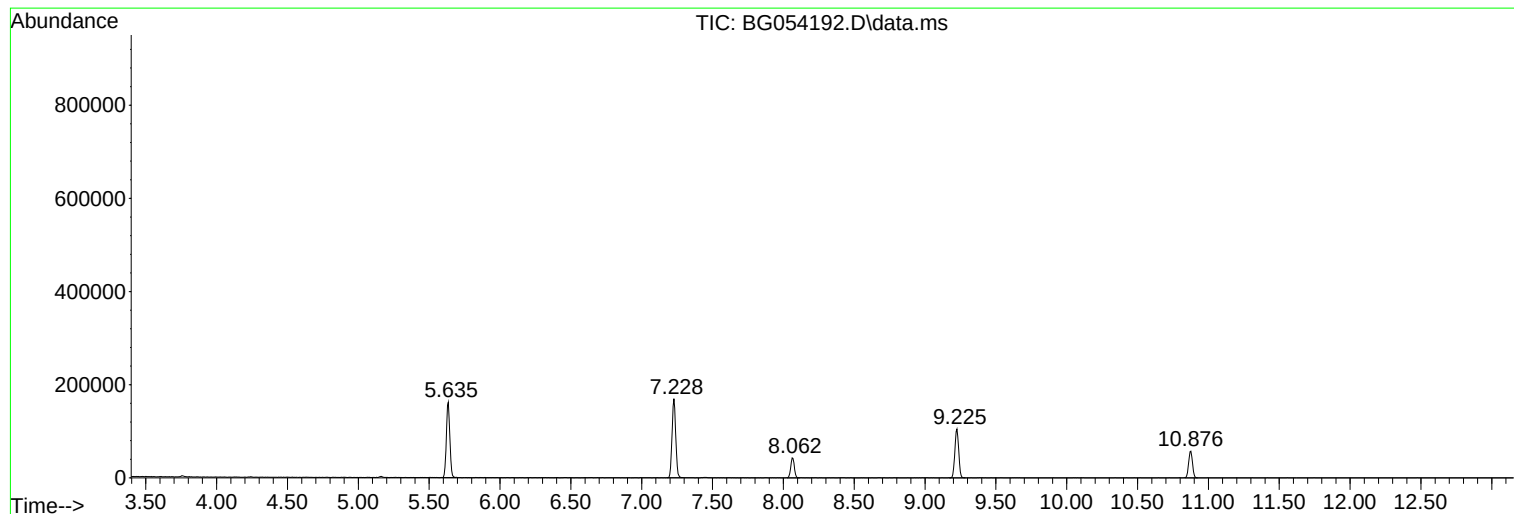

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070122\
Data File : BG054192.D
Acq On : 1 Jul 2022 15:37
Operator : CG/JU
Sample : N3561-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
S-3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Trifluoroacetoxy hexadecane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.340	4.69 ng	88462	Chrysene-d12	21.711

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Trifluoroacetoxy hexadecane	338	C18H33F3O2	006222-03-3	94
2			Dichloroacetic acid, heptadecyl ...	366	C19H36Cl2O2	1000282-98-2	94
3			1-Heneicosanol	312	C21H44O	015594-90-8	91
4			Pentafluoropropionic acid, penta...	374	C18H31F5O2	959092-08-1	91
5			Trichloroacetic acid, hexadecyl ...	386	C18H33Cl3O2	074339-54-1	91

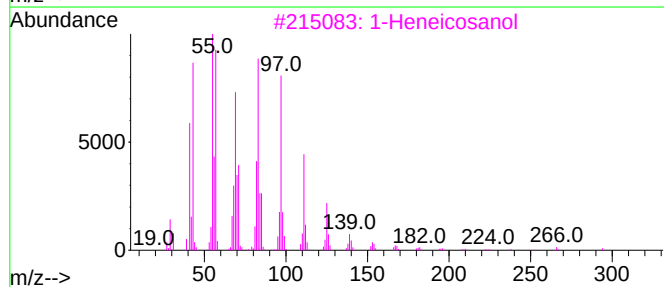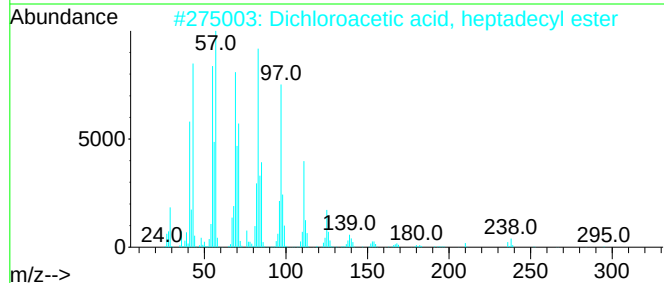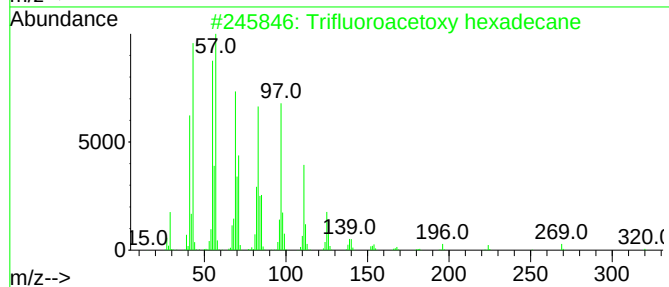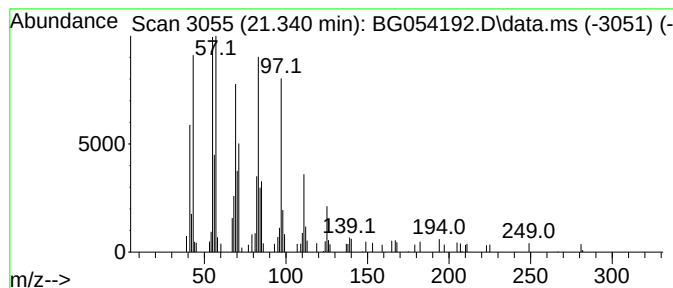

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070122\
Data File : BG054192.D
Acq On : 1 Jul 2022 15:37
Operator : CG/JU
Sample : N3561-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
S-3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Trifluoroacetox...	21.340	4.7	ng	88462	5	21.711	377636	20.0