
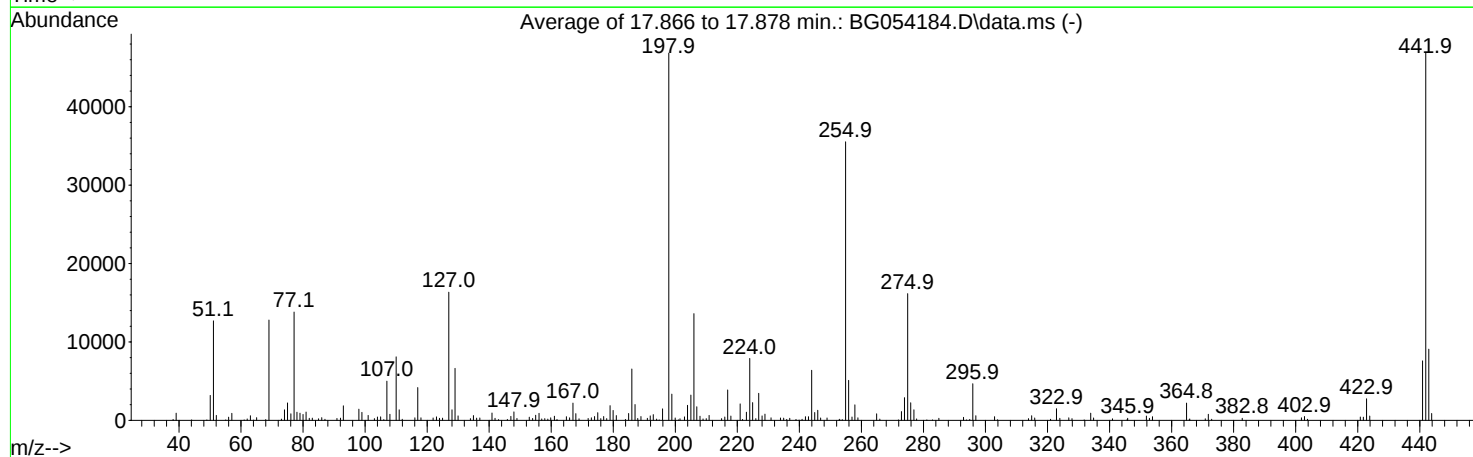


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070122\
 Data File : BG054184.D
 Acq On : 1 Jul 2022 10:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 27 00:27:54 2022

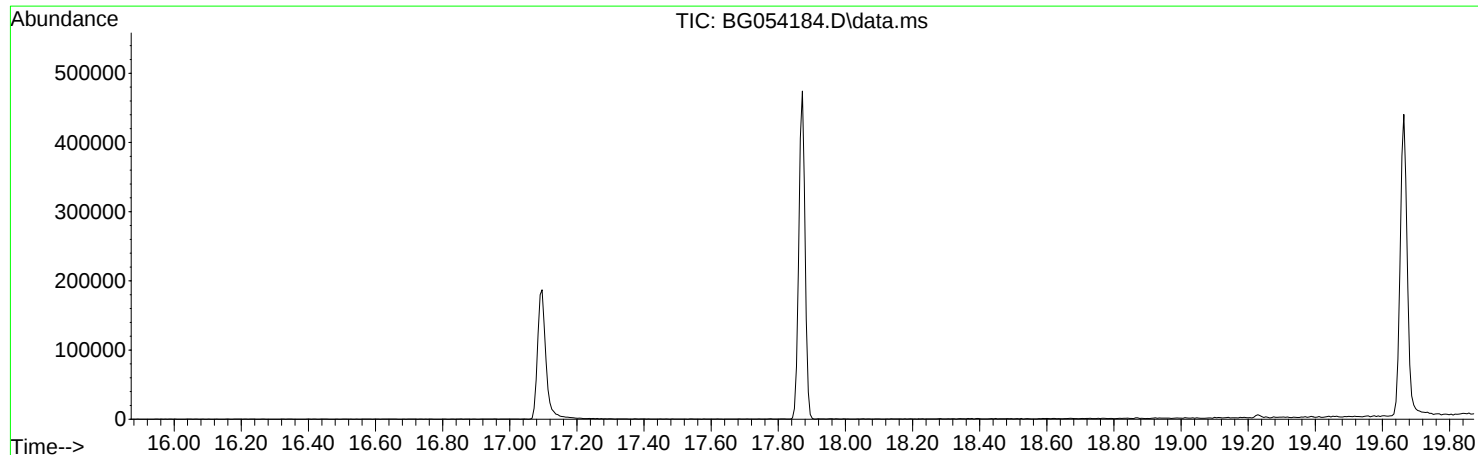




AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.1	12687	PASS
68	69	0.00	2	0.7	94	PASS
69	198	0.00	100	27.3	12802	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	34.9	16356	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	46829	PASS
199	198	5	9	7.1	3342	PASS
275	198	10	60	34.5	16171	PASS
365	198	1	100	4.7	2210	PASS
441	198	0.01	100	16.2	7600	PASS
442	442	50	100	100.0	46915	PASS
443	442	15	24	19.3	9076	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070122\
Data File : BG054184.D
Acq On : 1 Jul 2022 10:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 02 04:10:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 00:27:54 2022
Response via : Initial Calibration

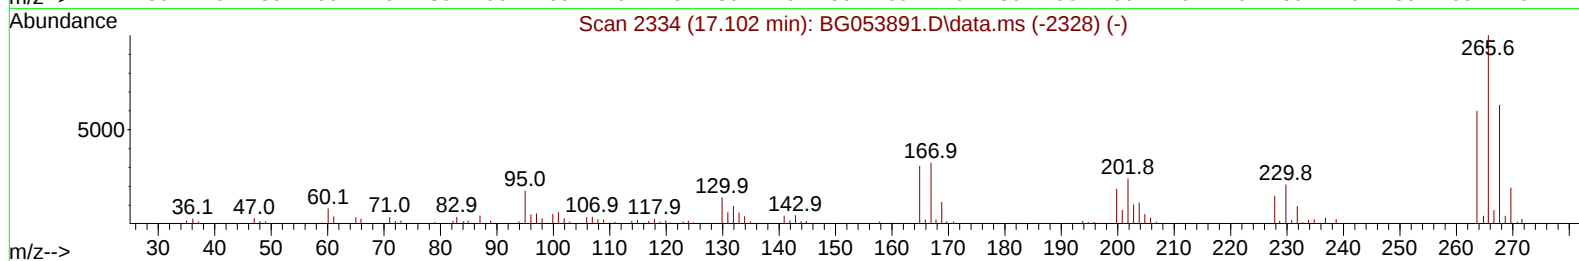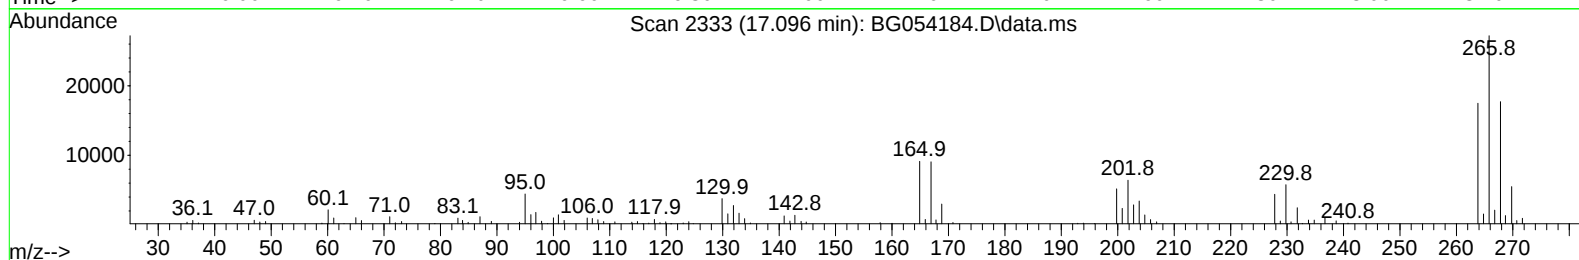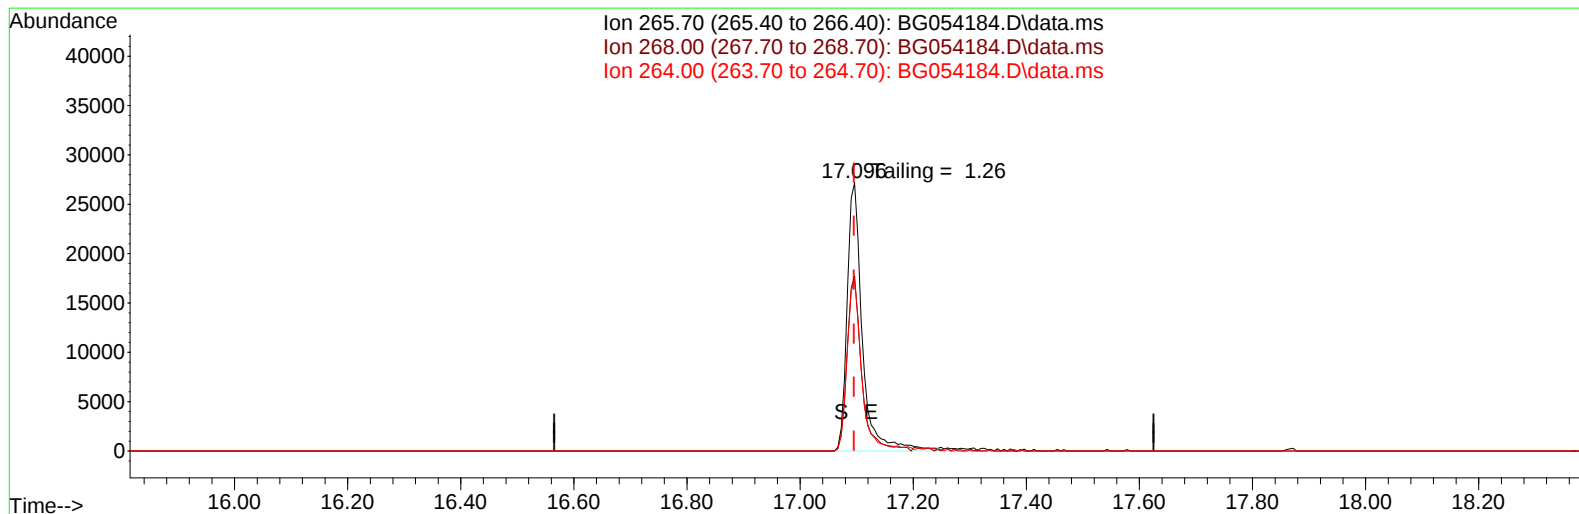

TIC: BG054184.D\data.ms

(70) Pentachlorophenol (C)

17.096min (+ 0.001) 29775.97 ng




response 50587

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	70.09
264.00	66.20	64.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070122\
Data File : BG054184.D
Acq On : 1 Jul 2022 10:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 02 04:10:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 00:27:54 2022
Response via : Initial Calibration

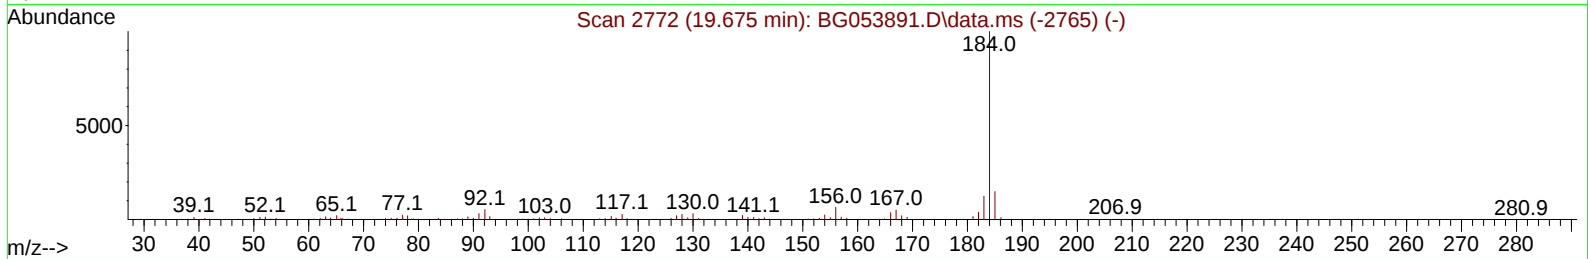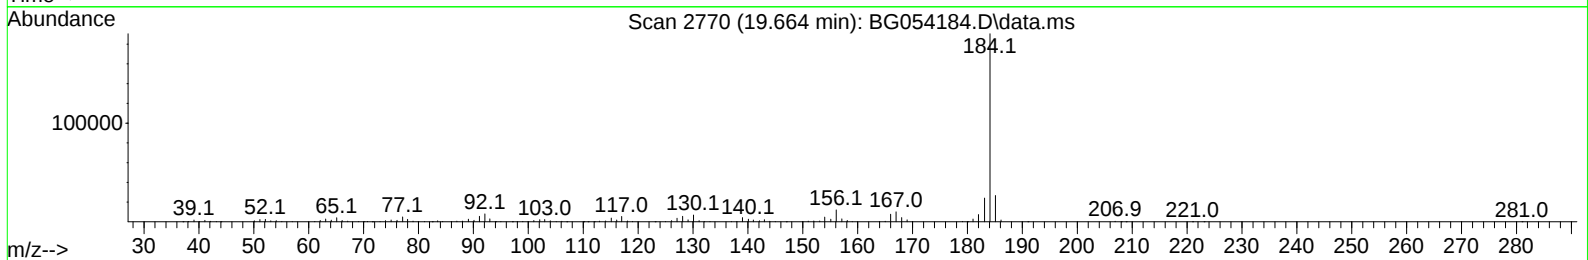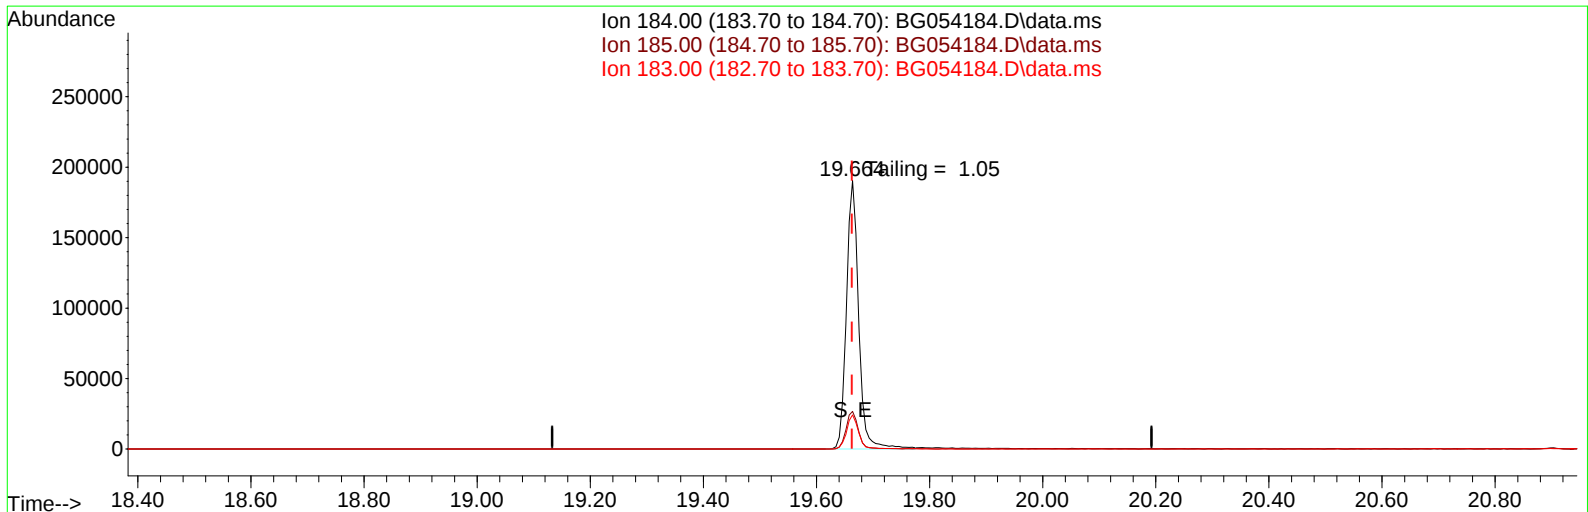

TIC: BG054184.D\data.ms

(77) Benzidine

19.664min (+ 0.001) 246936.32 ng

response 286372

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.01
183.00	11.10	12.71
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/1/2022	BNA_G	<u>BG054184.D</u>
Compound Name	Response	Retention Time
DDT	161862	20.903
DDD	4852	20.457
DDE	819	19.952
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5671	167533	3.39

Instrument :
BNA_G
ClientSampleId :
DFTPP