


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070218\
 Data File : BG035550.D
 Acq On : 2 Jul 2018 14:25
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG060718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 08 17:16:28 2018

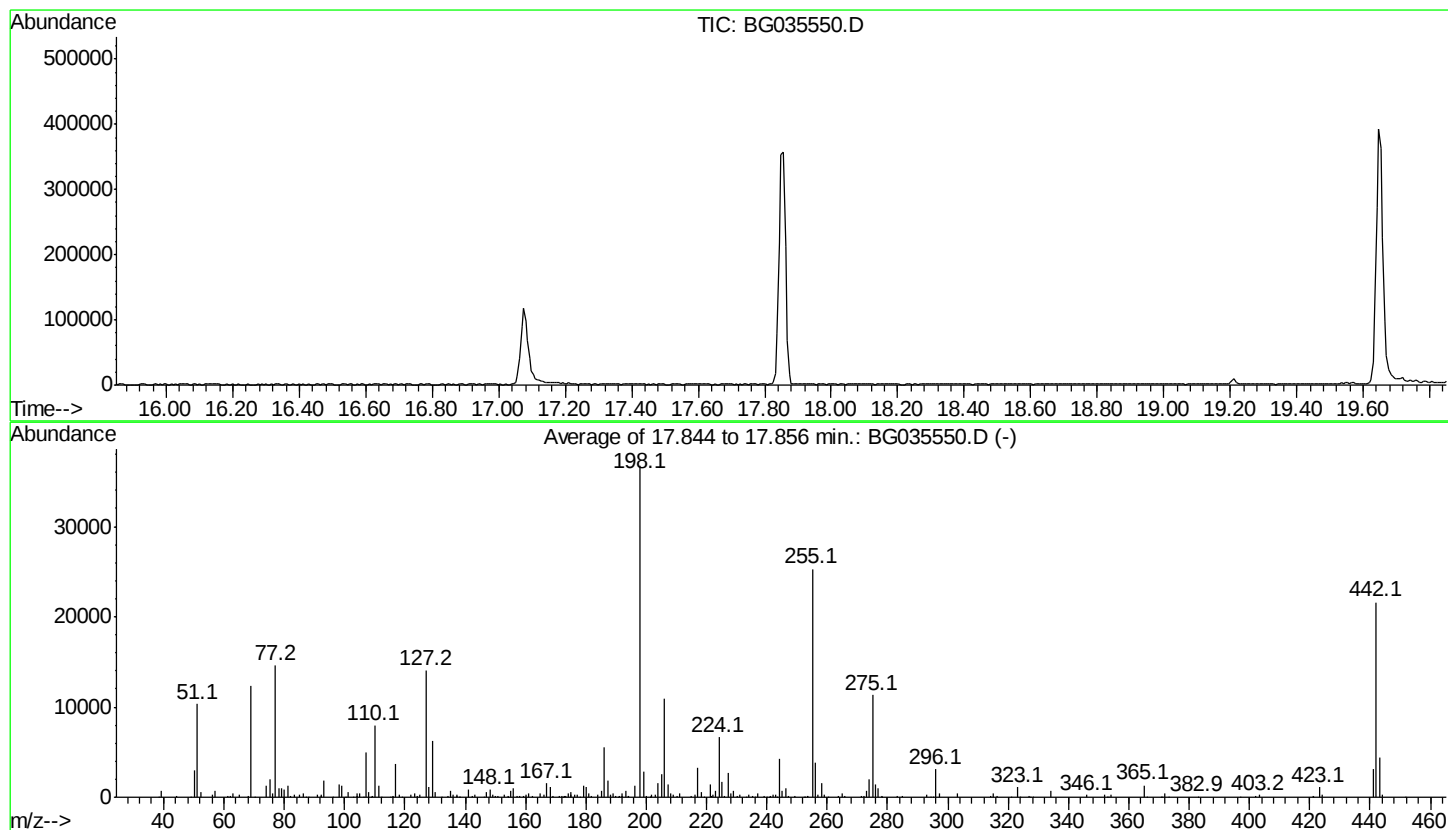

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.0	10293	PASS
68	69	0.00	2	1.7	208	PASS
69	198	0.00	100	33.8	12405	PASS
70	69	0.00	2	0.5	57	PASS
127	198	10	80	38.1	13998	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	36754	PASS
199	198	5	9	7.7	2817	PASS
275	198	10	60	30.8	11335	PASS
365	198	1	100	3.5	1294	PASS
441	443	0.01	100	69.5	3090	PASS
442	198	50	100	58.8	21608	PASS
443	442	15	24	20.6	4447	PASS