

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070323\
 Data File : BG057948.D
 Acq On : 3 Jul 2023 10:04
 Operator : CG/JU
 Sample : PB153507BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK507

Quant Time: Jul 04 00:52:53 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 07:50:15 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.930	152	30849	20.000	ng/ul	0.00
20) Naphthalene-d8	10.739	136	139798	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.569	164	101596	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.313	188	267235	20.000	ng/ul	0.00
79) Chrysene-d12	21.561	240	252126	20.000	ng/ul	0.00
88) Perylene-d12	24.722	264	303622	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.371	96	6464	7.337	ng/uL	0.00
4) Pyridine-d5	3.776	84	92896	34.733	ng/ul	0.00
7) Phenol-d5	7.090	99	103337	32.801	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.260	67	69455	36.583	ng/ul	0.00
11) 2-Chlorophenol-d4	7.466	132	77785	35.798	ng/ul	0.00
15) 4-Methylphenol-d8	8.635	113	81115	34.122	ng/ul	0.00
21) Nitrobenzene-d5	9.093	128	40935	35.926	ng/ul	0.00
24) 2-Nitrophenol-d4	9.816	143	42950	35.866	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.357	165	74187	32.294	ng/ul	0.00
31) 4-Chloroaniline-d4	10.868	131	123785	35.540	ng/ul	0.00
46) Dimethylphthalate-d6	13.970	166	314124	39.187	ng/ul	0.00
49) Acenaphthylene-d8	14.264	160	323467	36.979	ng/ul	0.00
54) 4-Nitrophenol-d4	14.757	143	47932	33.844	ng/ul	0.00
60) Fluorene-d10	15.556	176	256102	37.619	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.668	200	41459	28.571	ng/ul	0.00
73) Anthracene-d10	17.407	188	472226	38.082	ng/ul	0.00
81) Pyrene-d10	19.699	212	601970	37.910	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.505	264	610122	39.442	ng/ul	0.00
Target Compounds						
17) N-Nitroso-di-n-propyla...	8.635	70	2144	1.017	ng/ul#	Qvalue 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070323\
Data File : BG057948.D
Acq On : 3 Jul 2023 10:04
Operator : CG/JU
Sample : PB153507BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK507


Quant Time: Jul 04 00:52:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jul 02 07:50:15 2023
Response via : Initial Calibration

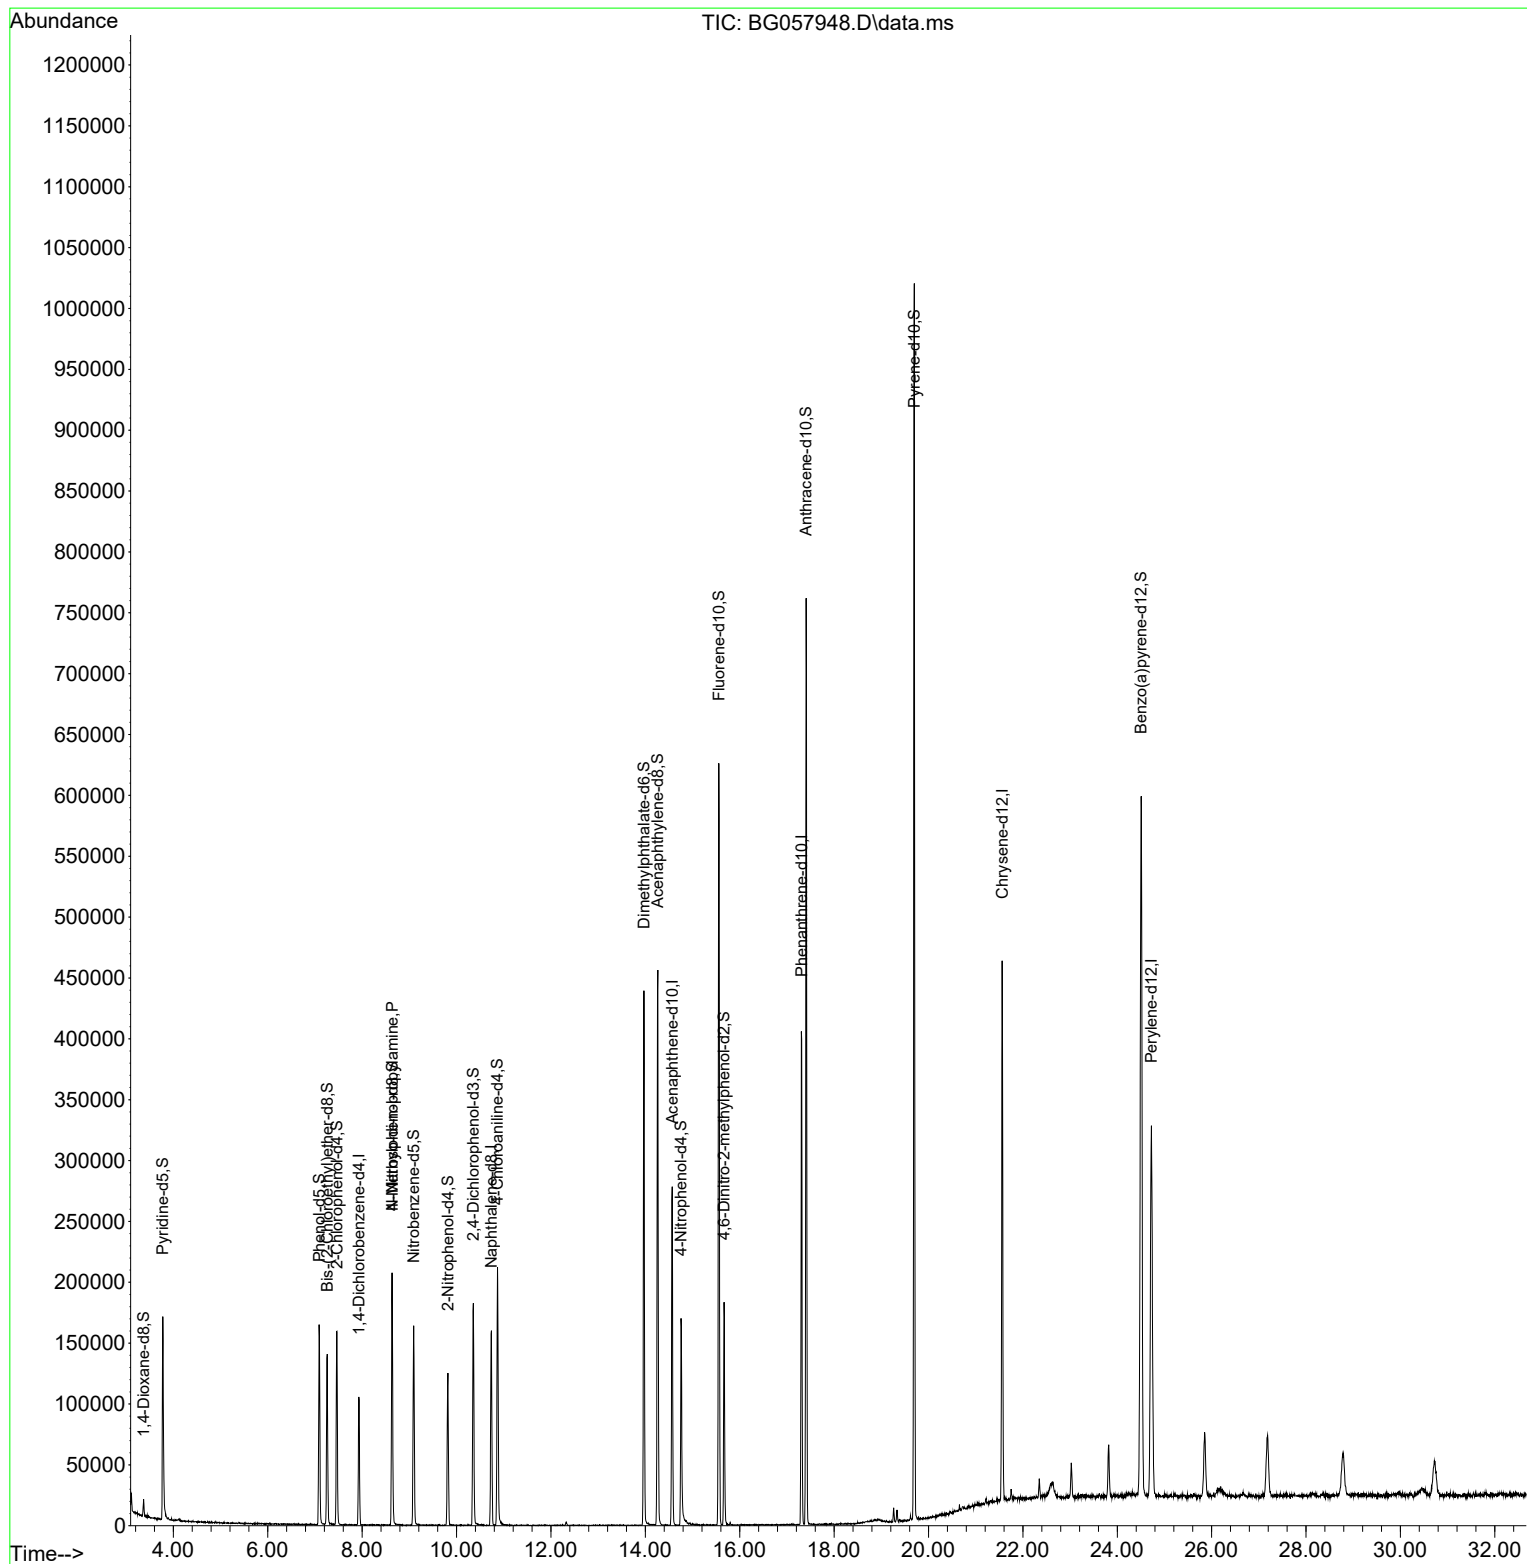

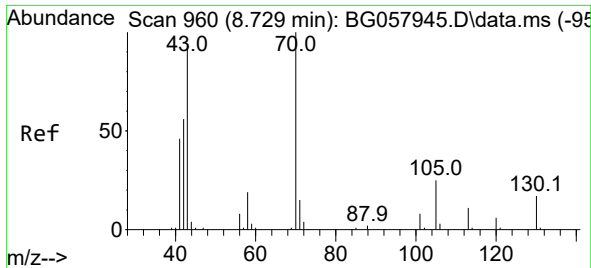

#17
N-Nitroso-di-n-propylamine
Concen: 1.017 ng/ul
RT: 8.635 min Scan# 94
Delta R.T. -0.093 min
Lab File: BG057948.D
Acq: 3 Jul 2023 10:04

Instrument :
BNA_G
ClientSampleId :
SBLK507

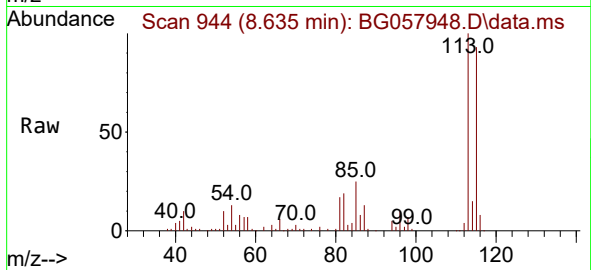

Tgt Ion: 70 Resp: 2144
Ion Ratio Lower Upper
70 100
42 373.4 48.0 72.0#
101 0.0 7.4 11.2#
130 0.0 13.4 20.0#

