

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070323\
 Data File : BG057959.D
 Acq On : 3 Jul 2023 17:40
 Operator : CG/JU
 Sample : PB153507BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK507

Quant Time: Jul 04 00:55:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 07:50:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.935	152	36672	20.000	ng/ul	0.00
20) Naphthalene-d8	10.738	136	170329	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.568	164	124633	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.306	188	316374	20.000	ng/ul	0.00
79) Chrysene-d12	21.560	240	266069	20.000	ng/ul	0.00
88) Perylene-d12	24.715	264	319421	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.376	96	7529	7.189	ng/uL	0.01
4) Pyridine-d5	3.781	84	108430	34.104	ng/ul	0.00
7) Phenol-d5	7.095	99	130691	34.896	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.259	67	81439	36.084	ng/ul	0.00
11) 2-Chlorophenol-d4	7.465	132	97422	37.716	ng/ul	0.00
15) 4-Methylphenol-d8	8.640	113	101196	35.810	ng/ul	0.00
21) Nitrobenzene-d5	9.092	128	50413	36.314	ng/ul	0.00
24) 2-Nitrophenol-d4	9.815	143	54383	37.273	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.356	165	98692	35.260	ng/ul	0.00
31) 4-Chloroaniline-d4	10.873	131	148930	35.095	ng/ul	0.00
46) Dimethylphthalate-d6	13.969	166	348283	35.417	ng/ul	0.00
49) Acenaphthylene-d8	14.263	160	396320	36.933	ng/ul	0.00
54) 4-Nitrophenol-d4	14.762	143	61144	35.193	ng/ul	0.00
60) Fluorene-d10	15.555	176	314584	37.668	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.673	200	55053	32.046	ng/ul	0.00
73) Anthracene-d10	17.406	188	547020	37.262	ng/ul	0.00
81) Pyrene-d10	19.698	212	641354	38.273	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.504	264	651150	40.012	ng/ul	0.00


Target Compounds					Qvalue	
17) N-Nitroso-di-n-propyla...	8.634	70	2609	1.041	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070323\
Data File : BG057959.D
Acq On : 3 Jul 2023 17:40
Operator : CG/JU
Sample : PB153507BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK507


Quant Time: Jul 04 00:55:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jul 02 07:50:15 2023
Response via : Initial Calibration

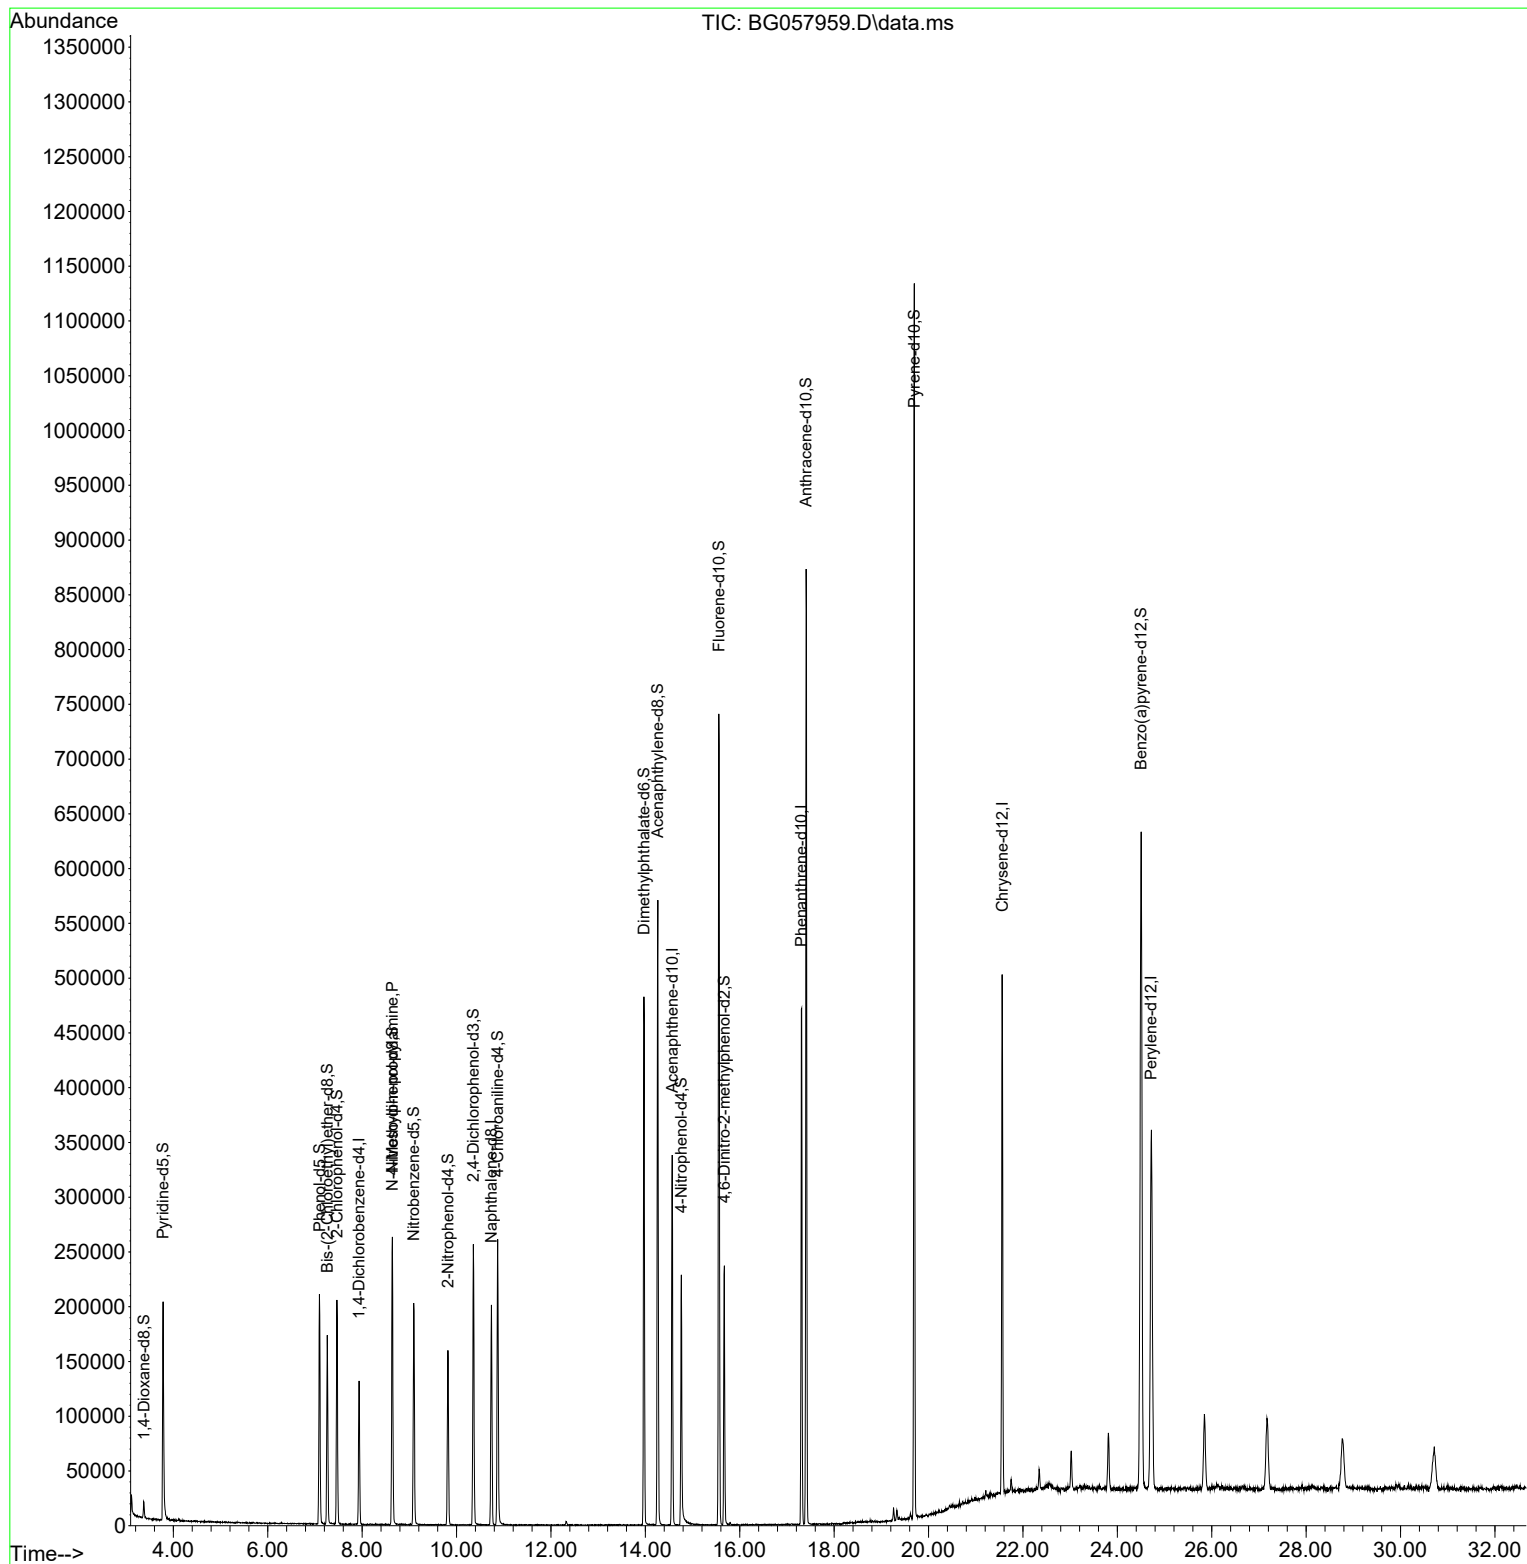

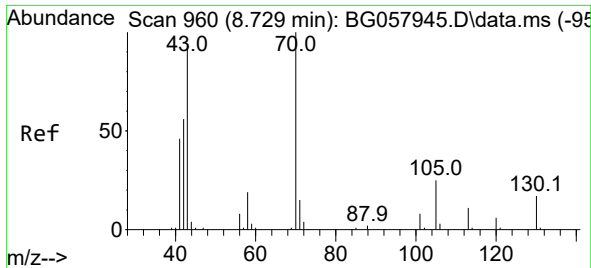

#17
 N-Nitroso-di-n-propylamine
 Concen: 1.041 ng/ul
 RT: 8.634 min Scan# 94
 Delta R.T. -0.094 min
 Lab File: BG057959.D
 Acq: 3 Jul 2023 17:40

Instrument :
 BNA_G
 ClientSampleId :
 SBLK507

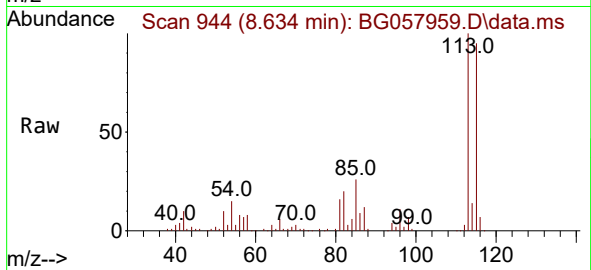

Tgt Ion:	70	Resp:	2609
Ion	Ratio	Lower	Upper
70	100		
42	347.0	48.0	72.0#
101	0.0	7.4	11.2#
130	0.0	13.4	20.0#

