

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070323\
 Data File : BG057982.D
 Acq On : 4 Jul 2023 10:32
 Operator : CG/JU
 Sample : 03247-22
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCGM8

Quant Time: Jul 05 00:12:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 04 05:09:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.942	152	40849	20.000	ng/ul	0.00
20) Naphthalene-d8	10.744	136	188261	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.575	164	127792	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.319	188	277321	20.000	ng/ul	0.00
79) Chrysene-d12	21.567	240	222964	20.000	ng/ul	0.00
88) Perylene-d12	24.734	264	271348	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.376	96	3993	3.423	ng/uL	0.00
4) Pyridine-d5	3.788	84	45679	12.898	ng/ul	0.00
7) Phenol-d5	7.107	99	79806	19.130	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.266	67	54952	21.858	ng/ul	0.00
11) 2-Chlorophenol-d4	7.472	132	63067	21.919	ng/ul	0.00
15) 4-Methylphenol-d8	8.647	113	38522	12.238	ng/ul	0.00
21) Nitrobenzene-d5	9.099	128	33925	22.109	ng/ul	0.00
24) 2-Nitrophenol-d4	9.822	143	37187	23.060	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.368	165	64270	20.775	ng/ul	0.00
31) 4-Chloroaniline-d4	10.879	131	48605	10.363	ng/ul	0.00
46) Dimethylphthalate-d6	13.976	166	221148	21.933	ng/ul	0.00
49) Acenaphthylene-d8	14.270	160	259641	23.598	ng/ul	0.00
54) 4-Nitrophenol-d4	14.775	143	31278	17.558	ng/ul	0.00
60) Fluorene-d10	15.562	176	200245	23.385	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.680	200	21628	14.363	ng/ul	0.00
73) Anthracene-d10	17.413	188	249027	19.352	ng/ul	0.00
81) Pyrene-d10	19.704	212	344413	24.527	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.516	264	335303	24.254	ng/ul	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.449	149	9616	1.010	ng/ul#	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070323\
Data File : BG057982.D
Acq On : 4 Jul 2023 10:32
Operator : CG/JU
Sample : 03247-22
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCGM8

Quant Time: Jul 05 00:12:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 04 05:09:13 2023
Response via : Initial Calibration

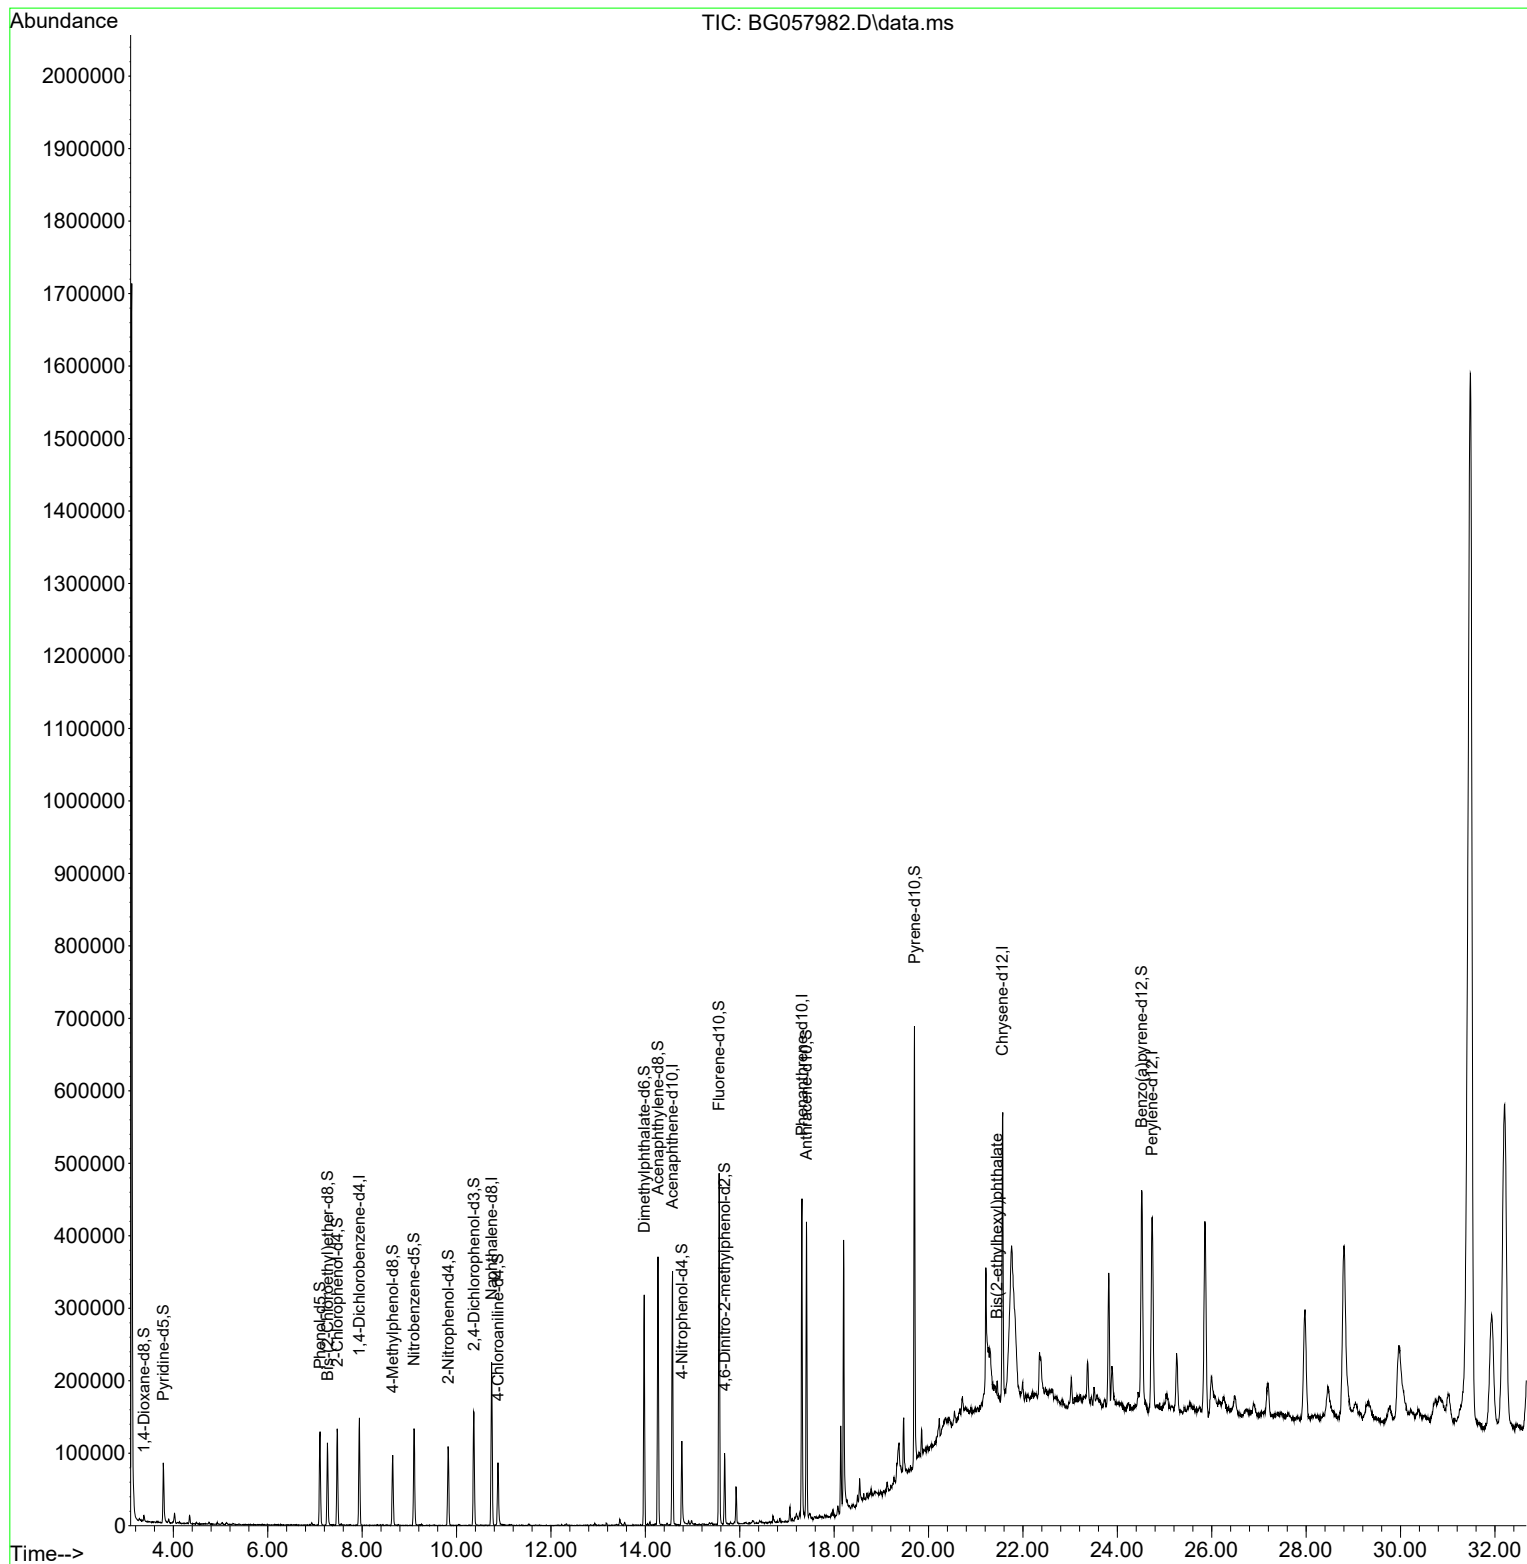

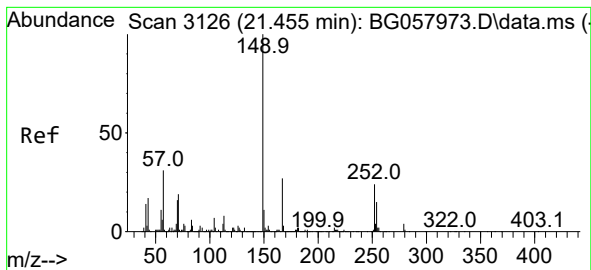

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.010 ng/ul
 RT: 21.449 min Scan# 31
 Delta R.T. -0.005 min
 Lab File: BG057982.D
 Acq: 4 Jul 2023 10:32

Instrument :
 BNA_G
 ClientSampleId :
 DCGM8

Tgt Ion:149 Resp: 9616
 Ion Ratio Lower Upper
 149 100
 167 28.5 20.9 31.3
 279 6.2 3.1 4.7#

