

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070323\
 Data File : BG057999.D
 Acq On : 4 Jul 2023 23:11
 Operator : CG/JU
 Sample : 03248-19
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCGK2

Quant Time: Jul 05 00:15:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 04 05:09:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.944	152	39545	20.000	ng/ul	0.00
20) Naphthalene-d8	10.746	136	183616	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.577	164	125765	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.315	188	276701	20.000	ng/ul	0.00
79) Chrysene-d12	21.569	240	228577	20.000	ng/ul	0.00
88) Perylene-d12	24.741	264	273256	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.372	96	2641	2.339	ng/uL	0.00
4) Pyridine-d5	3.795	84	2312	0.674	ng/ul	0.00
7) Phenol-d5	7.103	99	52687	13.046	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.268	67	33214	13.647	ng/ul	0.00
11) 2-Chlorophenol-d4	7.473	132	40604	14.578	ng/ul	0.00
15) 4-Methylphenol-d8	8.649	113	25405	8.337	ng/ul	0.00
21) Nitrobenzene-d5	9.101	128	21782	14.555	ng/ul	0.00
24) 2-Nitrophenol-d4	9.824	143	22843	14.523	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.370	165	41094	13.620	ng/ul	0.00
31) 4-Chloroaniline-d4	10.881	131	36186	7.910	ng/ul	0.00
46) Dimethylphthalate-d6	13.978	166	138222	13.929	ng/ul	0.00
49) Acenaphthylene-d8	14.271	160	159277	14.709	ng/ul	0.00
54) 4-Nitrophenol-d4	14.783	143	15833	9.031	ng/ul	0.00
60) Fluorene-d10	15.564	176	124432	14.765	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.682	200	13153	8.754	ng/ul	0.00
73) Anthracene-d10	17.415	188	166889	12.998	ng/ul	0.00
81) Pyrene-d10	19.700	212	220583	15.323	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.518	264	210849	15.145	ng/ul	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.457	149	13952	1.430	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070323\
Data File : BG057999.D
Acq On : 4 Jul 2023 23:11
Operator : CG/JU
Sample : 03248-19
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCGK2


Quant Time: Jul 05 00:15:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 04 05:09:13 2023
Response via : Initial Calibration

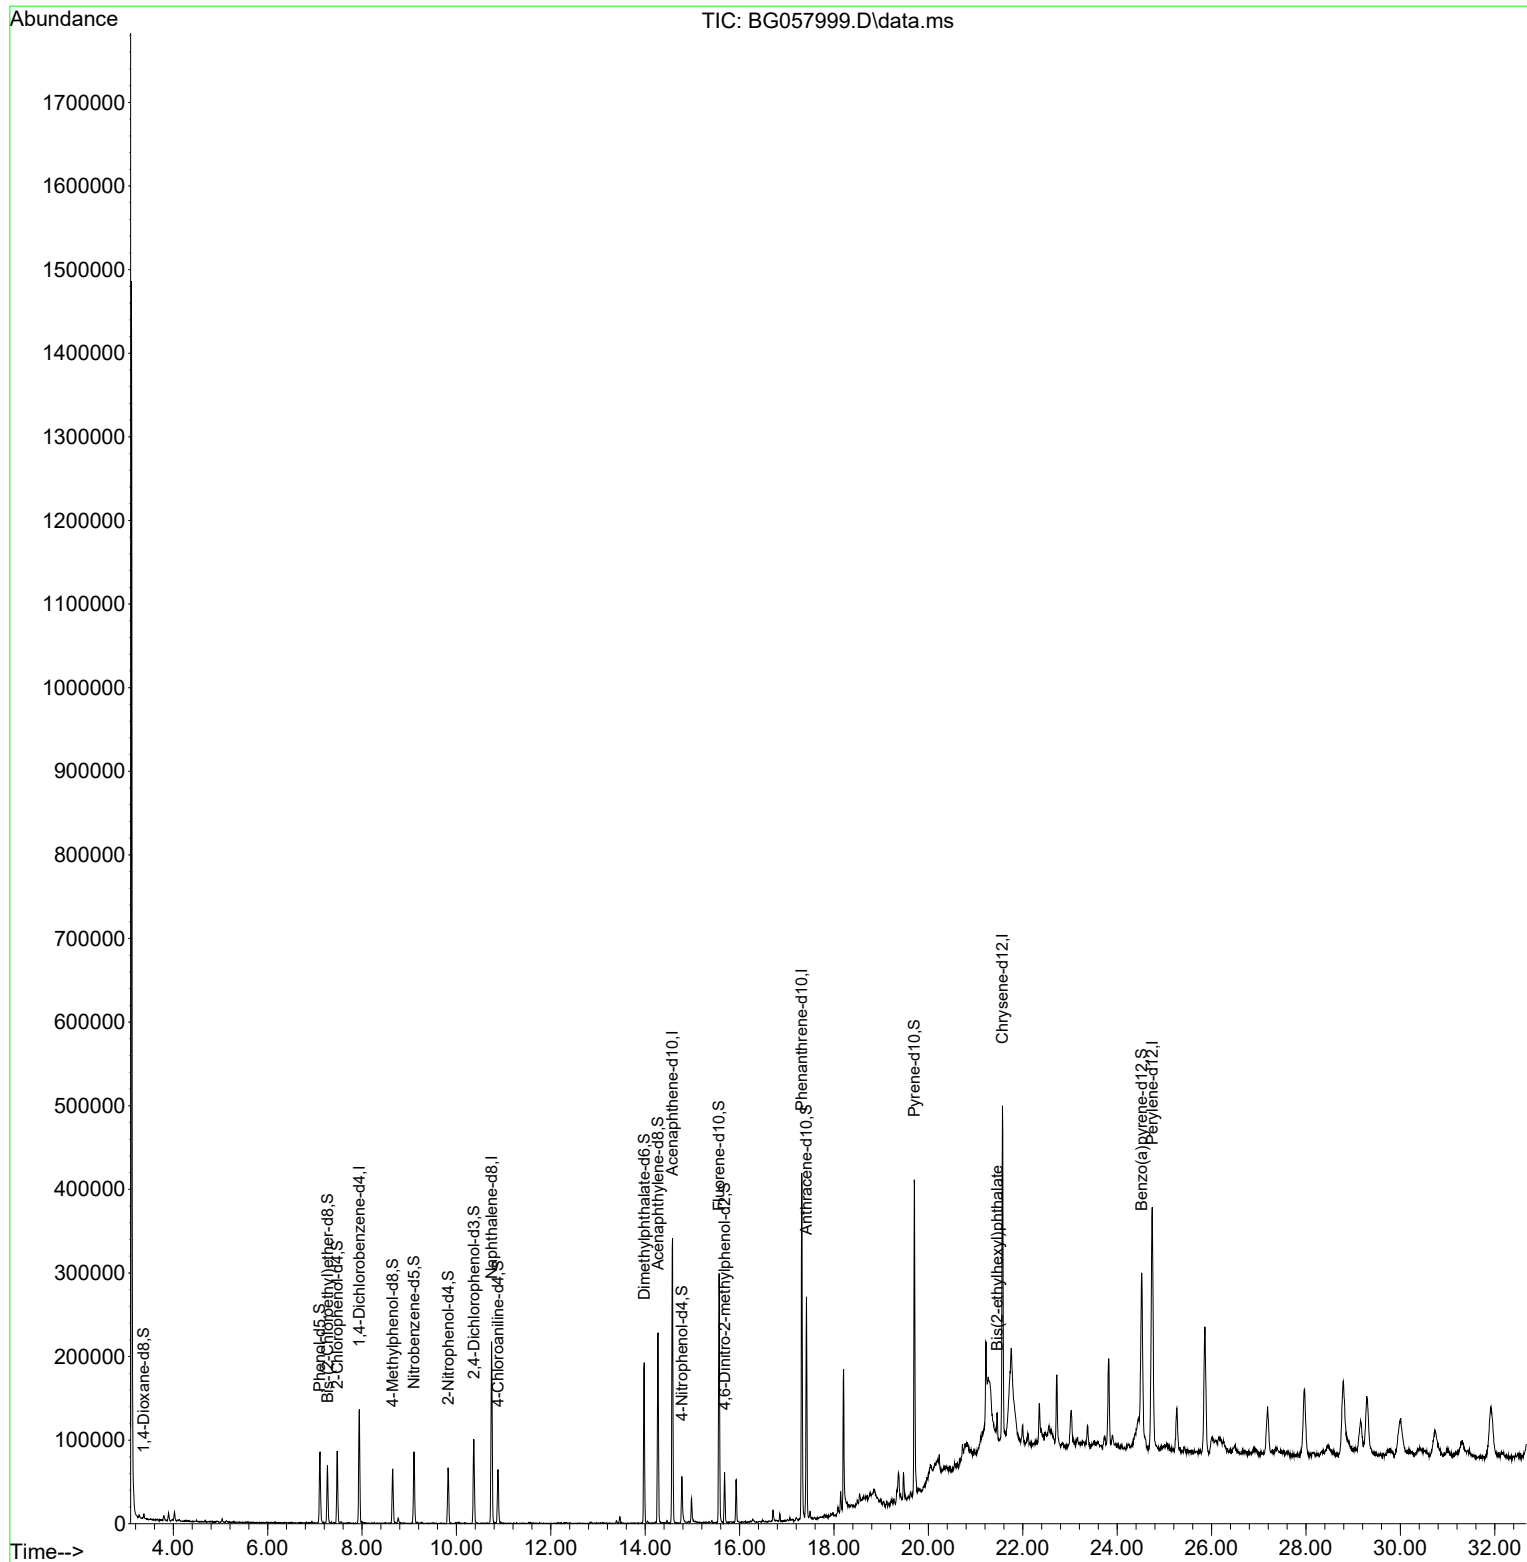

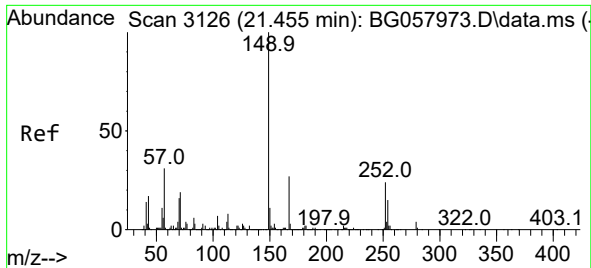

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.430 ng/ul
 RT: 21.457 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: BG057999.D
 Acq: 4 Jul 2023 23:11

Instrument :
 BNA_G
 ClientSampleId :
 DCGK2

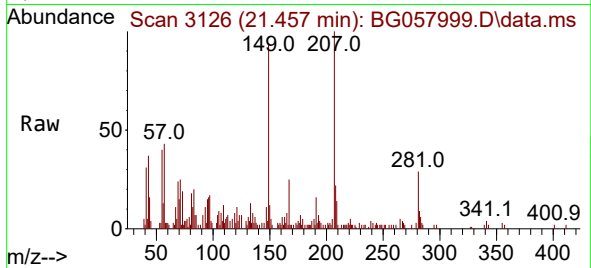

Tgt Ion:149 Resp: 13952
 Ion Ratio Lower Upper
 149 100
 167 26.8 20.9 31.3
 279 3.7 3.1 4.7

