




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070323\
 Data File : BG057949.D
 Acq On : 3 Jul 2023 10:45
 Operator : CG/JU
 Sample : 03248-15
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCGP3

Manual IntegrationsAPPROVED

Quant Time: Jul 04 00:53:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 07:50:15 2023
 Response via : Initial Calibration

Reviewed By :Sohil Jodhani 07/04/2023
 Supervised By :mohammad ahmed 07/04/2023

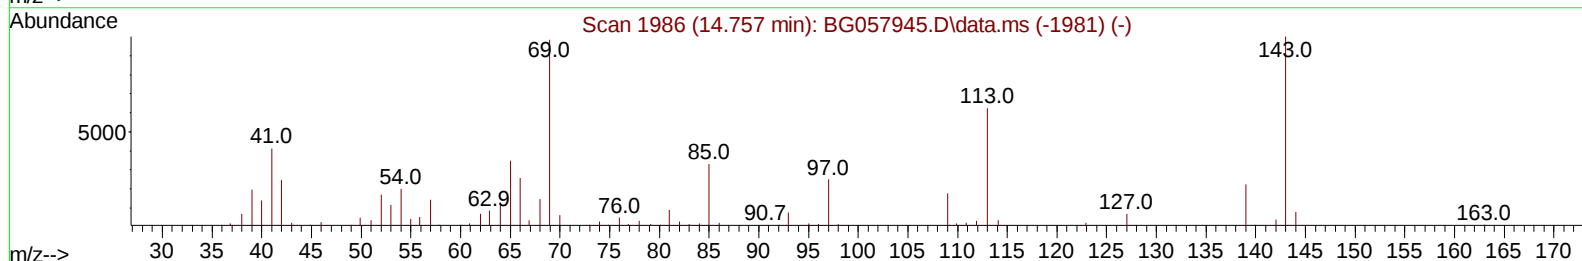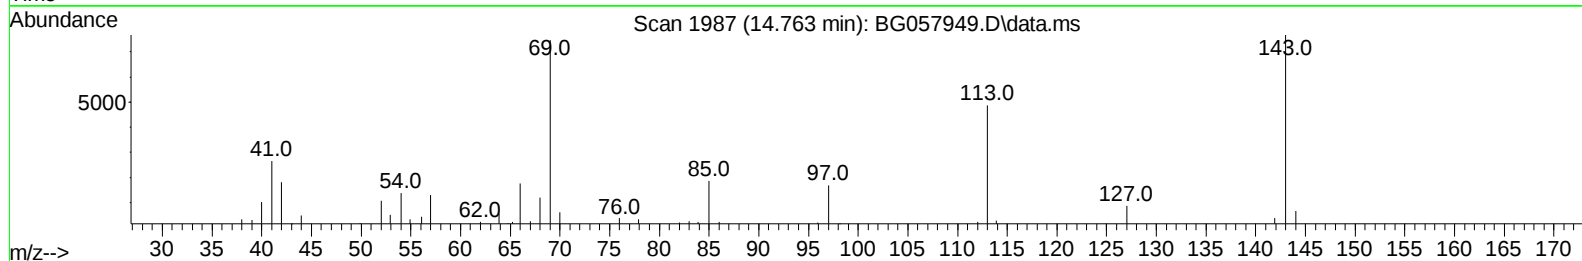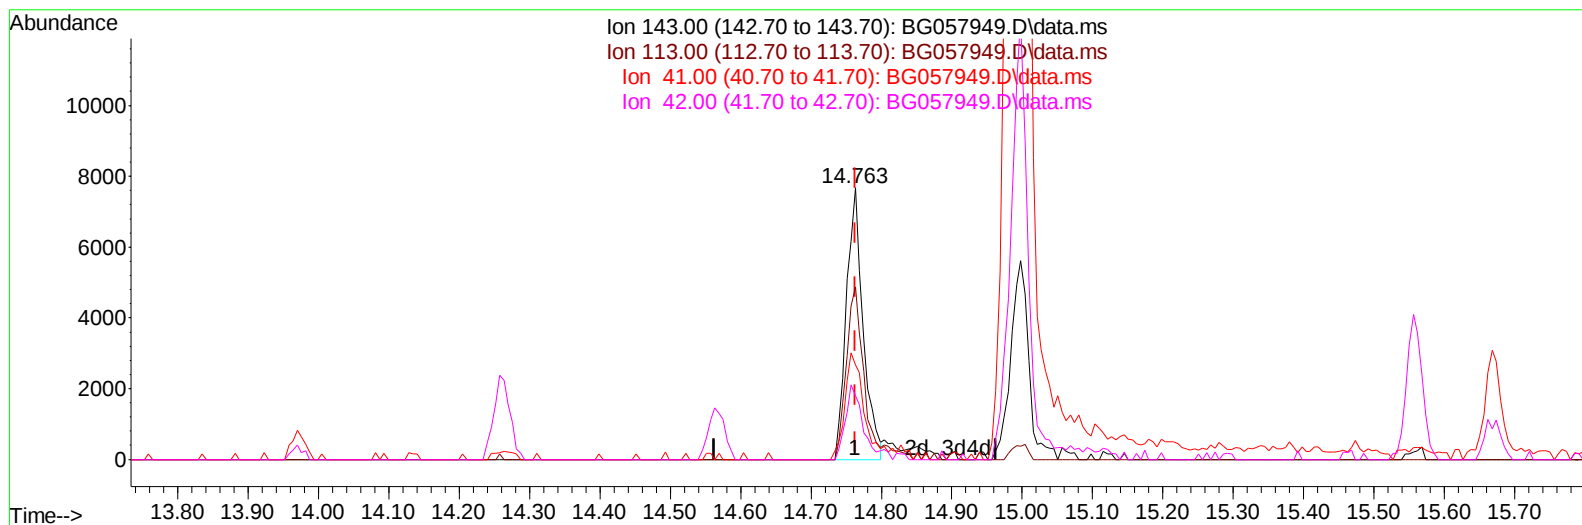

TIC: BG057949.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.763min (+ 0.000) 10.02 ng/u1

response 12585

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	66.40	63.50
41.00	40.50	34.68
42.00	27.50	23.49




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070323\
Data File : BG057949.D
Acq On : 3 Jul 2023 10:45
Operator : CG/JU
Sample : 03248-15
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCGP3

Manual IntegrationsAPPROVED

Quant Time: Jul 04 00:53:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jul 02 07:50:15 2023
Response via : Initial Calibration

Reviewed By :Sohil Jodhani 07/04/2023
Supervised By :mohammad ahmed 07/04/2023

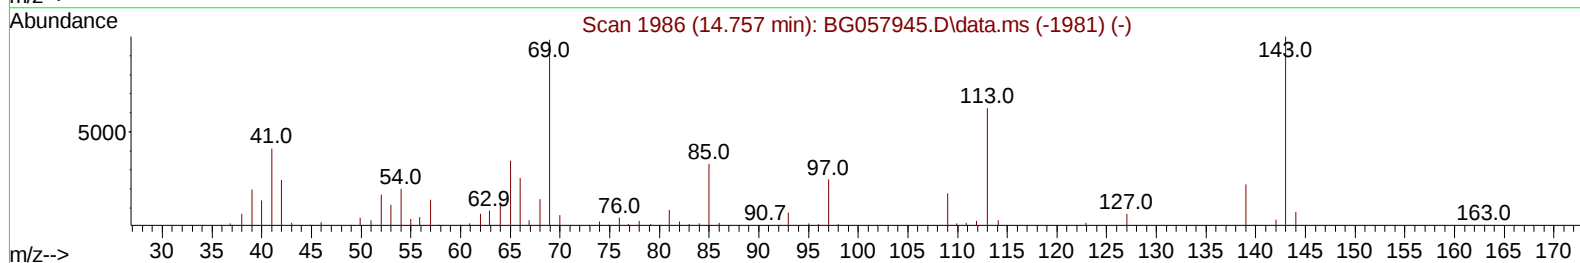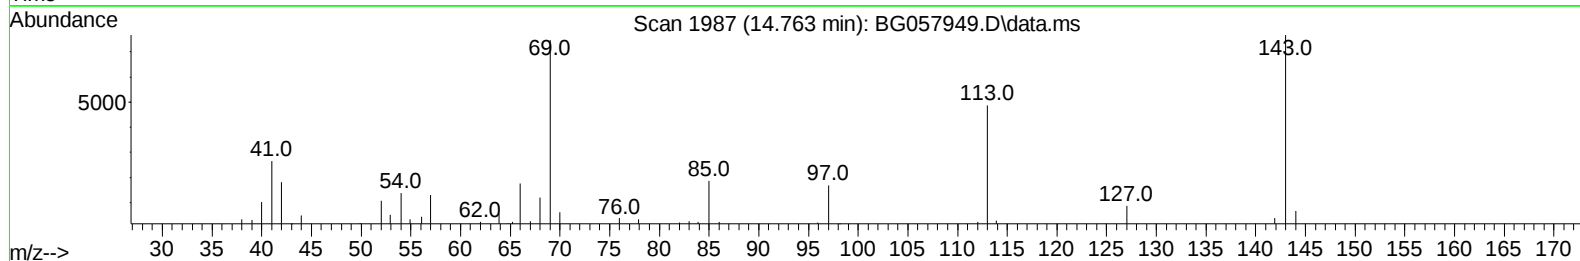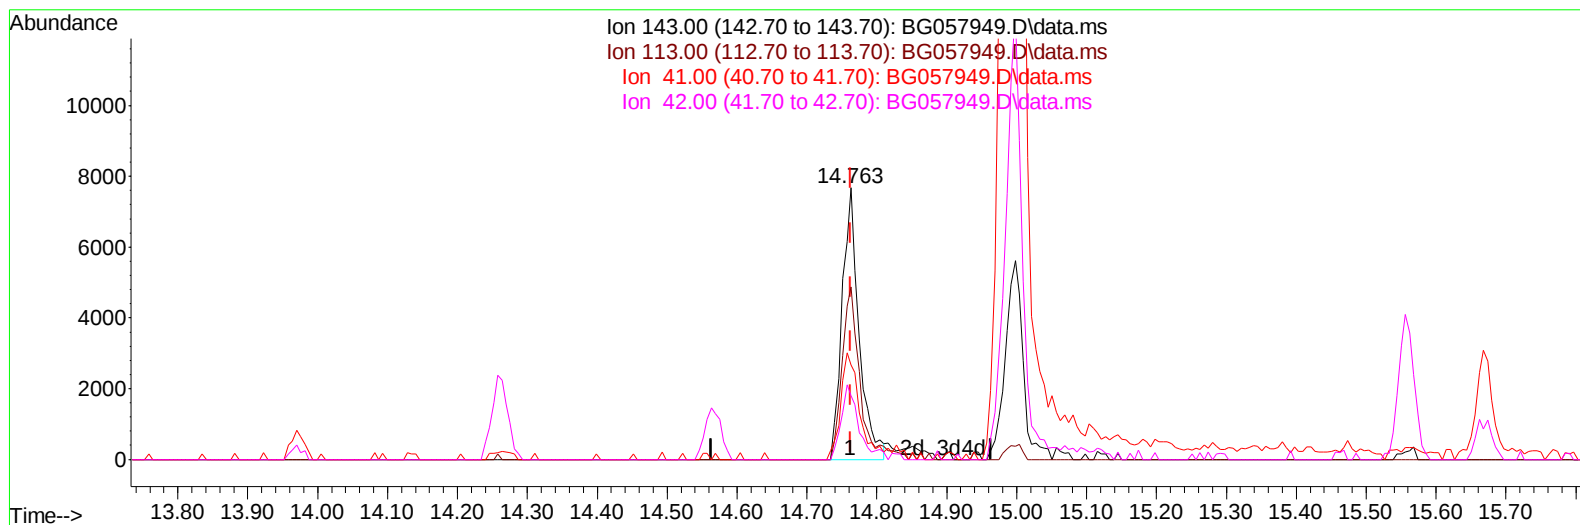

TIC: BG057949.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.763min (+ 0.000) 10.30 ng/ul m

response 12940

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	66.40	63.50
41.00	40.50	34.68
42.00	27.50	23.49

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070323\
 Data File : BG057949.D
 Acq On : 3 Jul 2023 10:45
 Operator : CG/JU
 Sample : 03248-15
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCGP3

Manual IntegrationsAPPROVED

Reviewed By :Sohil Jodhani 07/04/2023
 Supervised By :mohammad ahmed 07/04/2023

Quant Time: Jul 04 02:54:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 07:50:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.936	152	26911	20.000	ng/ul	0.00
20) Naphthalene-d8	10.738	136	123992	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.569	164	90091	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.313	188	240354	20.000	ng/ul	0.00
79) Chrysene-d12	21.561	240	221909	20.000	ng/ul	0.00
88) Perylene-d12	24.722	264	261650	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.365	96	4913	6.393	ng/uL	0.00
4) Pyridine-d5	3.782	84	25694	11.013	ng/ul	0.00
7) Phenol-d5	7.090	99	26801	9.752	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.260	67	67415	40.705	ng/ul	0.00
11) 2-Chlorophenol-d4	7.466	132	62297	32.866	ng/ul	0.00
15) 4-Methylphenol-d8	8.635	113	45667	22.022	ng/ul	0.00
21) Nitrobenzene-d5	9.093	128	41552	41.117	ng/ul	0.00
24) 2-Nitrophenol-d4	9.816	143	40490	38.122	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.356	165	72568	35.616	ng/ul	0.00
31) 4-Chloroaniline-d4	10.868	131	105361	34.107	ng/ul	0.00
46) Dimethylphthalate-d6	13.970	166	313769	44.141	ng/ul	0.00
49) Acenaphthylene-d8	14.264	160	334839	43.167	ng/ul	0.00
54) 4-Nitrophenol-d4	14.763	143	12940m	10.304	ng/ul	0.00
60) Fluorene-d10	15.556	176	270340	44.782	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.674	200	49871	38.212	ng/ul	0.00
73) Anthracene-d10	17.407	188	535850	48.045	ng/ul	0.00
81) Pyrene-d10	19.698	212	669358	47.894	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.505	264	659986	49.510	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070323\
Data File : BG057949.D
Acq On : 3 Jul 2023 10:45
Operator : CG/JU
Sample : 03248-15
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCGP3

Manual IntegrationsAPPROVED

Quant Time: Jul 04 02:54:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jul 02 07:50:15 2023
Response via : Initial Calibration

Reviewed By :Sohil Jodhani 07/04/2023
Supervised By :mohammad ahmed 07/04/2023

