




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070323\
 Data File : BG057977.D
 Acq On : 4 Jul 2023 7:02
 Operator : CG/JU
 Sample : 03247-17
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCGM3

Manual IntegrationsAPPROVED

Quant Time: Jul 04 07:45:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 04 05:09:13 2023
 Response via : Initial Calibration

Reviewed By :Sohil Jodhani 07/04/2023
 Supervised By :mohammad ahmed 07/04/2023

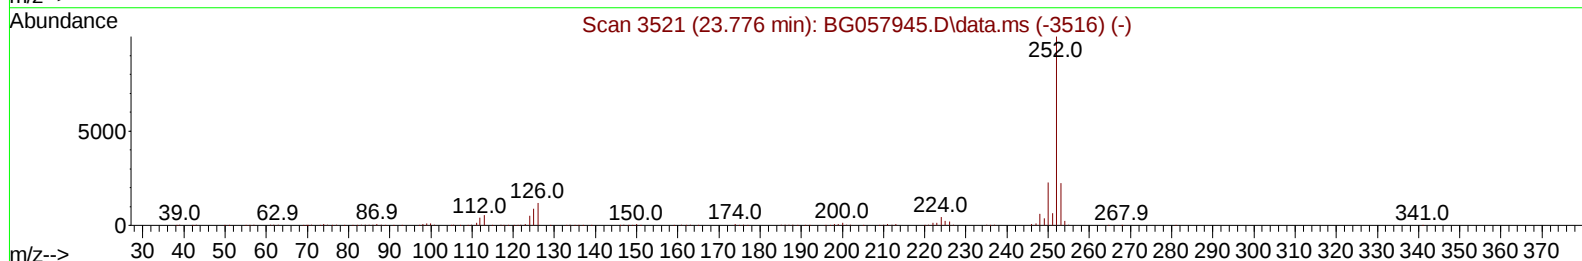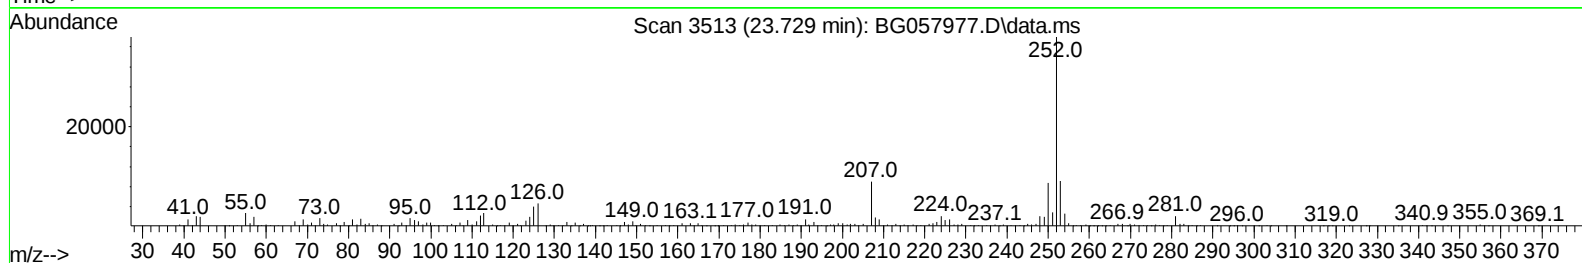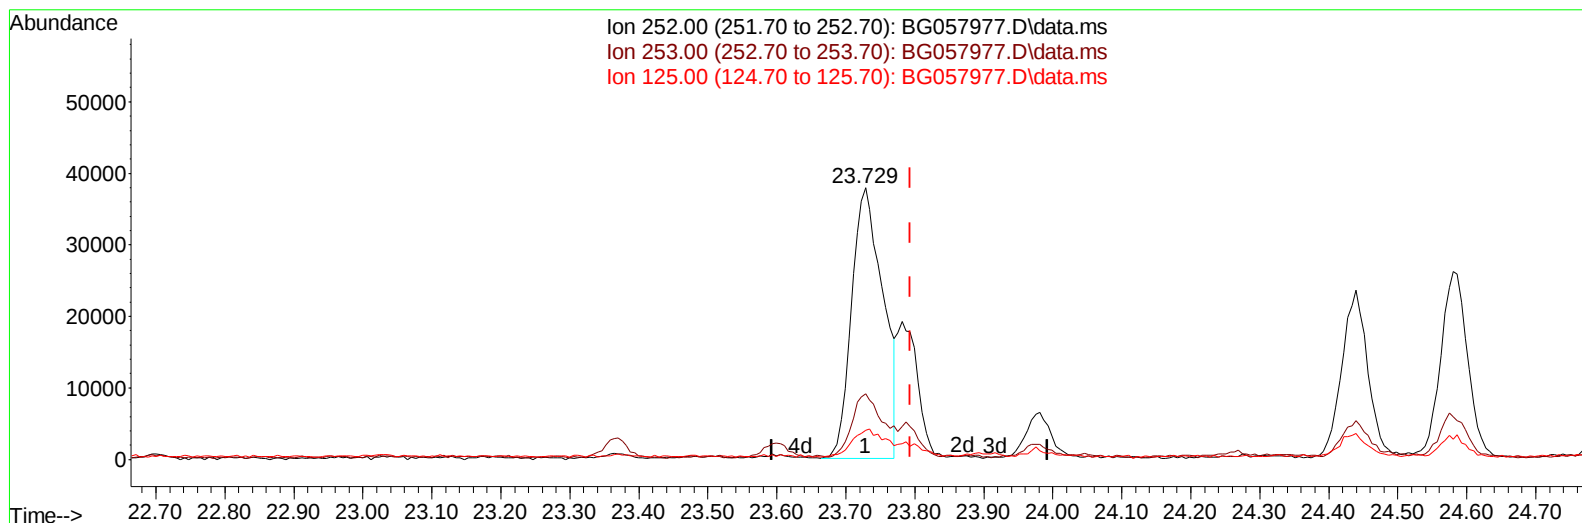

TIC: BG057977.D\data.ms

(91) Benzo(k)fluoranthene

23.729min (-0.064) 7.53 ng/u1

response 119309

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.10	24.17
125.00	9.30	10.65
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070323\
 Data File : BG057977.D
 Acq On : 4 Jul 2023 7:02
 Operator : CG/JU
 Sample : 03247-17
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCGM3

Manual IntegrationsAPPROVED

Quant Time: Jul 04 07:45:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 04 05:09:13 2023
 Response via : Initial Calibration

Reviewed By :Sohil Jodhani 07/04/2023
 Supervised By :mohammad ahmed 07/04/2023

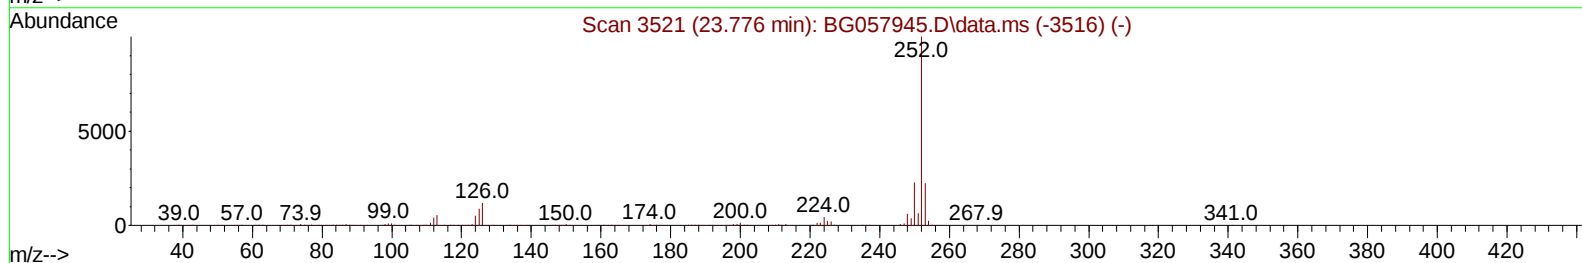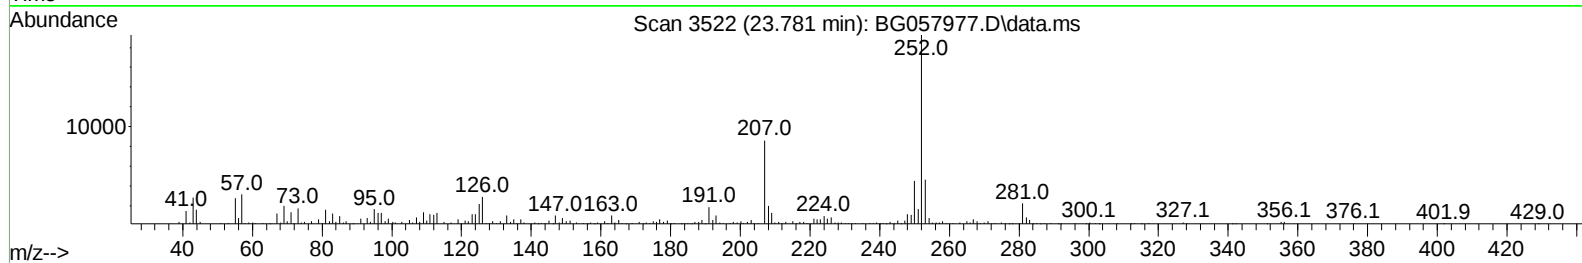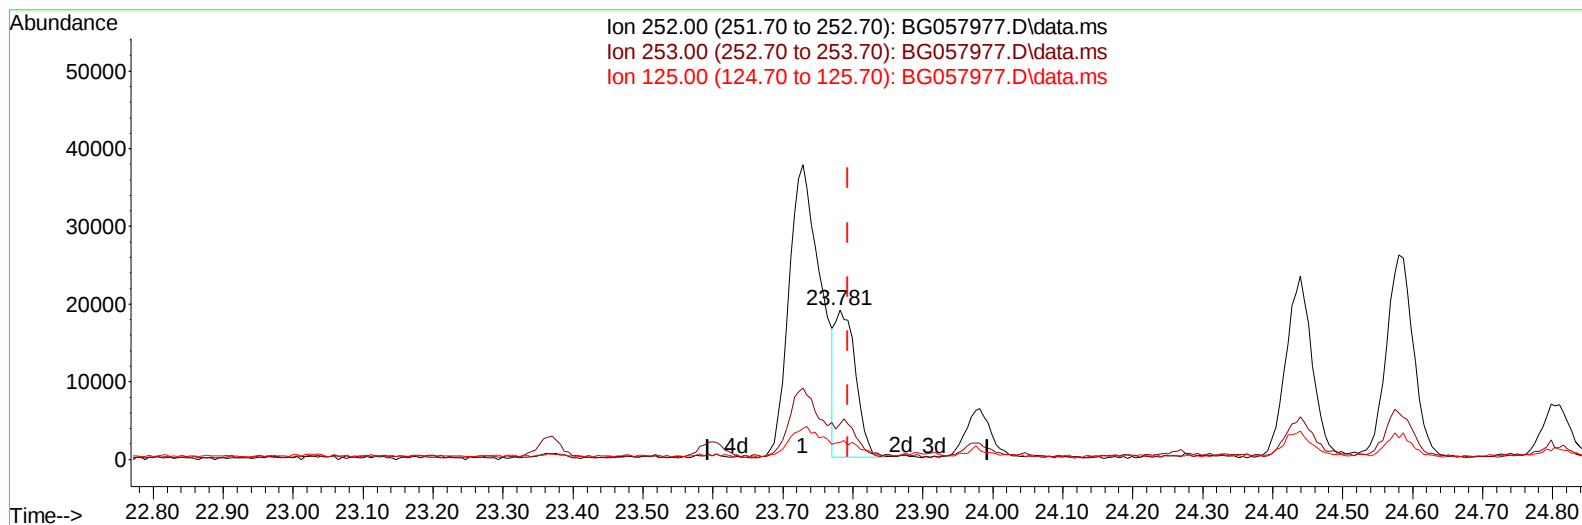

TIC: BG057977.D\data.ms

(91) Benzo(k)fluoranthene

23.781min (-0.012) 2.45 ng/ul m

response 38838

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.10	23.95
125.00	9.30	11.32#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070323\
 Data File : BG057977.D
 Acq On : 4 Jul 2023 7:02
 Operator : CG/JU
 Sample : 03247-17
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCGM3

Manual IntegrationsAPPROVED

Quant Time: Jul 04 07:45:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 04 05:09:13 2023
 Response via : Initial Calibration

Reviewed By :Sohil Jodhani 07/04/2023
 Supervised By :mohammad ahmed 07/04/2023

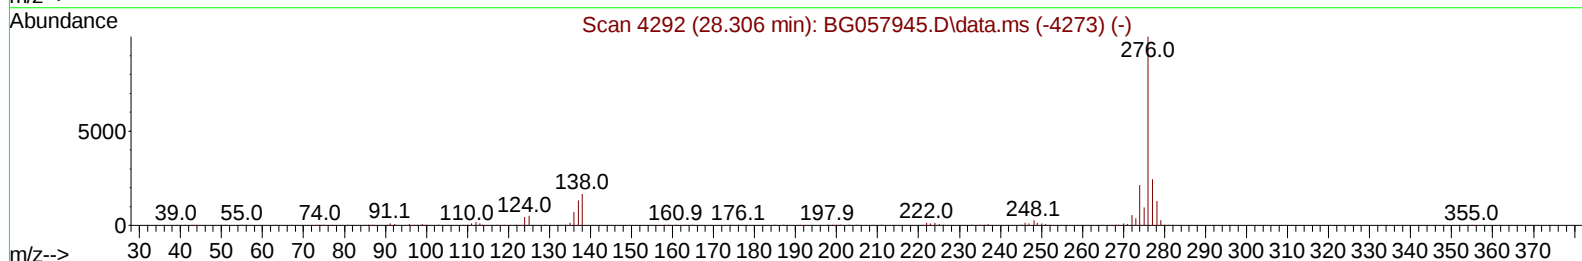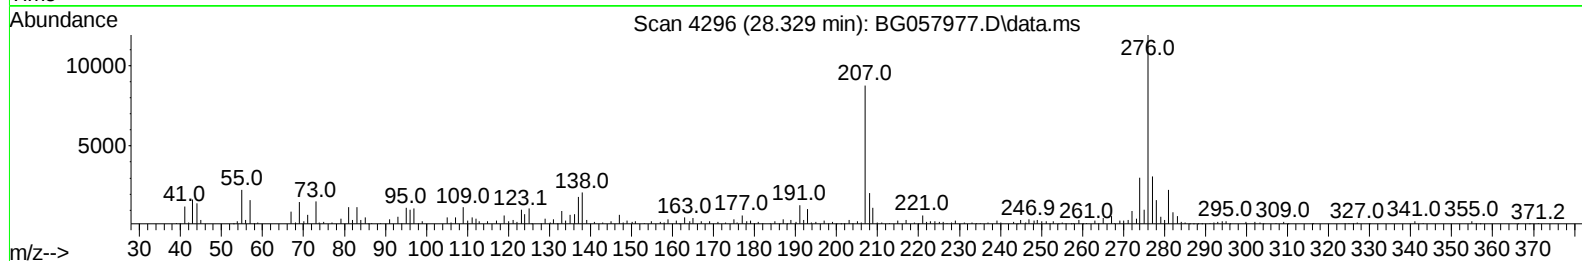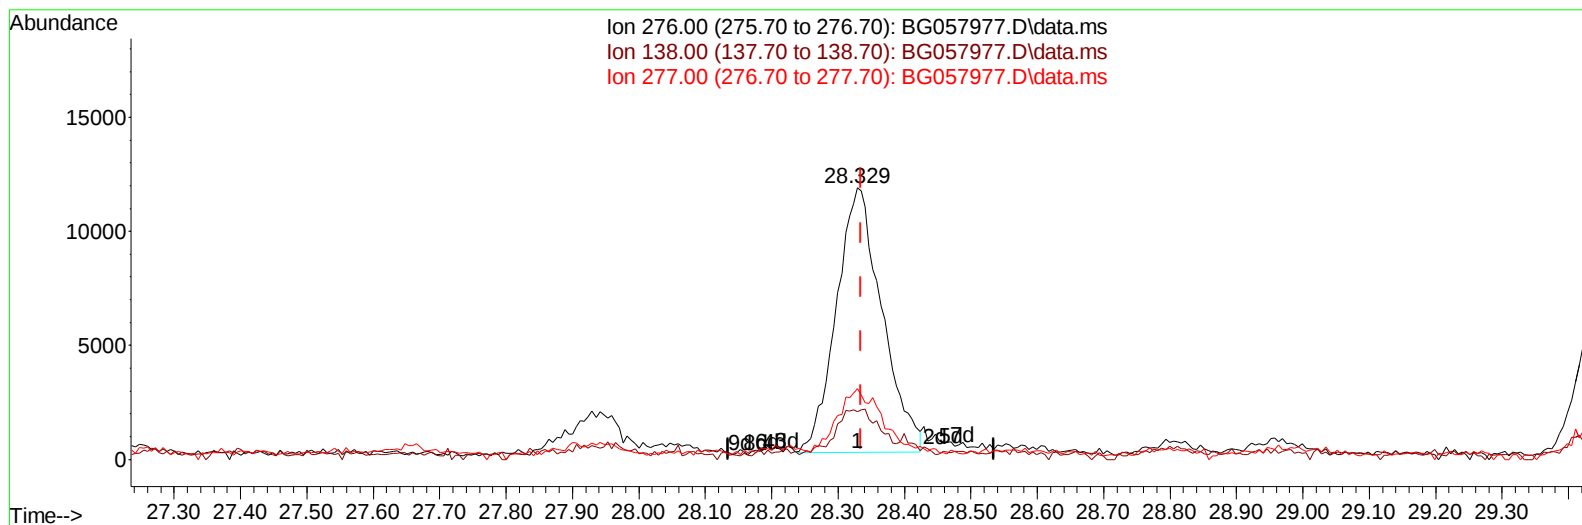

TIC: BG057977.D\data.ms

(94) Indeno(1,2,3-cd)pyrene

28.329min (-0.006) 2.91 ng/u1

response 55312

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	17.50	17.58
277.00	24.30	25.99
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070323\
Data File : BG057977.D
Acq On : 4 Jul 2023 7:02
Operator : CG/JU
Sample : 03247-17
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCGM3

Manual IntegrationsAPPROVED

Reviewed By :Sohil Jodhani 07/04/2023
Supervised By :mohammad ahmed 07/04/2023

Quant Time: Jul 04 07:45:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 04 05:09:13 2023
Response via : Initial Calibration

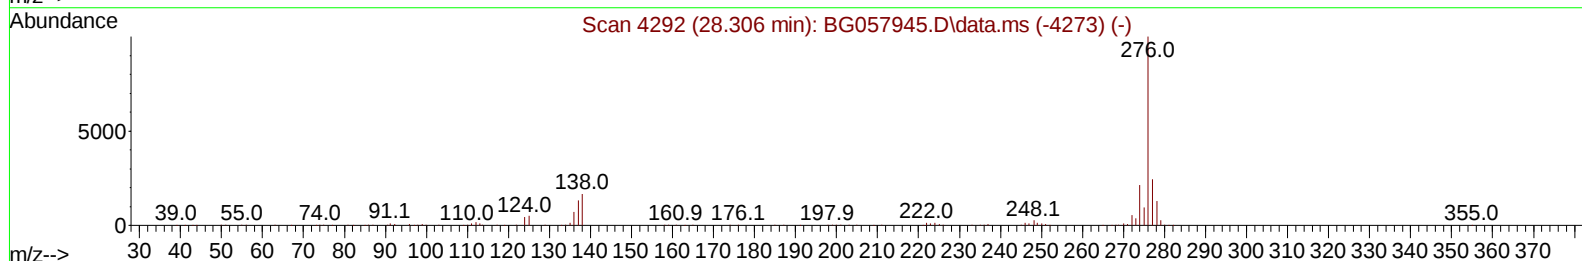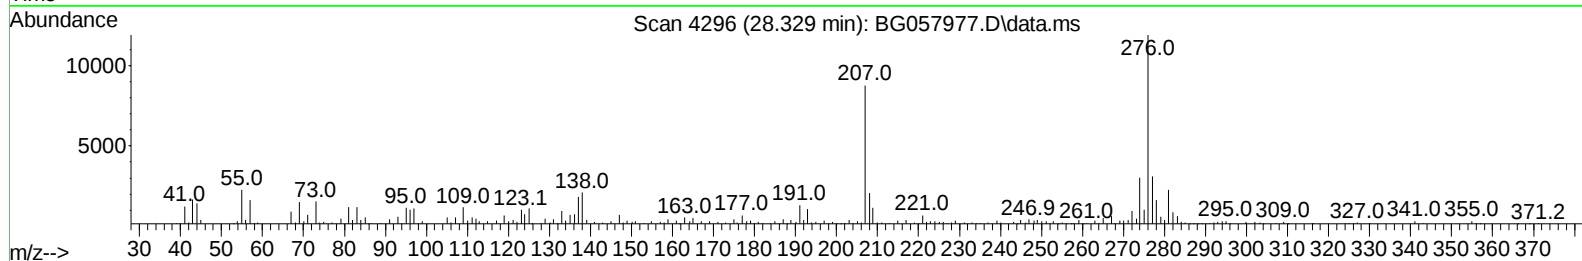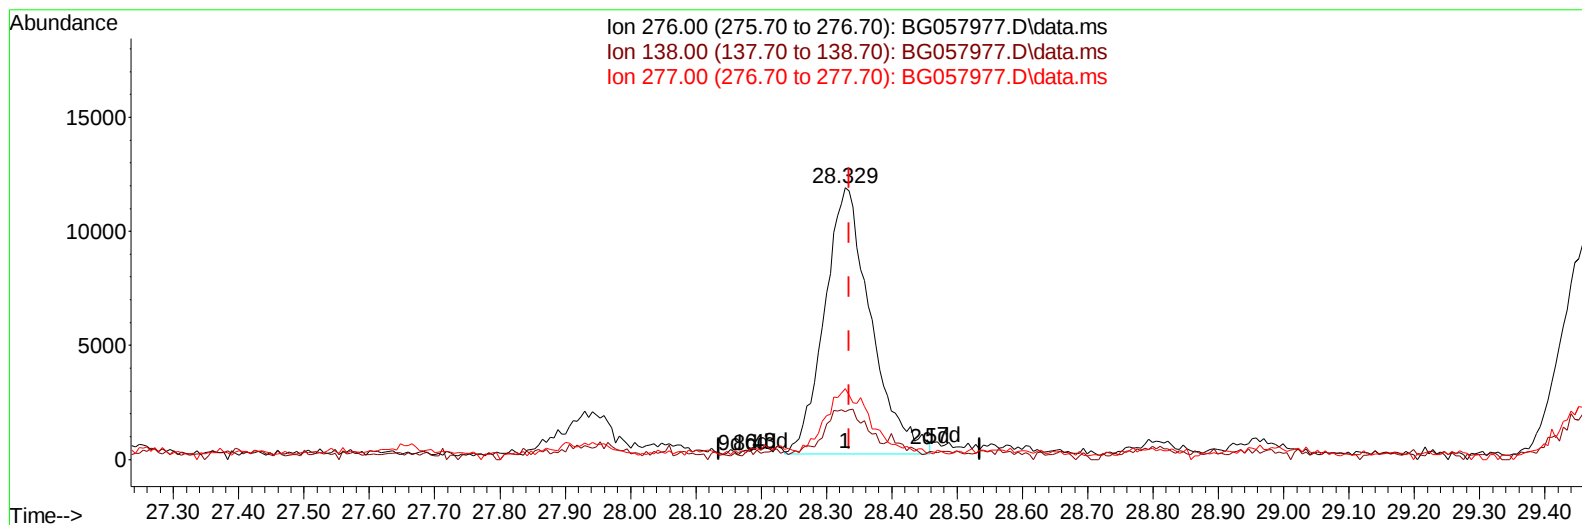

TIC: BG057977.D\data.ms

(94) Indeno(1,2,3-cd)pyrene

28.329min (-0.006) 3.04 ng/u1 m

response 57693

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	17.50	17.58
277.00	24.30	25.99
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070323\
 Data File : BG057977.D
 Acq On : 4 Jul 2023 7:02
 Operator : CG/JU
 Sample : 03247-17
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCGM3

Manual IntegrationsAPPROVED

Quant Time: Jul 04 07:47:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 04 05:09:13 2023
 Response via : Initial Calibration

Reviewed By :Sohil Jodhani 07/04/2023
 Supervised By :mohammad ahmed 07/04/2023

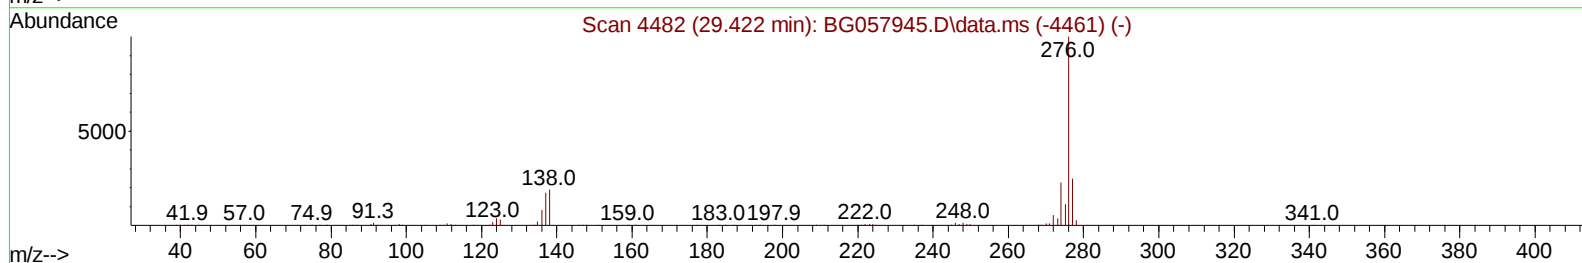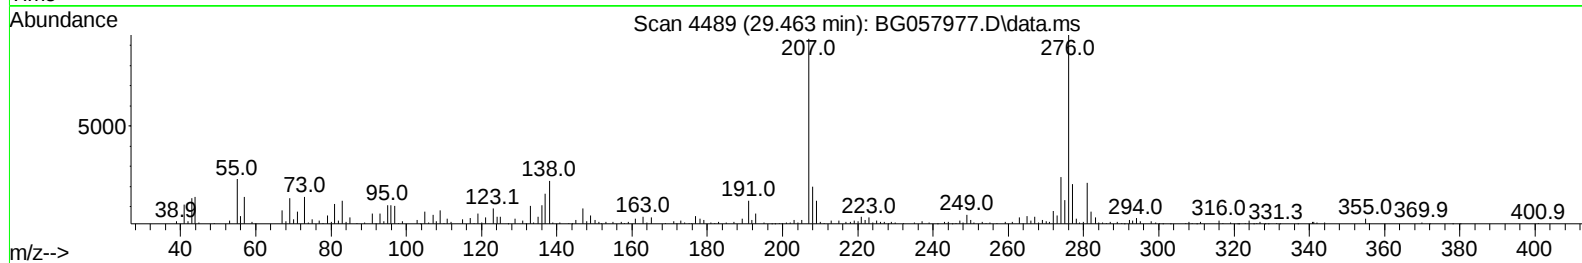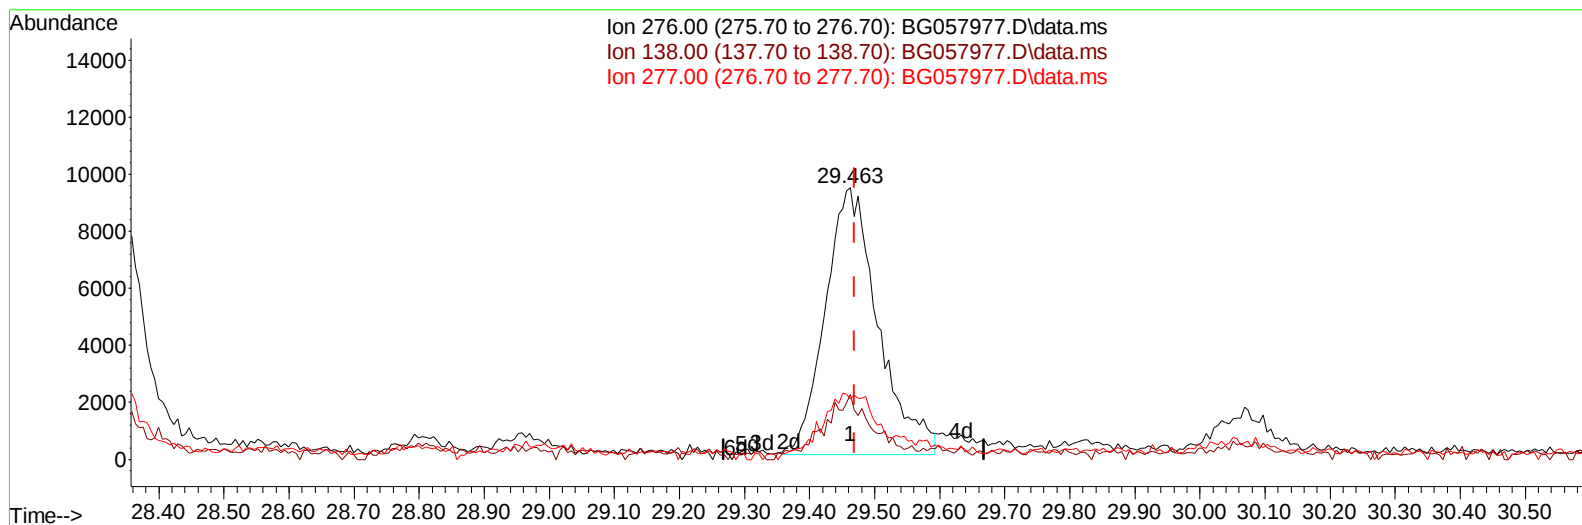

TIC: BG057977.D\data.ms

(96) Benzo(g,h,i)perylene

29.463min (-0.006) 3.42 ng/ul m

response 53126

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	17.70	24.05#
277.00	23.20	22.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070323\
 Data File : BG057977.D
 Acq On : 4 Jul 2023 7:02
 Operator : CG/JU
 Sample : 03247-17
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCGM3

Manual IntegrationsAPPROVED

Reviewed By :Sohil Jodhani 07/04/2023
 Supervised By :mohammad ahmed 07/04/2023

Quant Time: Jul 04 07:47:22 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 04 05:09:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.941	152	39382	20.000	ng/ul	0.00
20) Naphthalene-d8	10.744	136	183587	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.569	164	120685	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.313	188	266183	20.000	ng/ul	0.00
79) Chrysene-d12	21.566	240	217670	20.000	ng/ul	0.00
88) Perylene-d12	24.733	264	261185	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.376	96	4784	4.254	ng/uL	0.00
4) Pyridine-d5	3.793	84	3864	1.132	ng/ul	0.00
7) Phenol-d5	7.101	99	99810	24.817	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.265	67	65923	27.199	ng/ul	0.00
11) 2-Chlorophenol-d4	7.471	132	78786	28.403	ng/ul	0.00
15) 4-Methylphenol-d8	8.646	113	44921	14.802	ng/ul	0.00
21) Nitrobenzene-d5	9.099	128	40798	27.266	ng/ul	0.00
24) 2-Nitrophenol-d4	9.821	143	42732	27.173	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.362	165	79740	26.432	ng/ul	0.00
31) 4-Chloroaniline-d4	10.873	131	47908	10.474	ng/ul	0.00
46) Dimethylphthalate-d6	13.975	166	256115	26.897	ng/ul	0.00
49) Acenaphthylene-d8	14.263	160	306118	29.460	ng/ul	0.00
54) 4-Nitrophenol-d4	14.768	143	32229	19.157	ng/ul	0.00
60) Fluorene-d10	15.562	176	227935	28.186	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.679	200	30146	20.857	ng/ul	0.00
73) Anthracene-d10	17.412	188	333139	26.971	ng/ul	0.00
81) Pyrene-d10	19.698	212	399518	29.143	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.516	264	399147	29.996	ng/ul	0.00
Target Compounds						
					Qvalue	
72) Phenanthrene	17.354	178	25162	1.858	ng/ul	99
80) Fluoranthene	19.369	202	131983	8.309	ng/ul	99
82) Pyrene	19.727	202	108312	6.774	ng/ul	98
85) Benzo(a)anthracene	21.549	228	75370	4.822	ng/ul	96
87) Chrysene	21.613	228	81736	5.579	ng/ul	97
90) Benzo(b)fluoranthene	23.729	252	119309	7.378	ng/ul	97
91) Benzo(k)fluoranthene	23.781	252	38838m	2.450	ng/ul	
93) Benzo(a)pyrene	24.580	252	69556	4.859	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	28.329	276	57693m	3.035	ng/ul	
96) Benzo(g,h,i)perylene	29.463	276	53126m	3.422	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070323\
Data File : BG057977.D
Acq On : 4 Jul 2023 7:02
Operator : CG/JU
Sample : 03247-17
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCGM3

Manual IntegrationsAPPROVED

Reviewed By :Sohil Jodhani 07/04/2023
Supervised By :mohammad ahmed 07/04/2023

Quant Time: Jul 04 07:47:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 04 05:09:13 2023
Response via : Initial Calibration

