

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070323\
 Data File : BG058003.D
 Acq On : 5 Jul 2023 2:41
 Operator : CG/JU
 Sample : PB153768BL
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK768

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG058003.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.117	3	5	15	rVB	58107	67803	3.92%	0.372%
2	3.211	18	21	30	rVB	6422	10910	0.63%	0.060%
3	3.376	45	49	54	rBV	18198	25264	1.46%	0.138%
4	3.787	114	119	132	rBV	259801	424476	24.54%	2.326%
5	4.128	173	177	181	rVB2	7981	11154	0.64%	0.061%
6	7.106	676	684	700	rBV	294723	504801	29.19%	2.766%
7	7.265	704	711	722	rBV	228931	375671	21.72%	2.058%
8	7.471	740	746	756	rBV	284822	489020	28.27%	2.679%
9	7.941	819	826	833	rVB	206378	337846	19.53%	1.851%
10	8.646	937	946	956	rBV	361462	631517	36.51%	3.460%
11	9.104	1016	1024	1035	rBV	277608	491809	28.43%	2.695%
12	9.821	1139	1146	1155	rBV	218505	395254	22.85%	2.166%
13	10.367	1231	1239	1251	rBV	348585	632106	36.55%	3.463%
14	10.743	1295	1303	1312	rBV	302445	532818	30.81%	2.919%
15	10.879	1318	1326	1340	rBV	354419	650076	37.58%	3.562%
16	12.330	1568	1573	1579	rVB2	6007	9448	0.55%	0.052%
17	13.458	1761	1765	1770	rBV3	3798	5759	0.33%	0.032%
18	13.975	1847	1853	1863	rBV	603306	888669	51.38%	4.869%
19	14.269	1896	1903	1920	rBV	704097	1120042	64.76%	6.137%
20	14.574	1948	1955	1970	rVB	452874	719300	41.59%	3.941%
21	14.774	1980	1989	2009	rBV	234456	412837	23.87%	2.262%
22	15.567	2117	2124	2138	rBV	885629	1374590	79.47%	7.532%
23	15.679	2138	2143	2156	rVV	226979	346070	20.01%	1.896%
24	15.802	2161	2164	2171	rVB2	4133	5562	0.32%	0.030%
25	17.318	2415	2422	2431	rVB	543451	840315	48.58%	4.604%
26	17.418	2431	2439	2450	rBV	962636	1436609	83.06%	7.872%
27	17.694	2479	2486	2489	rBV2	1224	2394	0.14%	0.013%
28	18.423	2608	2610	2613	rBV2	1720	1784	0.10%	0.010%
29	19.269	2749	2754	2760	rBV3	12922	18260	1.06%	0.100%
30	19.339	2762	2766	2770	rBV	11752	15393	0.89%	0.084%
31	19.703	2822	2828	2837	rBV	1166745	1664711	96.25%	9.121%
32	19.944	2866	2869	2870	rBV2	2490	2731	0.16%	0.015%
33	21.572	3139	3146	3153	rBV	531651	860772	49.77%	4.716%
34	23.822	3524	3529	3539	rVB3	31468	66226	3.83%	0.363%
35	24.521	3638	3648	3662	rBV2	607535	1729644	100.00%	9.477%
36	24.739	3676	3685	3700	rVB	357829	1025402	59.28%	5.618%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070323\
Data File : BG058003.D
Acq On : 5 Jul 2023 2:41
Operator : CG/JU
Sample : PB153768BL
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK768

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Title : SVOA CALIBRATION

37	25.855	3871	3875	3885	rVB4	38538	91130	5.27%	0.499%
38	28.781	4367	4373	4374	rBV5	18470	32545	1.88%	0.178%




Sum of corrected areas: 18250718

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070323\
Data File : BG058003.D
Acq On : 5 Jul 2023 2:41
Operator : CG/JU
Sample : PB153768BL
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK768

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

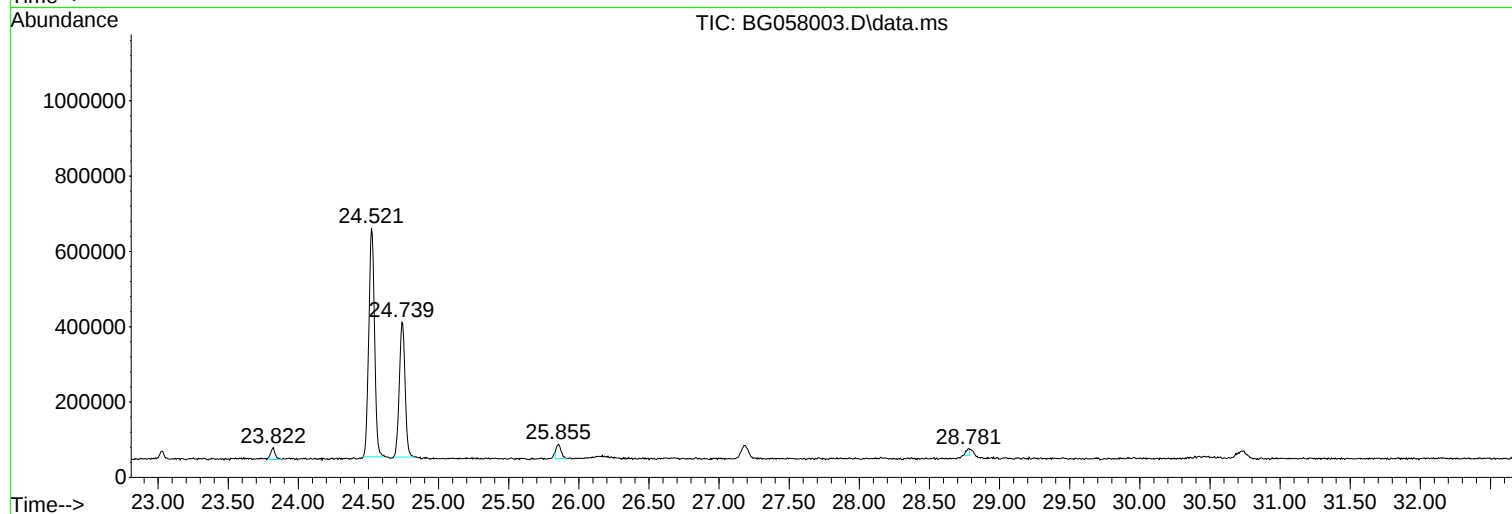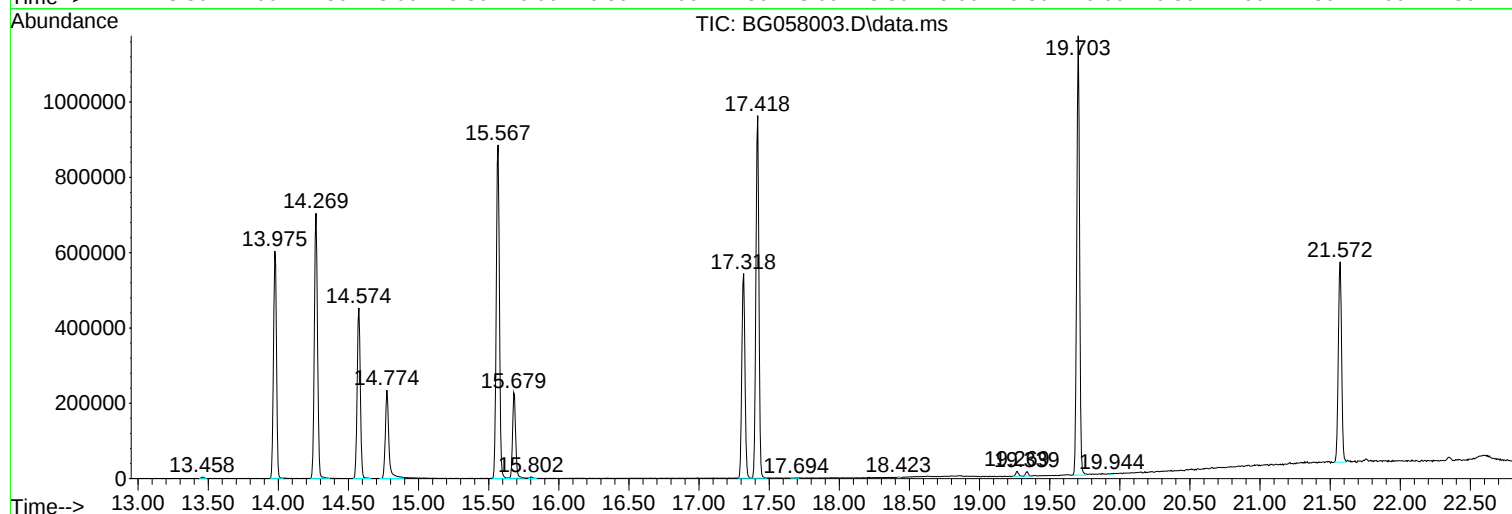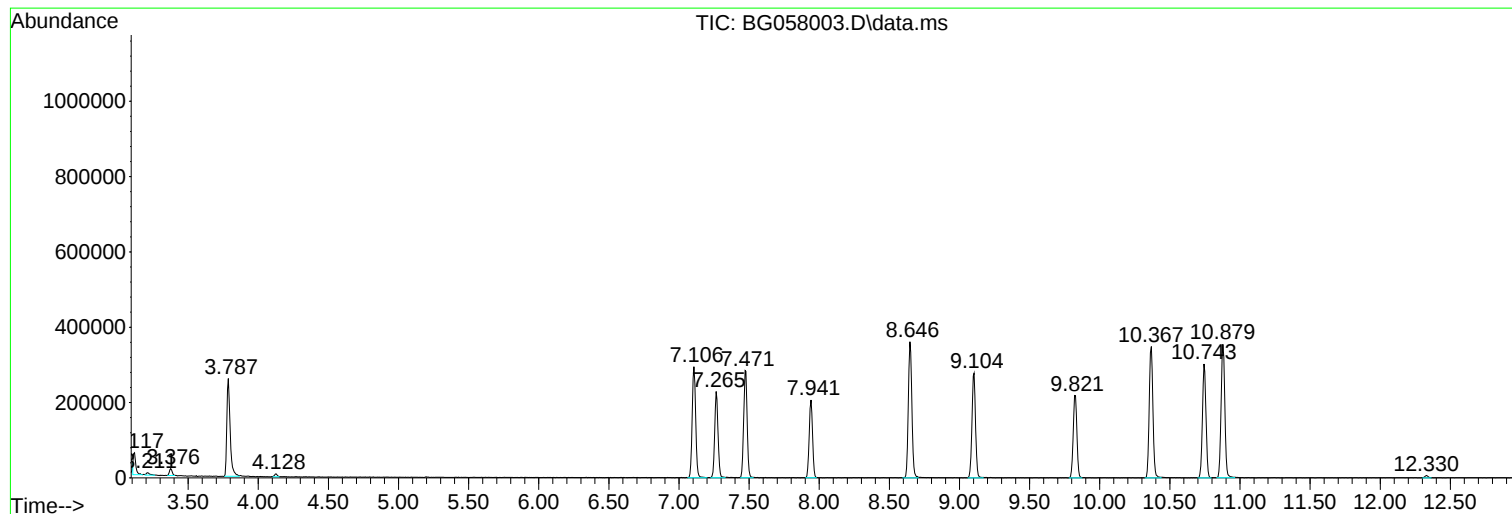

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070323\
Data File : BG058003.D
Acq On : 5 Jul 2023 2:41
Operator : CG/JU
Sample : PB153768BL
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK768










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.117	4.01 ng/ul	67803	1,4-Dichlorobenzene-d4	7.941

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	45
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	32
3			2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	23
4			Methane, isothiocyanato-	73	C2H3NS	000556-61-6	9
5			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9

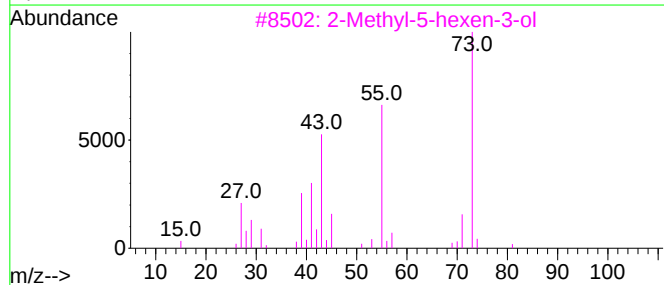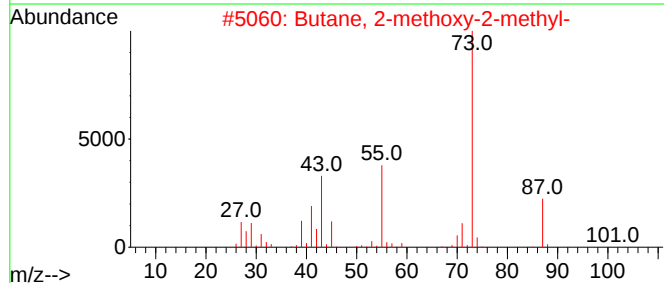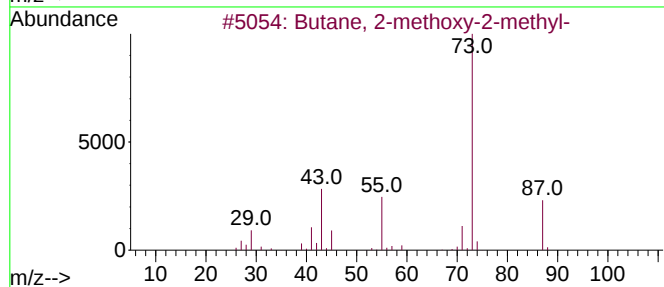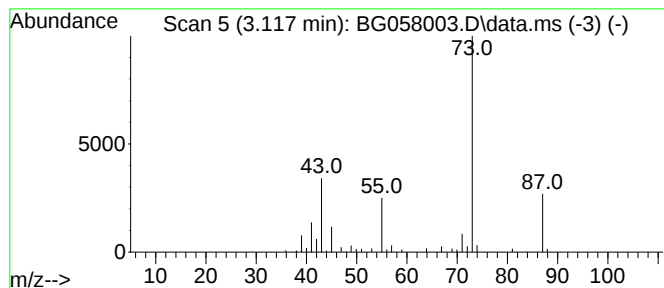

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070323\
Data File : BG058003.D
Acq On : 5 Jul 2023 2:41
Operator : CG/JU
Sample : PB153768BL
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK768

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	3.117	4.0	ng/ul	67803	1	7.941	337846	20.0