

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070324\
 Data File : BG061859.D
 Acq On : 3 Jul 2024 10:30
 Operator : MA/JU
 Sample : PB161628BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK628

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG061859.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.440	24	26	27	rBV	5205	2673	0.17%	0.017%
2	3.457	27	29	30	rVB2	6098	3777	0.24%	0.024%
3	3.481	30	33	42	rBV3	13003	26052	1.68%	0.165%
4	3.904	101	105	113	rBV	180517	301138	19.42%	1.905%
5	4.192	152	154	157	rVB3	3025	2511	0.16%	0.016%
6	4.245	160	163	166	rBV4	6174	7958	0.51%	0.050%
7	4.991	285	290	291	rVV4	3754	3692	0.24%	0.023%
8	5.014	291	294	297	rVB2	2439	3366	0.22%	0.021%
9	5.114	309	311	314	rVB2	3435	2920	0.19%	0.018%
10	5.138	314	315	319	rBV4	3273	4431	0.29%	0.028%
11	5.273	334	338	339	rBV3	2151	2933	0.19%	0.019%
12	5.361	349	353	355	rVB2	2735	2949	0.19%	0.019%
13	5.385	355	357	359	rBV2	2887	2450	0.16%	0.016%
14	5.426	359	364	366	rVB5	1650	2900	0.19%	0.018%
15	5.649	400	402	404	rBV2	2942	3534	0.23%	0.022%
16	5.672	404	406	408	rVB	2797	2467	0.16%	0.016%
17	5.790	425	426	433	rVB2	3124	2631	0.17%	0.017%
18	5.855	433	437	439	rVB2	1858	2522	0.16%	0.016%
19	5.896	439	444	445	rBV2	2412	3194	0.21%	0.020%
20	5.966	453	456	458	rBV3	2395	2703	0.17%	0.017%
21	6.295	509	512	515	rBV3	2013	2812	0.18%	0.018%
22	7.247	667	674	683	rBV2	217620	392120	25.29%	2.481%
23	7.417	694	703	711	rBV	157660	276539	17.84%	1.750%
24	7.623	731	738	745	rBV	196008	349136	22.52%	2.209%
25	8.093	811	818	828	rVB2	141110	253862	16.37%	1.606%
26	8.798	928	938	946	rBV	275444	490851	31.66%	3.106%
27	9.127	990	994	996	rVV2	2544	2448	0.16%	0.015%
28	9.168	1000	1001	1005	rVB2	2648	2521	0.16%	0.016%
29	9.262	1010	1017	1026	rVB	220506	400237	25.82%	2.532%
30	9.985	1133	1140	1148	rVV2	201749	359736	23.20%	2.276%
31	10.061	1152	1153	1159	rVB2	3719	5176	0.33%	0.033%
32	10.526	1224	1232	1240	rBV	278054	492932	31.80%	3.119%
33	10.743	1266	1269	1272	rBV2	2115	3073	0.20%	0.019%
34	10.831	1279	1284	1285	rBV3	2115	2550	0.16%	0.016%
35	10.907	1290	1297	1305	rVV	225550	405904	26.18%	2.568%
36	10.996	1308	1312	1313	rBV	2884	3637	0.23%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070324\
 Data File : BG061859.D
 Acq On : 3 Jul 2024 10:30
 Operator : MA/JU
 Sample : PB161628BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK628

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

37	11.043	1313	1320	1330	rVB2	291413	545846	35.21%	3.454%
38	11.201	1345	1347	1350	rVB	3117	2722	0.18%	0.017%
39	11.242	1350	1354	1357	rBV	1759	2746	0.18%	0.017%
40	11.542	1404	1405	1410	rVB	3309	3631	0.23%	0.023%
41	11.677	1422	1428	1430	rBV	3723	7403	0.48%	0.047%
42	11.748	1438	1440	1443	rBV4	2830	4025	0.26%	0.025%
43	11.806	1447	1450	1451	rBV4	2059	2516	0.16%	0.016%
44	11.942	1472	1473	1478	rVB	2979	3455	0.22%	0.022%
45	12.094	1497	1499	1503	rBV	2410	2577	0.17%	0.016%
46	12.406	1548	1552	1554	rBV2	3054	3855	0.25%	0.024%
47	12.482	1562	1565	1566	rBV	4347	2776	0.18%	0.018%
48	12.576	1578	1581	1585	rBV	2534	2914	0.19%	0.018%
49	13.093	1665	1669	1672	rBV	1766	3200	0.21%	0.020%
50	13.293	1702	1703	1707	rVB	3354	3254	0.21%	0.021%
51	13.522	1738	1742	1743	rVB	2818	2602	0.17%	0.016%
52	13.687	1767	1770	1771	rBV	3308	3558	0.23%	0.023%
53	13.704	1771	1773	1776	rVV	2571	2797	0.18%	0.018%
54	13.751	1778	1781	1783	rVB	2746	2985	0.19%	0.019%
55	13.957	1813	1816	1819	rBV	1573	2718	0.18%	0.017%
56	14.121	1838	1844	1850	rBV	619381	853567	55.06%	5.400%
57	14.262	1865	1868	1871	rBV2	3458	4962	0.32%	0.031%
58	14.292	1871	1873	1876	rVB2	3025	3023	0.19%	0.019%
59	14.415	1887	1894	1901	rVB	570667	908426	58.60%	5.748%
60	14.721	1938	1946	1952	rBV	384295	600579	38.74%	3.800%
61	14.909	1972	1978	1985	rBV	283041	449092	28.97%	2.841%
62	15.020	1996	1997	2000	rBV	3291	3051	0.20%	0.019%
63	15.050	2000	2002	2005	rVV2	4293	3971	0.26%	0.025%
64	15.091	2007	2009	2010	rVV2	2853	2535	0.16%	0.016%
65	15.120	2012	2014	2016	rVB	3578	3202	0.21%	0.020%
66	15.185	2024	2025	2028	rBV	2685	3198	0.21%	0.020%
67	15.291	2041	2043	2047	rVB	2390	2644	0.17%	0.017%
68	15.420	2062	2065	2068	rVB2	3115	4424	0.29%	0.028%
69	15.443	2068	2069	2071	rBV	4406	2613	0.17%	0.017%
70	15.567	2087	2090	2094	rBV	2295	2589	0.17%	0.016%
71	15.708	2106	2114	2120	rBV	782693	1161732	74.93%	7.350%
72	15.819	2126	2133	2141	rBV	268848	414634	26.74%	2.623%
73	15.943	2150	2154	2156	rBV3	4260	4610	0.30%	0.029%
74	16.348	2221	2223	2225	rBV	3191	3426	0.22%	0.022%
75	16.378	2225	2228	2230	rVB	3991	4016	0.26%	0.025%
76	16.401	2230	2232	2234	rBV	2323	2472	0.16%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070324\
 Data File : BG061859.D
 Acq On : 3 Jul 2024 10:30
 Operator : MA/JU
 Sample : PB161628BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK628

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

77	16.571	2258	2261	2264	rVB	3281	3060	0.20%	0.019%
78	16.806	2299	2301	2303	rVB2	4291	2751	0.18%	0.017%
79	17.218	2369	2371	2373	rVV	3267	2780	0.18%	0.018%
80	17.247	2373	2376	2378	rVB2	4083	3794	0.24%	0.024%
81	17.288	2380	2383	2386	rBV	2850	5111	0.33%	0.032%
82	17.400	2399	2402	2405	rBV3	2724	3178	0.20%	0.020%
83	17.459	2406	2412	2421	rVV	506077	756344	48.79%	4.785%
84	17.558	2423	2429	2438	rVV	873432	1304860	84.17%	8.256%
85	17.641	2441	2443	2445	rBV3	3712	2609	0.17%	0.017%
86	17.870	2480	2482	2484	rVB	3608	2450	0.16%	0.016%
87	18.046	2510	2512	2514	rBV	3890	2685	0.17%	0.017%
88	18.081	2517	2518	2519	rBV	6222	2691	0.17%	0.017%
89	18.175	2532	2534	2538	rVB2	3835	4481	0.29%	0.028%
90	18.269	2546	2550	2551	rVB3	3149	2878	0.19%	0.018%
91	18.634	2608	2612	2614	rBV4	4000	4057	0.26%	0.026%
92	18.910	2657	2659	2660	rBV2	3486	3352	0.22%	0.021%
93	19.004	2674	2675	2677	rBV2	3886	2668	0.17%	0.017%
94	19.168	2701	2703	2708	rBV5	4130	5285	0.34%	0.033%
95	19.409	2740	2744	2746	rBV3	15342	19683	1.27%	0.125%
96	19.474	2751	2755	2758	rVV3	15330	16349	1.05%	0.103%
97	19.838	2811	2817	2826	rVB	1038818	1498056	96.63%	9.478%
98	21.718	3132	3137	3144	rVB2	474861	780758	50.36%	4.940%
99	24.738	3643	3651	3663	rVB2	558155	1550341	100.00%	9.809%
100	24.962	3682	3689	3705	rVB	304343	950532	61.31%	6.014%


Sum of corrected areas: 15805434

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070324\
Data File : BG061859.D
Acq On : 3 Jul 2024 10:30
Operator : MA/JU
Sample : PB161628BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK628

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

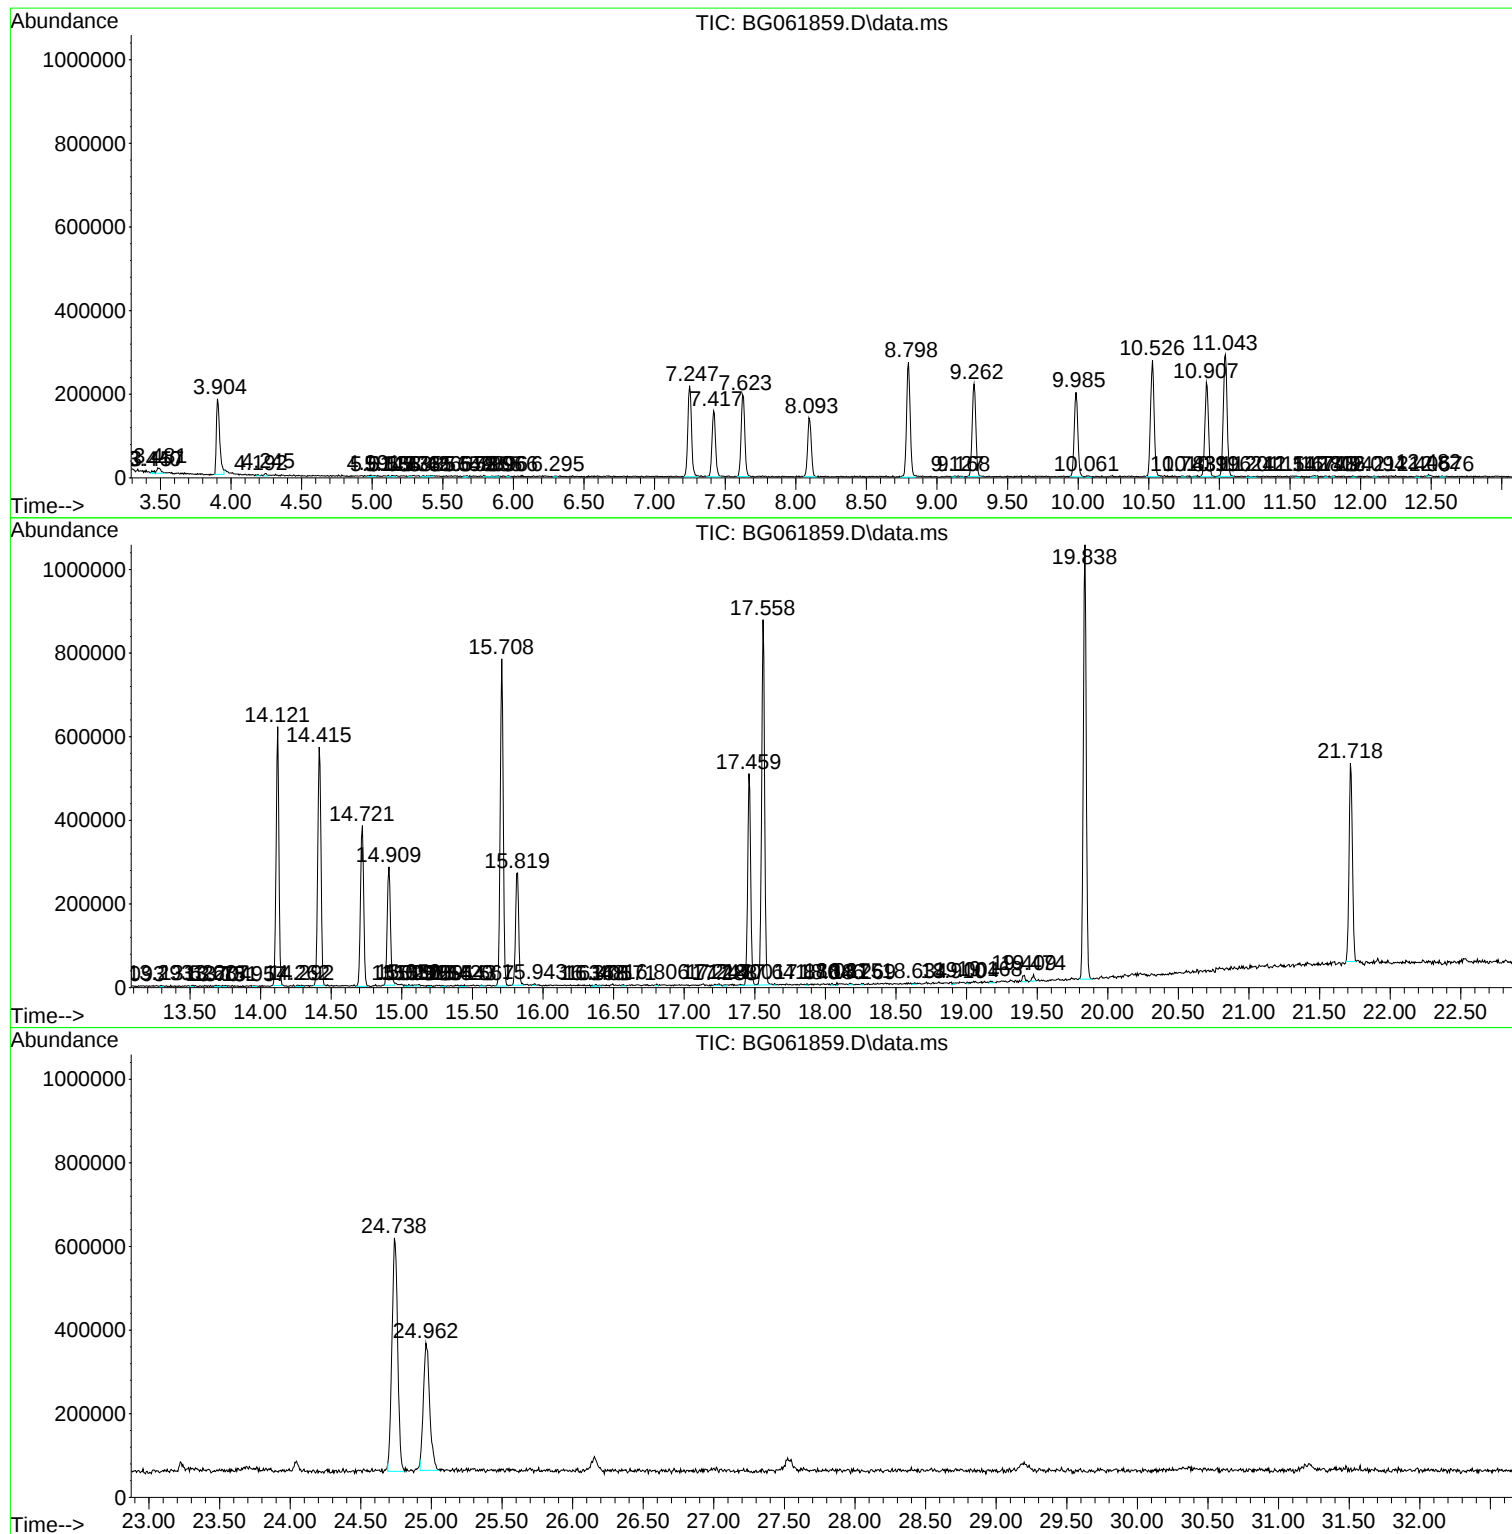

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070324\
Data File : BG061859.D
Acq On : 3 Jul 2024 10:30
Operator : MA/JU
Sample : PB161628BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK628

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070324\
Data File : BG061859.D
Acq On : 3 Jul 2024 10:30
Operator : MA/JU
Sample : PB161628BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK628

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc