

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070324\
 Data File : BG061882.D
 Acq On : 4 Jul 2024 3:45
 Operator : MA/JU
 Sample : PB161651BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK651

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG061882.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.484	29	33	37	rVB2	18286	21995	1.17%	0.108%
2	3.901	101	104	118	rBV	226709	364489	19.33%	1.783%
3	4.247	158	163	168	rBV3	4993	9785	0.52%	0.048%
4	4.435	192	195	196	rBV3	2154	2466	0.13%	0.012%
5	4.500	202	206	209	rBV3	2766	2692	0.14%	0.013%
6	5.440	364	366	370	rBV	2042	2502	0.13%	0.012%
7	5.534	380	382	385	rVB	2485	2514	0.13%	0.012%
8	5.669	404	405	411	rVB2	2169	2825	0.15%	0.014%
9	5.722	411	414	416	rVV	2725	3144	0.17%	0.015%
10	5.757	416	420	422	rVB	3586	3243	0.17%	0.016%
11	6.116	478	481	482	rBV	2072	2560	0.14%	0.013%
12	6.304	508	513	515	rVB	2592	3028	0.16%	0.015%
13	6.333	515	518	521	rBV	2042	2578	0.14%	0.013%
14	6.562	556	557	562	rVB2	3415	3144	0.17%	0.015%
15	7.132	652	654	657	rBV	2763	2843	0.15%	0.014%
16	7.244	665	673	681	rBV2	289071	491847	26.08%	2.406%
17	7.414	696	702	711	rVB	184883	309664	16.42%	1.515%
18	7.626	730	738	744	rBV	249674	436215	23.13%	2.134%
19	8.096	810	818	824	rBV	212385	358394	19.01%	1.753%
20	8.413	870	872	876	rVB	3069	3931	0.21%	0.019%
21	8.454	876	879	881	rBV	2308	2644	0.14%	0.013%
22	8.495	881	886	888	rBV	2101	2771	0.15%	0.014%
23	8.795	929	937	944	rBV2	345733	591900	31.39%	2.895%
24	9.259	1007	1016	1025	rBV	284813	502554	26.65%	2.458%
25	9.982	1132	1139	1146	rBV2	253550	458655	24.32%	2.243%
26	10.052	1149	1151	1154	rVB	3003	2863	0.15%	0.014%
27	10.129	1163	1164	1169	rBV	2325	2456	0.13%	0.012%
28	10.522	1223	1231	1239	rVB	357130	630039	33.41%	3.082%
29	10.710	1259	1263	1264	rBV	2120	2505	0.13%	0.012%
30	10.910	1288	1297	1304	rBV	326632	595314	31.57%	2.912%
31	10.957	1304	1305	1308	rVB	2549	2537	0.13%	0.012%
32	11.039	1312	1319	1329	rBV	359501	674937	35.79%	3.301%
33	11.351	1366	1372	1375	rBV	1590	3342	0.18%	0.016%
34	11.451	1384	1389	1392	rBV	2421	3481	0.18%	0.017%
35	12.256	1523	1526	1529	rBV	2396	3454	0.18%	0.017%
36	12.485	1560	1565	1571	rVB3	7202	9911	0.53%	0.048%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070324\
 Data File : BG061882.D
 Acq On : 4 Jul 2024 3:45
 Operator : MA/JU
 Sample : PB161651BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK651

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

37	12.796	1616	1618	1622	rBV2	2061	2743	0.15%	0.013%
38	12.949	1642	1644	1647	rBV	2795	2801	0.15%	0.014%
39	13.031	1654	1658	1661	rVB	2477	4168	0.22%	0.020%
40	13.255	1694	1696	1700	rBV	2160	2448	0.13%	0.012%
41	13.648	1760	1763	1765	rBV	2365	2970	0.16%	0.015%
42	13.695	1769	1771	1775	rVB	3248	3754	0.20%	0.018%
43	13.913	1804	1808	1813	rVB	2127	3201	0.17%	0.016%
44	14.036	1827	1829	1831	rVB	3391	3039	0.16%	0.015%
45	14.118	1836	1843	1851	rBV	709716	1021035	54.15%	4.994%
46	14.324	1875	1878	1881	rVB	1727	2448	0.13%	0.012%
47	14.412	1886	1893	1901	rVB	721839	1131908	60.03%	5.537%
48	14.718	1938	1945	1953	rVB	568989	892513	47.33%	4.366%
49	14.906	1969	1977	1986	rBV	389961	613689	32.55%	3.002%
50	15.123	2011	2014	2016	rBV	2649	3096	0.16%	0.015%
51	15.705	2107	2113	2120	rVB	976694	1431355	75.91%	7.001%
52	15.816	2126	2132	2139	rBV	398890	564214	29.92%	2.760%
53	15.940	2147	2153	2155	rBV4	5616	11061	0.59%	0.054%
54	16.057	2169	2173	2175	rBV	2103	2724	0.14%	0.013%
55	16.128	2182	2185	2188	rBV2	3265	4747	0.25%	0.023%
56	16.269	2205	2209	2212	rBV2	3639	4921	0.26%	0.024%
57	16.521	2251	2252	2255	rBV2	2715	2522	0.13%	0.012%
58	16.615	2265	2268	2269	rBV	3367	2776	0.15%	0.014%
59	17.138	2353	2357	2360	rVB	4048	5716	0.30%	0.028%
60	17.185	2360	2365	2368	rBV2	2323	3636	0.19%	0.018%
61	17.455	2403	2411	2418	rBV	758280	1163665	61.71%	5.692%
62	17.555	2421	2428	2436	rVB	1078164	1640669	87.01%	8.025%
63	17.832	2471	2475	2479	rVB3	3153	4673	0.25%	0.023%
64	17.890	2483	2485	2487	rBV3	2515	2717	0.14%	0.013%
65	18.278	2548	2551	2552	rBV	3586	3076	0.16%	0.015%
66	18.372	2564	2567	2568	rBV	4497	3413	0.18%	0.017%
67	18.707	2620	2624	2625	rBV3	3591	4177	0.22%	0.020%
68	18.748	2630	2631	2634	rVB2	3170	2719	0.14%	0.013%
69	18.883	2652	2654	2656	rBV	3141	2772	0.15%	0.014%
70	19.136	2694	2697	2699	rVB2	3562	4016	0.21%	0.020%
71	19.159	2699	2701	2702	rBV2	3837	2609	0.14%	0.013%
72	19.342	2730	2732	2735	rBV3	3277	3718	0.20%	0.018%
73	19.400	2737	2742	2746	rVV4	14050	23970	1.27%	0.117%
74	19.477	2750	2755	2757	rBV2	13225	19235	1.02%	0.094%
75	19.624	2777	2780	2781	rBV3	4206	4565	0.24%	0.022%
76	19.747	2797	2801	2805	rBV3	9316	11262	0.60%	0.055%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070324\
Data File : BG061882.D
Acq On : 4 Jul 2024 3:45
Operator : MA/JU
Sample : PB161651BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK651

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Title : SVOA CALIBRATION

77	19.835	2809	2816	2824	rBV	1275161	1809875	95.98%	8.853%
78	19.947	2833	2835	2837	rBV3	7327	5397	0.29%	0.026%
79	20.011	2844	2846	2847	rBV2	4053	2665	0.14%	0.013%
80	20.282	2890	2892	2895	rBV3	5606	5215	0.28%	0.026%
81	21.715	3130	3136	3143	rBV	709461	1176856	62.41%	5.756%
82	24.024	3527	3529	3539	rVB5	34271	68565	3.64%	0.335%
83	24.741	3641	3651	3663	rVB3	678068	1885625	100.00%	9.223%
84	24.958	3679	3688	3700	rVB2	455870	1350006	71.59%	6.603%




Sum of corrected areas: 20444167

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070324\
Data File : BG061882.D
Acq On : 4 Jul 2024 3:45
Operator : MA/JU
Sample : PB161651BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK651

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

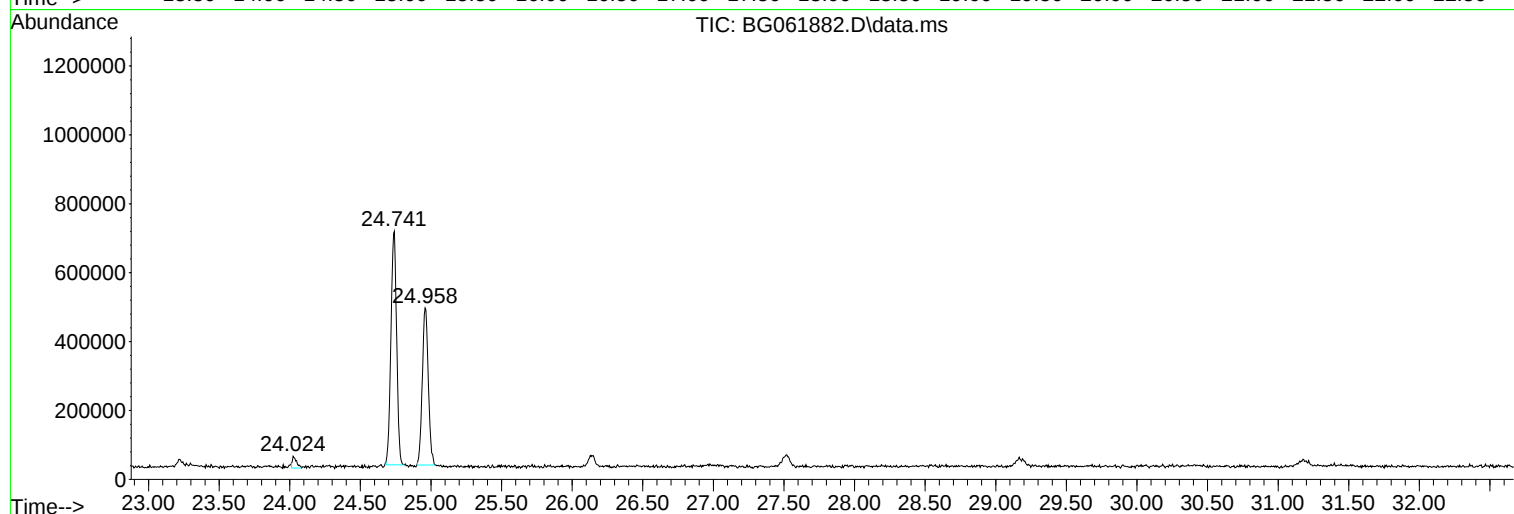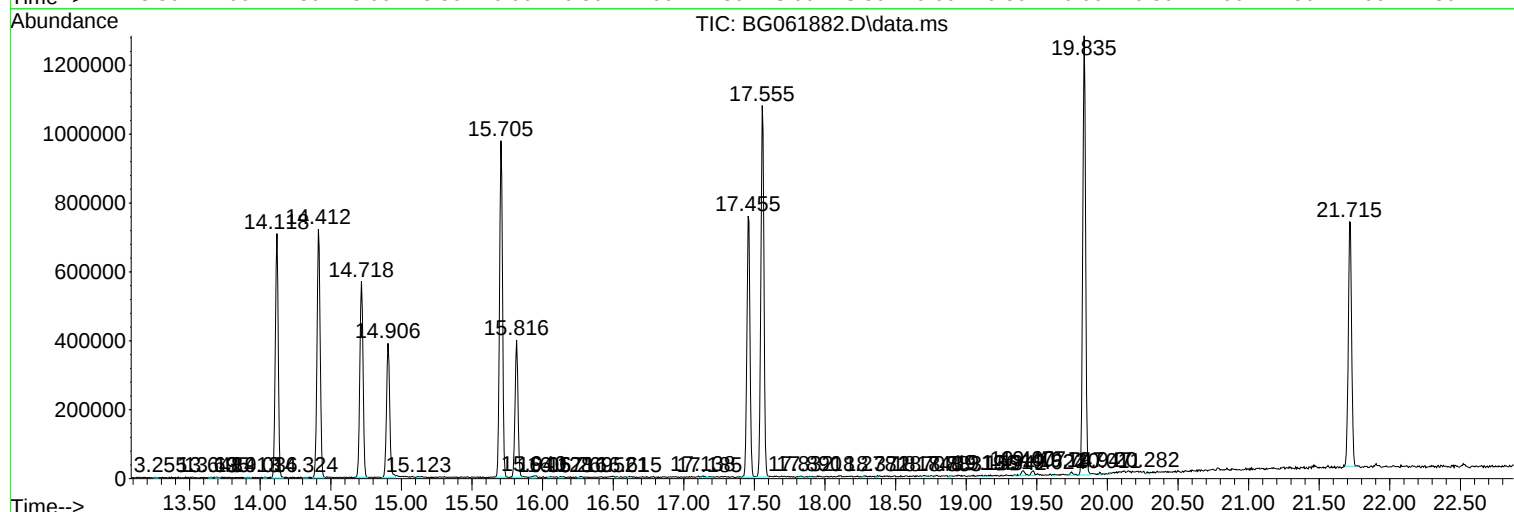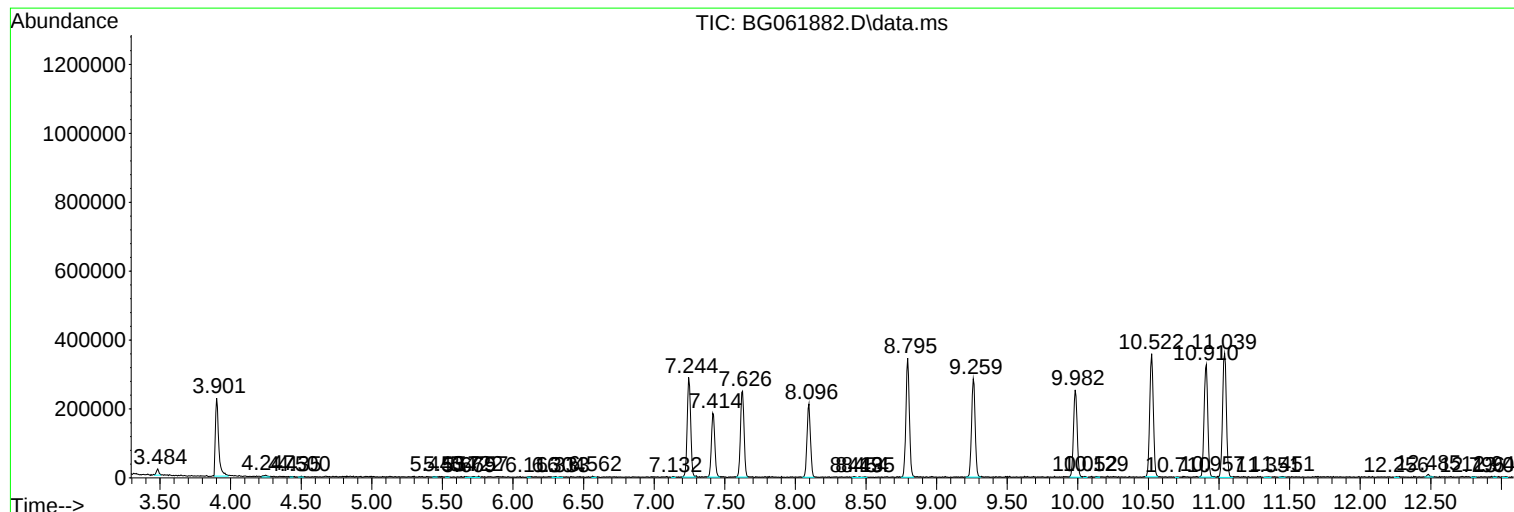

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070324\
Data File : BG061882.D
Acq On : 4 Jul 2024 3:45
Operator : MA/JU
Sample : PB161651BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK651

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070324\
Data File : BG061882.D
Acq On : 4 Jul 2024 3:45
Operator : MA/JU
Sample : PB161651BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK651

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc