

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
 Data File : BG058061.D
 Acq On : 7 Jul 2023 00:51
 Operator : CG/JU
 Sample : 03283-15
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EXYZ1

Quant Time: Jul 07 01:50:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 05 23:20:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.917	152	31964	20.000	ng/u1	0.00
20) Naphthalene-d8	10.720	136	147088	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.551	164	108463	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.300	188	292440	20.000	ng/u1	0.00
79) Chrysene-d12	21.554	240	272735	20.000	ng/u1	0.00
88) Perylene-d12	24.703	264	334550	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	4196	4.597	ng/uL	-0.01
4) Pyridine-d5	3.769	84	25389	9.162	ng/u1	0.00
7) Phenol-d5	7.077	99	18038	5.526	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.242	67	61524	31.275	ng/u1	0.00
11) 2-Chlorophenol-d4	7.447	132	50494	22.428	ng/u1	-0.01
15) 4-Methylphenol-d8	8.622	113	33950	13.783	ng/u1	-0.01
21) Nitrobenzene-d5	9.075	128	36858	30.745	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.797	143	39267	31.165	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.344	165	63330	26.202	ng/u1	0.00
31) 4-Chloroaniline-d4	10.855	131	90153	24.601	ng/u1	0.00
46) Dimethylphthalate-d6	13.957	166	317463	37.096	ng/u1	0.00
49) Acenaphthylene-d8	14.251	160	311294	33.334	ng/u1	0.00
54) 4-Nitrophenol-d4	14.756	143	8689	5.747	ng/u1	-0.01
60) Fluorene-d10	15.544	176	274578	37.780	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.661	200	53640	33.779	ng/u1	-0.01
73) Anthracene-d10	17.394	188	536092	39.506	ng/u1	-0.01
81) Pyrene-d10	19.686	212	664068	38.660	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.492	264	683175	40.082	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.387	88	24268	21.520	ng/uL	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
Data File : BG058061.D
Acq On : 7 Jul 2023 00:51
Operator : CG/JU
Sample : 03283-15
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EXYZ1

Quant Time: Jul 07 01:50:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 05 23:20:13 2023
Response via : Initial Calibration

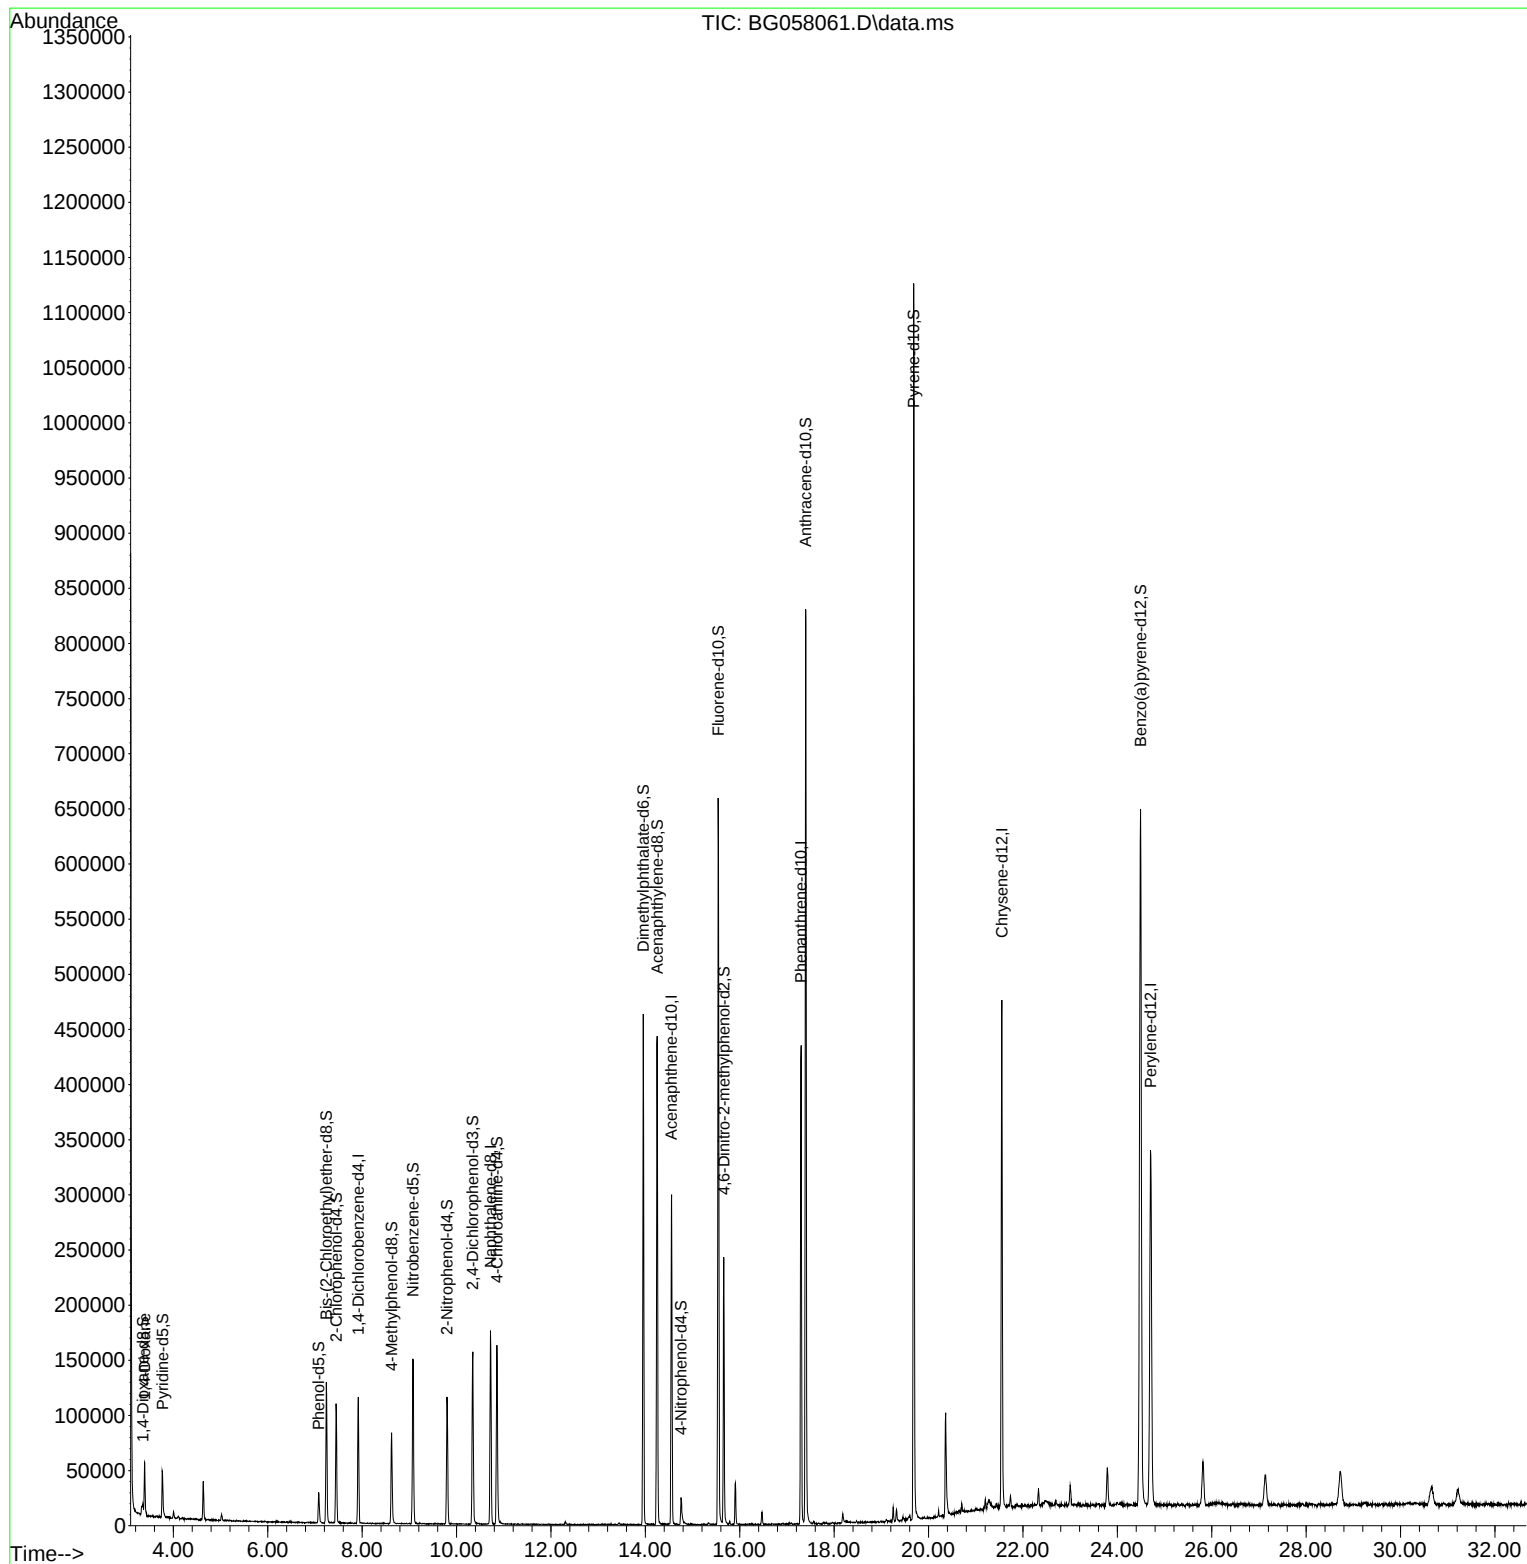

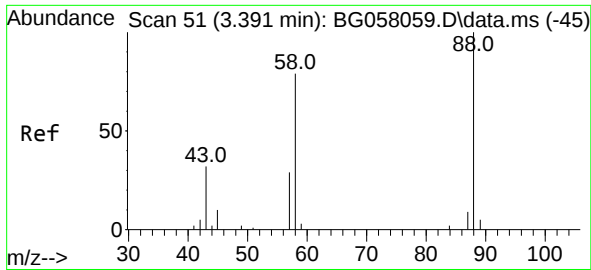

#2
 1,4-Dioxane
 Concen: 21.520 ng/uL
 RT: 3.387 min Scan# 51
 Delta R.T. -0.011 min
 Lab File: BG058061.D
 Acq: 7 Jul 2023 00:51

Instrument :
 BNA_G
 ClientSampleId :
 EXYZ1

Tgt Ion: 88 Resp: 24268
 Ion Ratio Lower Upper
 88 100
 43 28.8 20.6 30.8
 58 86.5 65.5 98.3

