

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
 Data File : BG058024.D
 Acq On : 5 Jul 2023 19:57
 Operator : CG/JU
 Sample : 03494-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG058024.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.658	95	97	100	rBV3	950	1257	0.14%	0.034%
2	3.876	132	134	137	rBV3	1573	1535	0.17%	0.041%
3	4.011	154	157	159	rBV2	1269	1264	0.14%	0.034%
4	4.076	165	168	171	rBV3	819	1467	0.16%	0.039%
5	4.117	171	175	178	rVV5	2359	3421	0.38%	0.091%
6	4.181	184	186	189	rBV4	1165	1167	0.13%	0.031%
7	4.363	216	217	220	rBV3	1143	945	0.10%	0.025%
8	4.745	278	282	285	rBV5	1066	1699	0.19%	0.045%
9	4.857	298	301	304	rBV3	670	975	0.11%	0.026%
10	4.957	313	318	321	rVB3	806	1311	0.14%	0.035%
11	5.756	452	454	459	rVB3	852	1187	0.13%	0.032%
12	6.596	591	597	600	rBV3	854	1717	0.19%	0.046%
13	7.260	707	710	713	rVB3	771	962	0.11%	0.026%
14	7.325	717	721	722	rVB2	1096	1006	0.11%	0.027%
15	7.360	722	727	730	rBV4	941	1673	0.18%	0.045%
16	7.524	750	755	758	rBV4	597	1151	0.13%	0.031%
17	7.830	803	807	809	rBV2	1003	1598	0.18%	0.043%
18	7.924	816	823	829	rBV	144359	241348	26.51%	6.433%
19	9.816	1141	1145	1149	rVB2	885	1127	0.12%	0.030%
20	10.727	1292	1300	1307	rBV	195177	349128	38.35%	9.306%
21	10.774	1307	1308	1315	rVB3	2155	2556	0.28%	0.068%
22	12.548	1604	1610	1613	rBV	639	1102	0.12%	0.029%
23	13.447	1756	1763	1770	rBV	6802	10381	1.14%	0.277%
24	14.557	1945	1952	1966	rBV	319046	510783	56.11%	13.615%
25	16.579	2294	2296	2300	rBV2	696	1045	0.11%	0.028%
26	17.084	2380	2382	2386	rBV2	1281	1480	0.16%	0.039%
27	17.301	2413	2419	2431	rVV	443277	690111	75.80%	18.396%
28	17.671	2478	2482	2484	rBV3	833	1009	0.11%	0.027%
29	17.777	2494	2500	2502	rVB2	803	1197	0.13%	0.032%
30	18.077	2549	2551	2553	rBV2	1022	949	0.10%	0.025%
31	18.188	2568	2570	2572	rBV3	1271	1344	0.15%	0.036%
32	18.230	2576	2577	2581	rVB2	1324	1055	0.12%	0.028%
33	18.341	2593	2596	2598	rBV2	1106	1316	0.14%	0.035%
34	18.794	2672	2673	2676	rBV2	1550	1300	0.14%	0.035%
35	18.893	2687	2690	2692	rBV4	1624	1718	0.19%	0.046%
36	18.929	2692	2696	2697	rBV3	1181	1446	0.16%	0.039%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
 Data File : BG058024.D
 Acq On : 5 Jul 2023 19:57
 Operator : CG/JU
 Sample : 03494-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Title : SVOA CALIBRATION

37	19.176	2735	2738	2741	rBV3	1908	3188	0.35%	0.085%
38	19.223	2744	2746	2751	rVV4	1401	2220	0.24%	0.059%
39	19.311	2759	2761	2763	rBV3	1702	1598	0.18%	0.043%
40	19.364	2768	2770	2771	rBV2	1357	1082	0.12%	0.029%
41	19.452	2783	2785	2787	rVB2	2369	1380	0.15%	0.037%
42	19.475	2787	2789	2790	rBV2	1255	1162	0.13%	0.031%
43	19.493	2790	2792	2795	rVV3	1978	1746	0.19%	0.047%
44	19.546	2799	2801	2802	rBV	1603	1001	0.11%	0.027%
45	19.575	2802	2806	2807	rBV3	2092	2962	0.33%	0.079%
46	19.593	2807	2809	2813	rVB5	1957	1902	0.21%	0.051%
47	19.622	2813	2814	2816	rBV2	1848	1057	0.12%	0.028%
48	20.245	2918	2920	2922	rBV3	3194	1916	0.21%	0.051%
49	21.156	3072	3075	3080	rBV2	13188	23656	2.60%	0.631%
50	21.226	3082	3087	3092	rBV	24388	43576	4.79%	1.162%
51	21.285	3093	3097	3108	rVV	71601	114076	12.53%	3.041%
52	21.555	3137	3143	3152	rBV	496834	793855	87.20%	21.161%
53	24.716	3671	3681	3697	rVB	325260	910389	100.00%	24.267%



Sum of corrected areas: 3751496

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
Data File : BG058024.D
Acq On : 5 Jul 2023 19:57
Operator : CG/JU
Sample : 03494-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

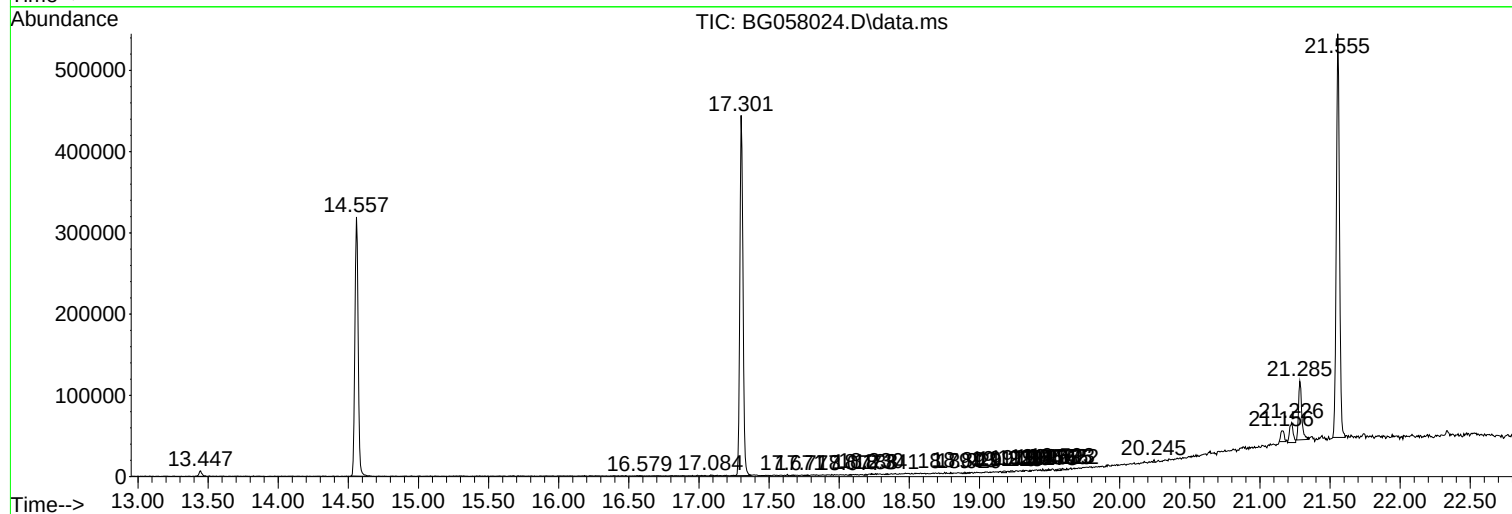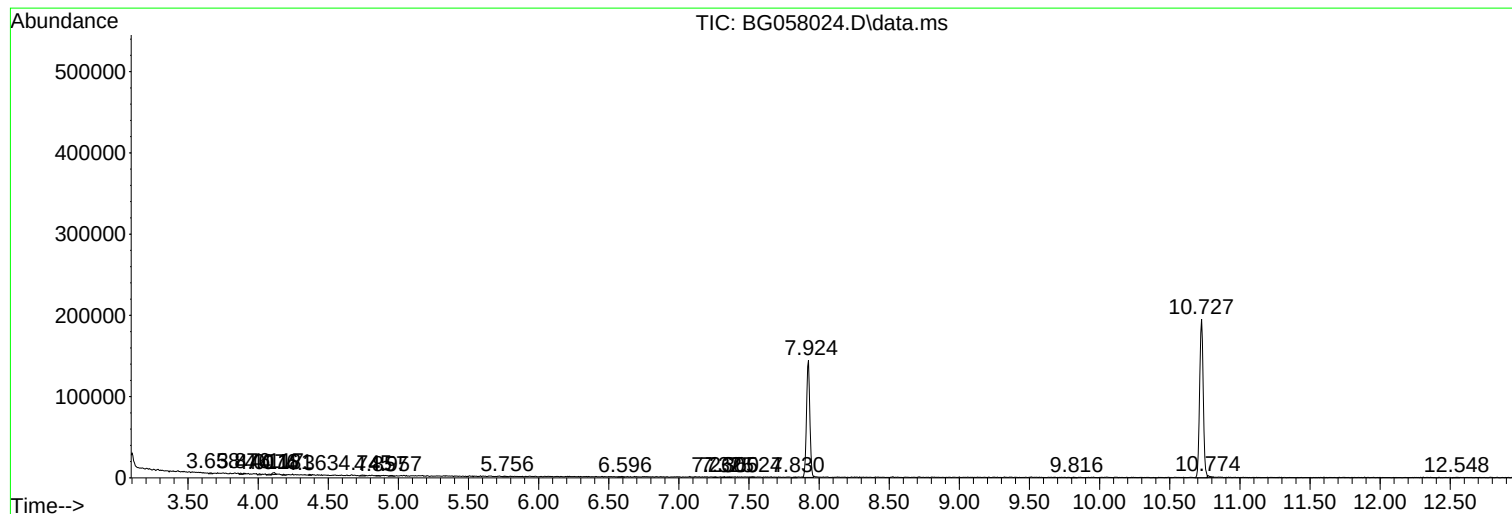

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
Data File : BG058024.D
Acq On : 5 Jul 2023 19:57
Operator : CG/JU
Sample : 03494-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC2-BLANK










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Diethylene glycol dibenzoate Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.285	2.87 ng/ul	114076	Chrysene-d12	21.555

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Diethylene glycol dibenzoate	314	C18H18O5	000120-55-8	83
2			Diethylene glycol dibenzoate	314	C18H18O5	000120-55-8	59
3			2,3-Dimethyl-4a,8a-diphenyl-hexa...	326	C20H22O4	1000297-07-0	43
4			1,3-propanedione, 2-(acetyloxy)-...	282	C17H14O4	1000401-92-5	38
5			N-(6-Methoxy-1,3-benzothiazol-2(...	284	C15H12N2O2S	035353-26-5	35

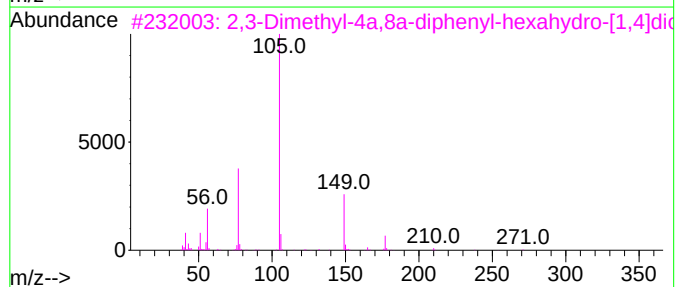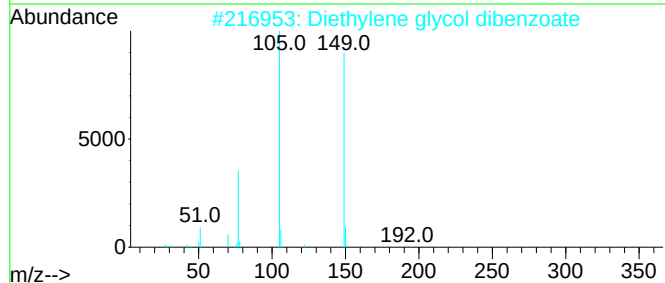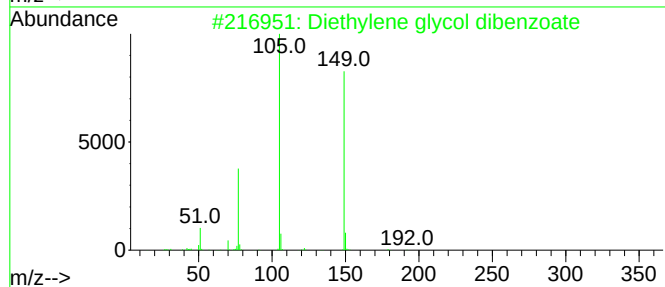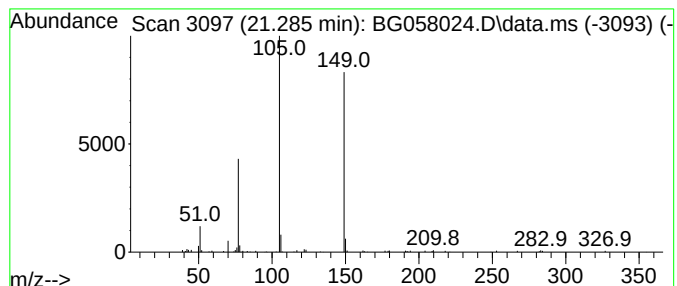

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
Data File : BG058024.D
Acq On : 5 Jul 2023 19:57
Operator : CG/JU
Sample : 03494-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Diethylene glyc...	21.285	2.9	ng/ul	114076	5	21.555	793855	20.0