

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
 Data File : BG058034.D
 Acq On : 6 Jul 2023 3:43
 Operator : CG/JU
 Sample : PB153516BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK516

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG058034.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.357	42	46	54	rVB	21886	30714	1.35%	0.155%
2	3.769	110	116	136	rBV	272633	445460	19.65%	2.251%
3	4.109	169	174	179	rVB3	5435	8602	0.38%	0.043%
4	7.082	673	680	691	rBV	263283	456642	20.14%	2.308%
5	7.247	700	708	718	rBV	227618	375079	16.55%	1.895%
6	7.453	736	743	753	rBV	263824	447003	19.72%	2.259%
7	7.917	815	822	831	rBV	178207	292365	12.90%	1.477%
8	8.628	935	943	956	rBV	332741	590697	26.06%	2.985%
9	9.080	1011	1020	1031	rBV	276680	478173	21.09%	2.416%
10	9.803	1134	1143	1157	rBV	224219	386781	17.06%	1.955%
11	10.343	1228	1235	1245	rBV	314770	557741	24.60%	2.819%
12	10.719	1290	1299	1308	rBV	254897	464310	20.48%	2.346%
13	10.860	1315	1323	1336	rBV	329941	627198	27.67%	3.170%
14	12.312	1563	1570	1577	rBV2	4460	8164	0.36%	0.041%
15	13.446	1757	1763	1770	rBV3	8331	13026	0.57%	0.066%
16	13.957	1843	1850	1859	rBV	683909	1020242	45.01%	5.156%
17	14.250	1893	1900	1915	rBV	725780	1164058	51.35%	5.883%
18	14.556	1945	1952	1963	rBV	445482	679565	29.98%	3.434%
19	14.756	1980	1986	2007	rBV	265470	501100	22.11%	2.532%
20	15.549	2114	2121	2135	rBV	975407	1493686	65.89%	7.548%
21	15.666	2135	2141	2151	rVV	335831	496205	21.89%	2.508%
22	15.784	2158	2161	2165	rVB4	2710	3805	0.17%	0.019%
23	17.300	2412	2419	2429	rBV	612005	911054	40.19%	4.604%
24	17.400	2429	2436	2448	rVB2	1133502	1749651	77.19%	8.842%
25	19.251	2747	2751	2756	rVB4	15989	23062	1.02%	0.117%
26	19.321	2759	2763	2770	rVB	13449	20355	0.90%	0.103%
27	19.691	2819	2826	2838	rBV	1398341	2109573	93.06%	10.661%
28	20.050	2883	2887	2888	rBV4	2118	2947	0.13%	0.015%
29	20.461	2954	2957	2960	rBV5	4223	5994	0.26%	0.030%
30	20.555	2971	2973	2975	rBV3	2512	2523	0.11%	0.013%
31	21.278	3093	3096	3104	rBV	19282	35016	1.54%	0.177%
32	21.554	3136	3143	3153	rVB	579856	976676	43.09%	4.936%
33	24.497	3633	3644	3660	rVB2	818558	2266792	100.00%	11.455%
34	24.709	3670	3680	3693	rVB	398433	1143754	50.46%	5.780%

Sum of corrected areas: 19788013

Instrument :

BNA_G

ClientSampleId :




SBLK516

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
Data File : BG058034.D
Acq On : 6 Jul 2023 3:43
Operator : CG/JU
Sample : PB153516BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK516

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

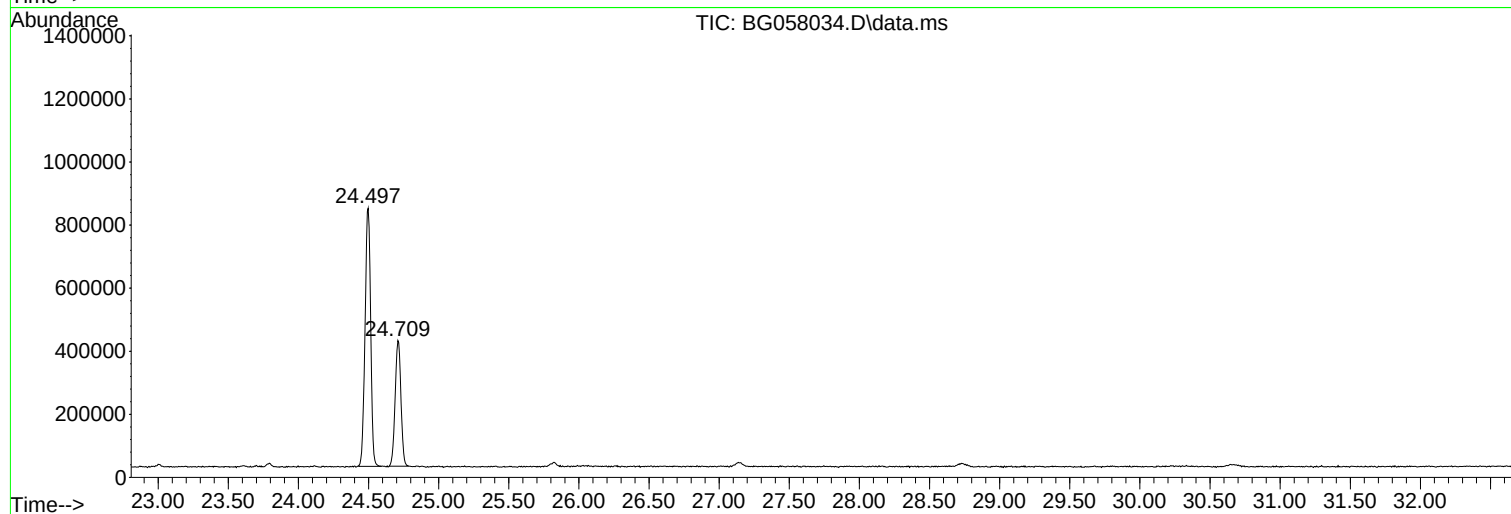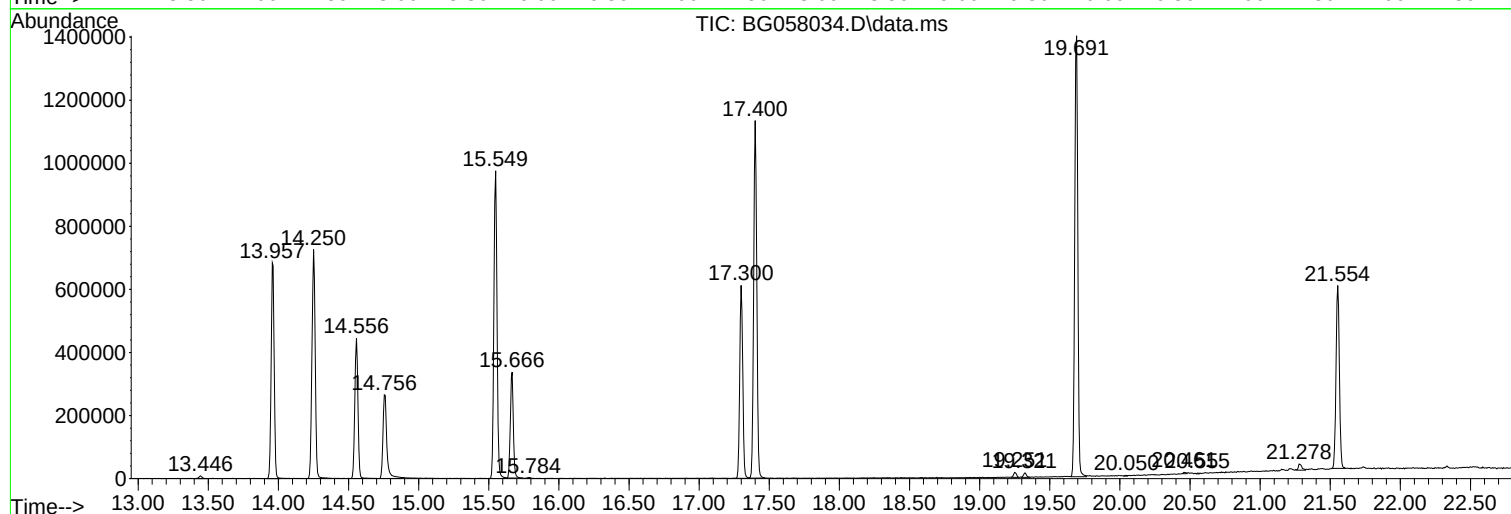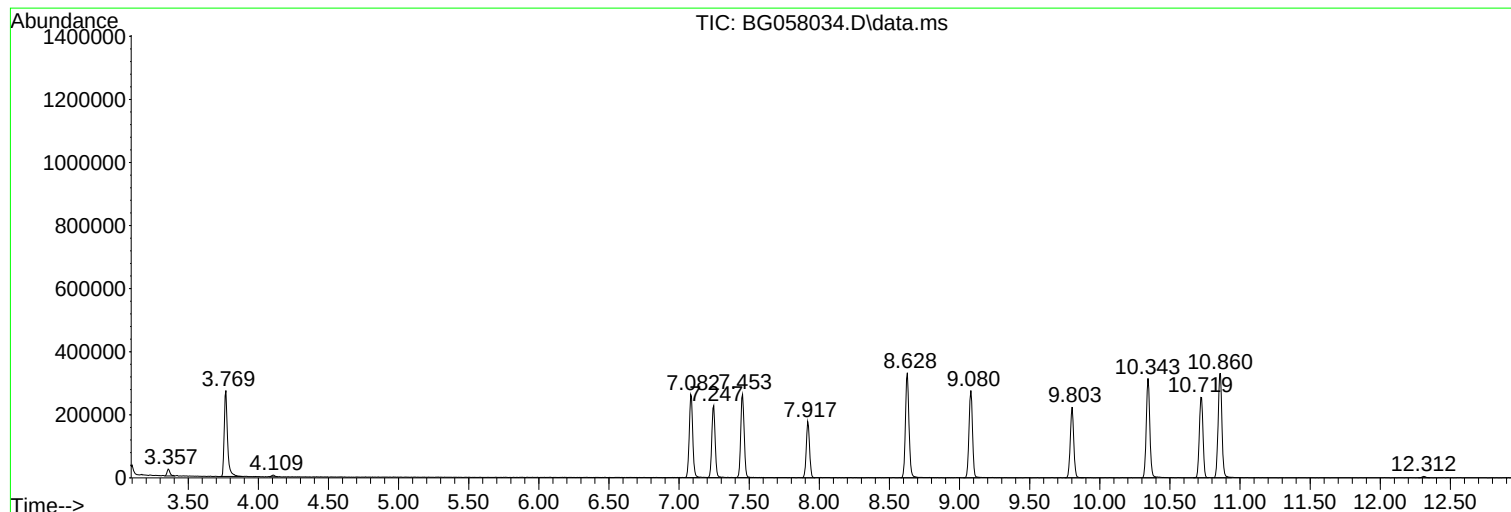

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
Data File : BG058034.D
Acq On : 6 Jul 2023 3:43
Operator : CG/JU
Sample : PB153516BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK516

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
Data File : BG058034.D
Acq On : 6 Jul 2023 3:43
Operator : CG/JU
Sample : PB153516BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK516

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc