

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
 Data File : BG058037.D
 Acq On : 6 Jul 2023 5:50
 Operator : CG/JU
 Sample : 03257-07
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EXYY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG058037.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.355	41	45	52	rBV	19263	28854	0.84%	0.115%
2	3.766	110	115	132	rBV	138050	231560	6.70%	0.926%
3	4.007	151	156	160	rVB2	4740	6077	0.18%	0.024%
4	4.101	169	172	179	rVB3	5141	7674	0.22%	0.031%
5	4.636	259	263	266	rBV3	4050	4097	0.12%	0.016%
6	7.086	672	680	689	rBV	117942	202592	5.86%	0.810%
7	7.245	699	707	719	rBV	280515	456771	13.22%	1.826%
8	7.450	733	742	753	rBV	262674	437373	12.66%	1.749%
9	7.920	815	822	829	rBV	213757	355788	10.30%	1.422%
10	8.625	934	942	953	rBV	236574	417582	12.09%	1.669%
11	9.078	1012	1019	1032	rBV	332393	589129	17.05%	2.355%
12	9.207	1037	1041	1050	rBV6	1605	4128	0.12%	0.017%
13	9.800	1135	1142	1153	rBV	256971	454455	13.15%	1.817%
14	10.341	1227	1234	1250	rBV	354440	639564	18.51%	2.557%
15	10.723	1290	1299	1309	rBV	309732	548333	15.87%	2.192%
16	10.858	1314	1322	1333	rBV	395297	705617	20.42%	2.821%
17	12.309	1563	1569	1573	rBV2	6362	9682	0.28%	0.039%
18	13.443	1757	1762	1771	rVB2	6707	10816	0.31%	0.043%
19	13.960	1843	1850	1860	rBV	912076	1309856	37.91%	5.237%
20	14.248	1892	1899	1907	rBV	916250	1457044	42.17%	5.825%
21	14.554	1944	1951	1960	rBV	506263	792456	22.94%	3.168%
22	14.759	1980	1986	2003	rBV	121584	229148	6.63%	0.916%
23	15.341	2078	2085	2090	rBV2	10406	14379	0.42%	0.057%
24	15.547	2113	2120	2134	rBV	1252615	2000926	57.91%	7.999%
25	15.664	2134	2140	2153	rVV	524100	753744	21.82%	3.013%
26	15.782	2156	2160	2166	rVB3	5065	8347	0.24%	0.033%
27	17.033	2369	2373	2379	rVB3	5939	9185	0.27%	0.037%
28	17.298	2412	2418	2428	rBV	711610	1115858	32.30%	4.461%
29	17.403	2428	2436	2452	rVB	1532003	2502326	72.43%	10.004%
30	17.574	2460	2465	2470	rBV	3158	4530	0.13%	0.018%
31	17.956	2526	2530	2534	rVB4	3204	4525	0.13%	0.018%
32	18.185	2566	2569	2575	rBV2	7240	11941	0.35%	0.048%
33	18.255	2578	2581	2584	rVB	3888	4697	0.14%	0.019%
34	18.473	2612	2618	2623	rBV4	3028	6256	0.18%	0.025%
35	19.031	2709	2713	2718	rVB	39102	47021	1.36%	0.188%
36	19.254	2746	2751	2756	rVB	25587	38330	1.11%	0.153%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
 Data File : BG058037.D
 Acq On : 6 Jul 2023 5:50
 Operator : CG/JU
 Sample : 03257-07
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EXYY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Title : SVOA CALIBRATION

37	19.319	2758	2762	2769	rVB2	25119	43268	1.25%	0.173%
38	19.601	2807	2810	2813	rBV3	4198	4778	0.14%	0.019%
39	19.689	2818	2825	2840	rBV	2097473	3077942	89.09%	12.305%
40	20.218	2912	2915	2917	rBV4	2384	3624	0.10%	0.014%
41	20.647	2985	2988	2989	rBV3	5306	5023	0.15%	0.020%
42	20.658	2989	2990	2996	rVB6	5266	6515	0.19%	0.026%
43	21.281	3093	3096	3099	rBV	11530	14076	0.41%	0.056%
44	21.440	3120	3123	3127	rVB3	14276	19305	0.56%	0.077%
45	21.551	3136	3142	3153	rBV	736874	1264313	36.59%	5.055%
46	22.333	3272	3275	3280	rVB5	10391	13793	0.40%	0.055%
47	23.003	3383	3389	3395	rVB5	17572	40463	1.17%	0.162%
48	23.790	3518	3523	3530	rVB2	31581	61936	1.79%	0.248%
49	24.501	3632	3644	3658	rBV2	1240360	3454993	100.00%	13.812%
50	24.712	3669	3680	3695	rVB	539074	1496562	43.32%	5.983%
51	25.817	3861	3868	3877	rVB3	31538	86333	2.50%	0.345%




Sum of corrected areas: 25013585

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
Data File : BG058037.D
Acq On : 6 Jul 2023 5:50
Operator : CG/JU
Sample : 03257-07
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EXYY3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

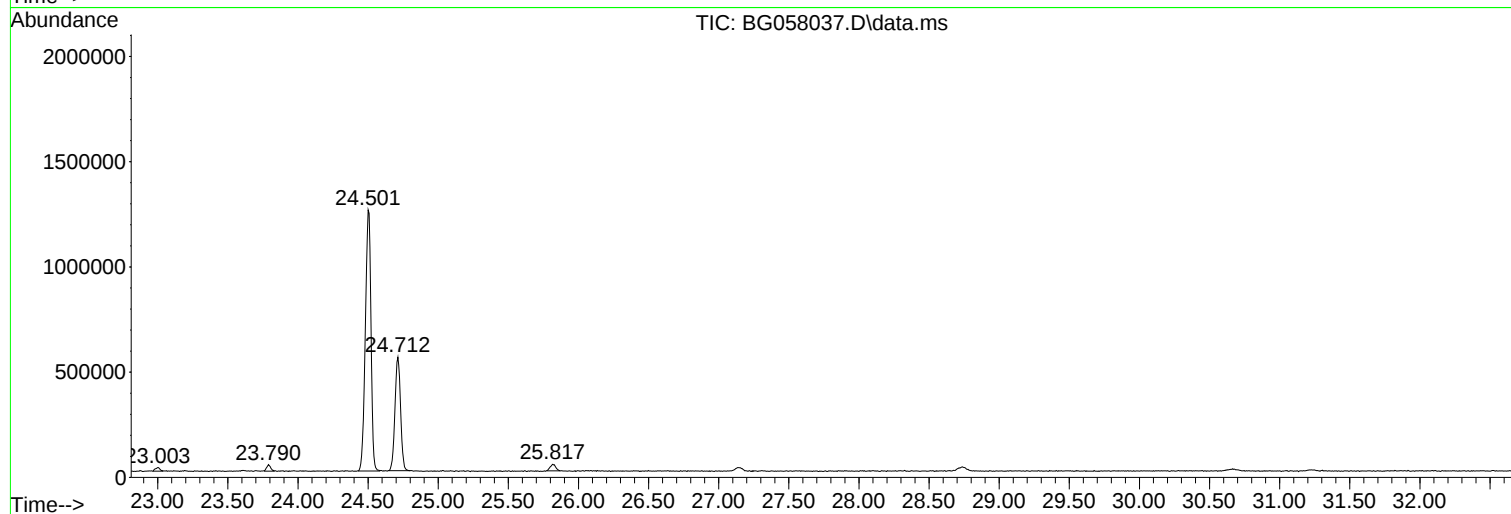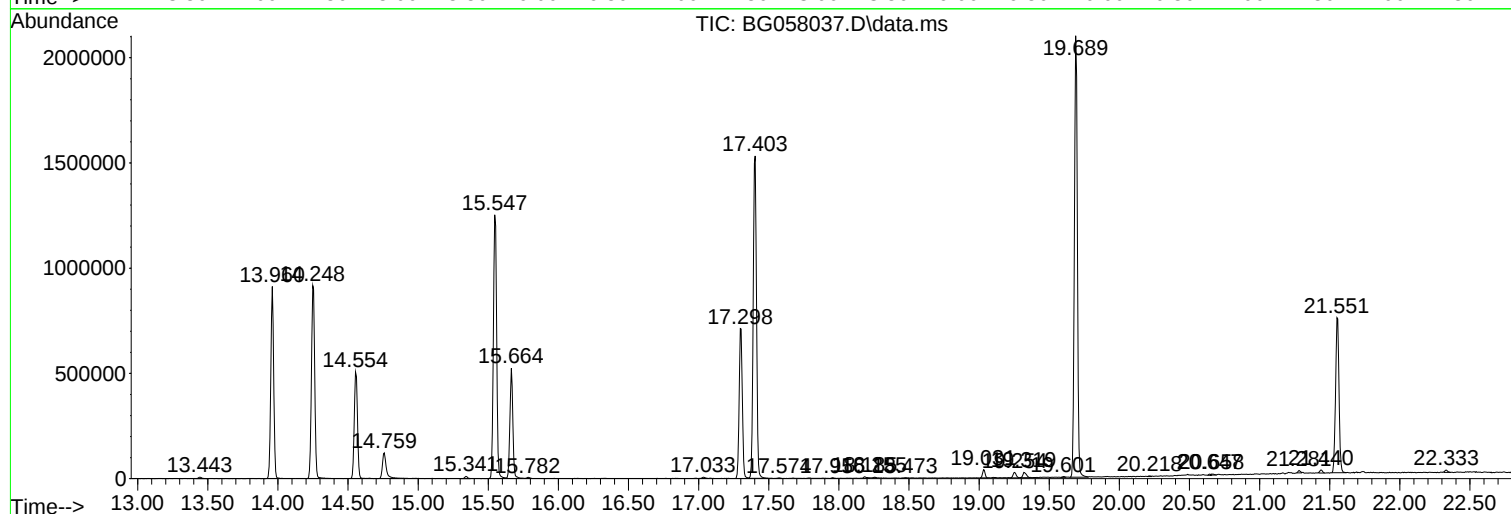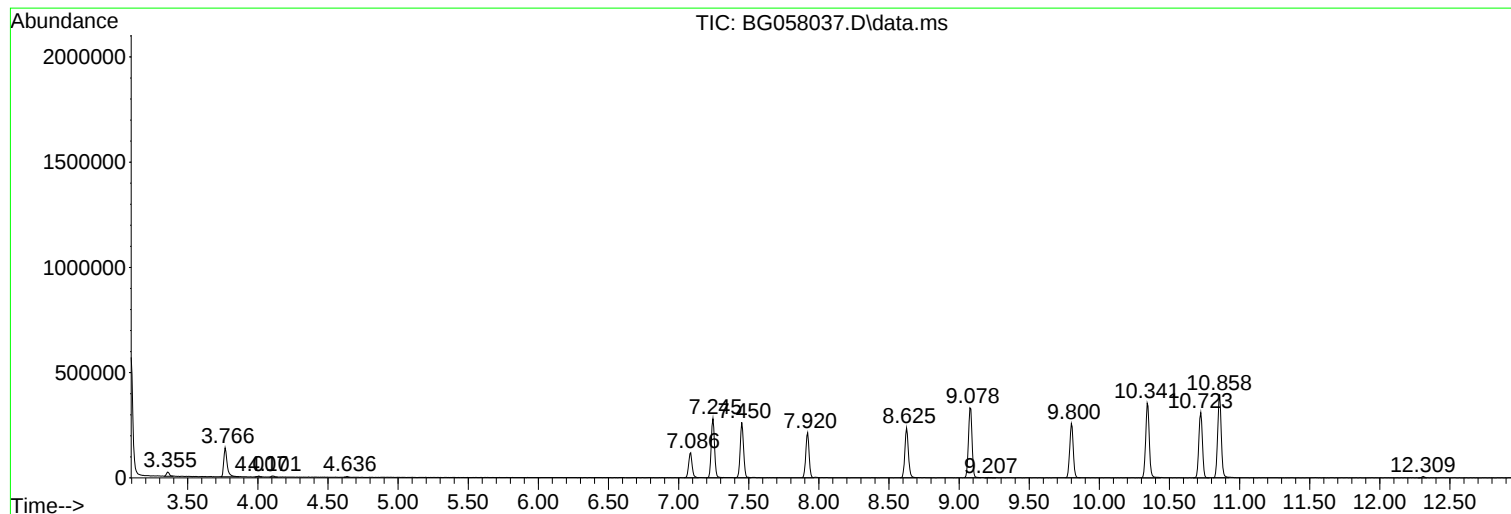

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
Data File : BG058037.D
Acq On : 6 Jul 2023 5:50
Operator : CG/JU
Sample : 03257-07
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EXYY3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
Data File : BG058037.D
Acq On : 6 Jul 2023 5:50
Operator : CG/JU
Sample : 03257-07
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EXYY3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------