

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
 Data File : BG058038.D
 Acq On : 6 Jul 2023 6:31
 Operator : CG/JU
 Sample : 03257-11
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EXYY1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG058038.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	42	46	52	rVB	14153	20986	0.83%	0.109%
2	3.769	112	116	126	rBV	75402	123480	4.91%	0.641%
3	4.004	151	156	161	rVB2	4864	7006	0.28%	0.036%
4	4.104	170	173	179	rVV3	4396	6706	0.27%	0.035%
5	4.639	258	264	269	rBV6	1992	3870	0.15%	0.020%
6	7.083	674	680	694	rVB	49713	84307	3.35%	0.437%
7	7.242	700	707	720	rBV	202751	335580	13.34%	1.741%
8	7.453	736	743	752	rBV	180493	299469	11.90%	1.554%
9	7.917	815	822	829	rBV	182586	300951	11.96%	1.561%
10	8.622	936	942	953	rBV	143678	255843	10.17%	1.327%
11	9.081	1012	1020	1028	rBV	243656	427575	16.99%	2.218%
12	9.803	1135	1143	1151	rBV	177158	322296	12.81%	1.672%
13	10.344	1228	1235	1248	rBV	261003	464827	18.47%	2.412%
14	10.720	1292	1299	1308	rBV	268228	476327	18.93%	2.471%
15	10.855	1315	1322	1336	rBV	284051	529670	21.05%	2.748%
16	12.306	1564	1569	1575	rVB4	4780	7310	0.29%	0.038%
17	13.446	1755	1763	1770	rBV2	7269	12410	0.49%	0.064%
18	13.957	1844	1850	1860	rBV	690954	989406	39.32%	5.133%
19	14.251	1892	1900	1909	rBV	692873	1096422	43.58%	5.689%
20	14.557	1945	1952	1960	rBV	455081	711556	28.28%	3.692%
21	14.756	1980	1986	1998	rBV	49261	99955	3.97%	0.519%
22	15.344	2081	2086	2093	rBV2	9647	14202	0.56%	0.074%
23	15.550	2114	2121	2135	rBV	963916	1503073	59.74%	7.798%
24	15.661	2135	2140	2152	rVB	345063	530290	21.08%	2.751%
25	15.785	2157	2161	2165	rVB3	3109	4794	0.19%	0.025%
26	17.030	2369	2373	2380	rBV4	5094	7079	0.28%	0.037%
27	17.301	2412	2419	2429	rBV	677013	997914	39.66%	5.177%
28	17.400	2429	2436	2453	rVB	1227059	1905090	75.72%	9.884%
29	17.571	2462	2465	2470	rBV3	2917	2840	0.11%	0.015%
30	17.953	2528	2530	2539	rBV4	2175	5090	0.20%	0.026%
31	18.188	2565	2570	2576	rBV2	9031	14950	0.59%	0.078%
32	18.258	2577	2582	2586	rVB	4748	7568	0.30%	0.039%
33	19.034	2709	2714	2719	rVB	18550	20857	0.83%	0.108%
34	19.251	2746	2751	2757	rVB2	18741	28848	1.15%	0.150%
35	19.322	2759	2763	2773	rVB2	19334	33861	1.35%	0.176%
36	19.457	2784	2786	2790	rBV4	4110	5490	0.22%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
 Data File : BG058038.D
 Acq On : 6 Jul 2023 6:31
 Operator : CG/JU
 Sample : 03257-11
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EXYY1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Title : SVOA CALIBRATION

37	19.610	2807	2812	2813	rBV5	3265	3476	0.14%	0.018%
38	19.692	2819	2826	2838	rBV	1584848	2306076	91.65%	11.965%
39	20.138	2899	2902	2904	rVB4	2611	2996	0.12%	0.016%
40	21.278	3093	3096	3102	rBV	13712	21652	0.86%	0.112%
41	21.443	3120	3124	3129	rBV2	13179	18359	0.73%	0.095%
42	21.554	3136	3143	3154	rVB	655580	1080328	42.94%	5.605%
43	22.330	3272	3275	3278	rBV5	7312	9915	0.39%	0.051%
44	23.793	3519	3524	3532	rVB4	25350	51071	2.03%	0.265%
45	24.498	3632	3644	3658	rBV2	861727	2516081	100.00%	13.054%
46	24.715	3670	3681	3695	rVB	465667	1315476	52.28%	6.825%
47	25.820	3863	3869	3878	rVB4	36393	98861	3.93%	0.513%
48	27.142	4088	4094	4103	rVB2	29587	92239	3.67%	0.479%
49	28.734	4358	4365	4380	rVB6	24516	99743	3.96%	0.517%




Sum of corrected areas: 19274171

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
Data File : BG058038.D
Acq On : 6 Jul 2023 6:31
Operator : CG/JU
Sample : 03257-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EXYY1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

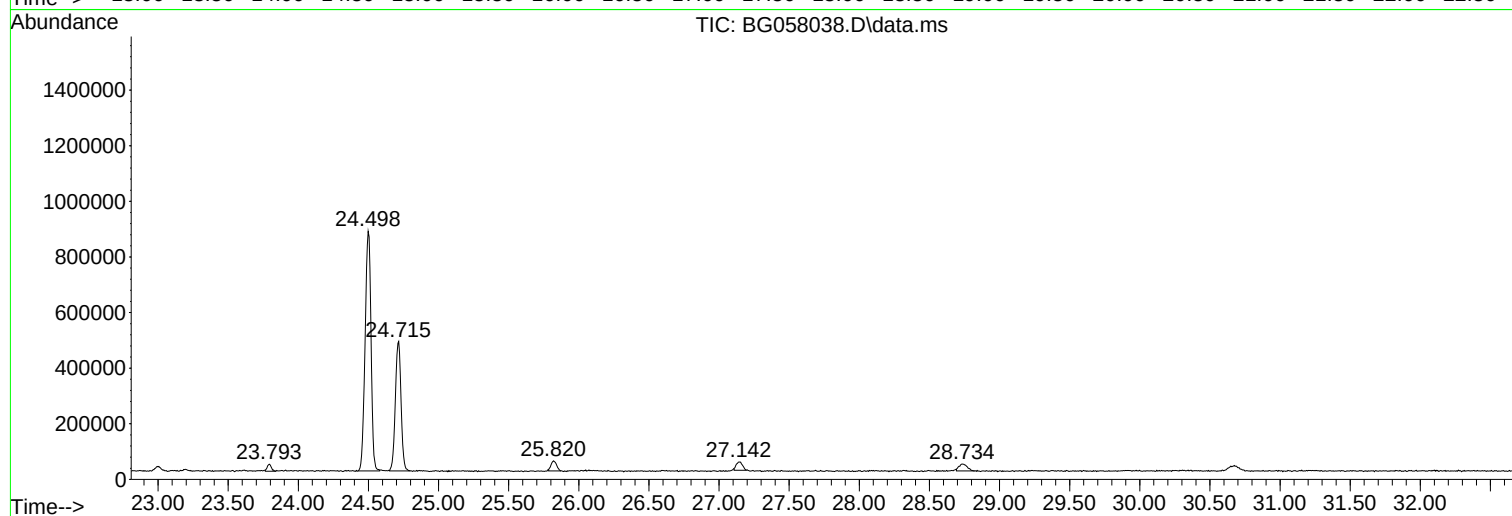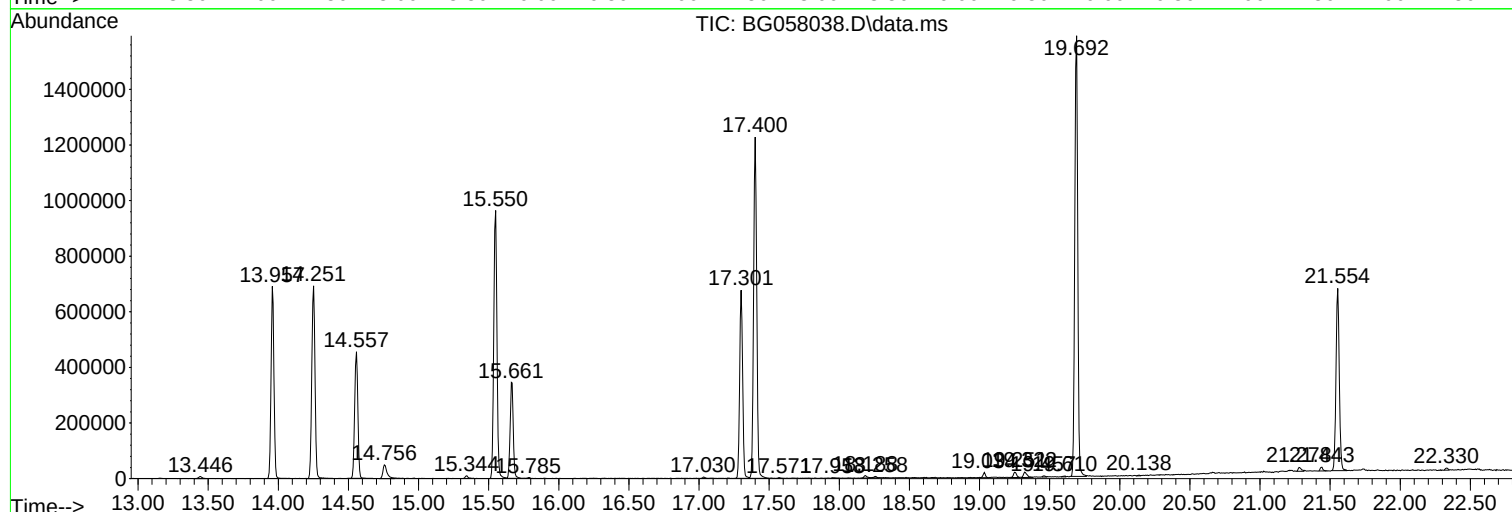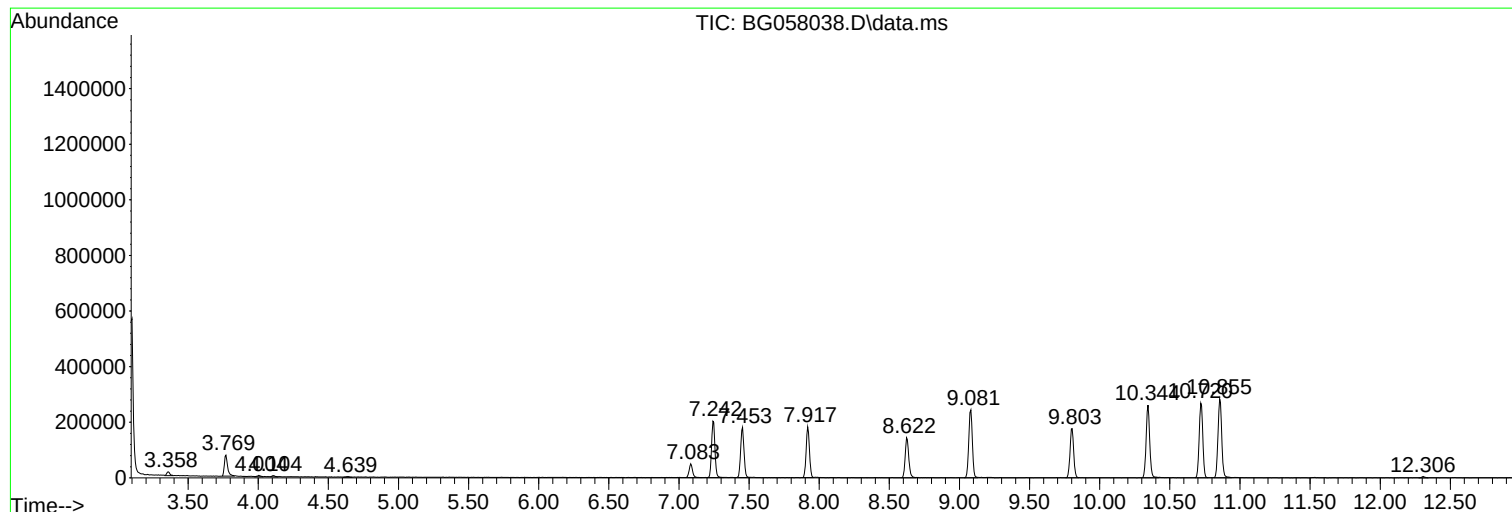

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
Data File : BG058038.D
Acq On : 6 Jul 2023 6:31
Operator : CG/JU
Sample : 03257-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EXYY1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
Data File : BG058038.D
Acq On : 6 Jul 2023 6:31
Operator : CG/JU
Sample : 03257-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EXYY1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
