

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
 Data File : BG058043.D
 Acq On : 6 Jul 2023 10:02
 Operator : CG/JU
 Sample : 03258-06
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCGW5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG058043.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	42	46	54	rVB	15523	22581	0.92%	0.120%
2	3.770	112	116	125	rBV	58067	91604	3.72%	0.485%
3	4.005	153	156	162	rVB4	5343	7966	0.32%	0.042%
4	4.105	170	173	179	rVB4	2426	4599	0.19%	0.024%
5	5.209	356	361	365	rVB2	5232	7758	0.31%	0.041%
6	7.084	674	680	693	rVB	64270	112818	4.58%	0.597%
7	7.248	701	708	717	rBV	220646	369854	15.00%	1.958%
8	7.454	736	743	750	rBV	205731	348476	14.14%	1.845%
9	7.918	815	822	830	rVB	169242	277584	11.26%	1.470%
10	8.623	936	942	952	rBV	176244	308570	12.52%	1.634%
11	9.081	1011	1020	1027	rBV	270729	476063	19.31%	2.520%
12	9.804	1136	1143	1150	rBV	206097	367220	14.90%	1.944%
13	10.344	1227	1235	1251	rBV	286596	522944	21.22%	2.768%
14	10.720	1292	1299	1307	rBV	242039	427896	17.36%	2.265%
15	10.856	1314	1322	1335	rBV	242869	432454	17.54%	2.289%
16	12.307	1564	1569	1575	rVB2	4363	7649	0.31%	0.040%
17	13.441	1758	1762	1768	rBV3	8179	13417	0.54%	0.071%
18	13.958	1843	1850	1861	rBV	676713	983928	39.92%	5.209%
19	14.252	1893	1900	1910	rBV	720615	1126163	45.69%	5.962%
20	14.557	1945	1952	1965	rVB	413984	639242	25.93%	3.384%
21	14.757	1981	1986	1999	rBV	60622	117704	4.78%	0.623%
22	15.292	2073	2077	2080	rBV	2422	2641	0.11%	0.014%
23	15.550	2114	2121	2135	rBV	987174	1505708	61.09%	7.971%
24	15.662	2135	2140	2150	rVB	355539	519572	21.08%	2.751%
25	15.791	2158	2162	2171	rVB4	4584	7425	0.30%	0.039%
26	15.908	2177	2182	2190	rVB	37892	55105	2.24%	0.292%
27	17.301	2412	2419	2429	rBV	593569	890687	36.13%	4.715%
28	17.401	2429	2436	2450	rVV2	1197370	1847607	74.96%	9.781%
29	17.577	2462	2466	2472	rVB4	1880	2839	0.12%	0.015%
30	18.182	2564	2569	2578	rBV3	30977	51861	2.10%	0.275%
31	18.253	2578	2581	2585	rVB	4311	5512	0.22%	0.029%
32	18.682	2650	2654	2658	rBV6	3704	6071	0.25%	0.032%
33	19.005	2706	2709	2712	rBV5	1796	2616	0.11%	0.014%
34	19.252	2746	2751	2758	rBV2	17149	26156	1.06%	0.138%
35	19.322	2758	2763	2769	rBV	16465	25601	1.04%	0.136%
36	19.404	2773	2777	2780	rBV3	1943	3330	0.14%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
 Data File : BG058043.D
 Acq On : 6 Jul 2023 10:02
 Operator : CG/JU
 Sample : 03258-06
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCGW5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Title : SVOA CALIBRATION

37	19.457	2782	2786	2792	rBV6	9613	17010	0.69%	0.090%
38	19.604	2806	2811	2815	rBV5	5104	6521	0.26%	0.035%
39	19.692	2819	2826	2842	rVV	1529485	2305180	93.52%	12.204%
40	20.215	2912	2915	2916	rBV3	3857	3352	0.14%	0.018%
41	20.662	2985	2991	2995	rBV8	5945	11954	0.48%	0.063%
42	20.879	3026	3028	3031	rBV4	3398	3662	0.15%	0.019%
43	21.232	3081	3088	3094	rBV9	27674	81059	3.29%	0.429%
44	21.437	3120	3123	3129	rVB2	13906	19001	0.77%	0.101%
45	21.555	3136	3143	3153	rVB	611484	1002292	40.66%	5.306%
46	22.330	3271	3275	3279	rBV4	11679	15688	0.64%	0.083%
47	23.006	3385	3390	3396	rVB5	15819	25659	1.04%	0.136%
48	23.188	3419	3421	3427	rVB2	12784	19789	0.80%	0.105%
49	23.787	3518	3523	3530	rVB3	20566	42698	1.73%	0.226%
50	24.498	3632	3644	3661	rVB2	887490	2464911	100.00%	13.049%
51	24.710	3670	3680	3691	rBV2	423920	1164963	47.26%	6.167%
52	25.021	3731	3733	3735	rBV3	4867	4414	0.18%	0.023%
53	25.815	3862	3868	3877	rVB3	25422	63250	2.57%	0.335%
54	27.131	4088	4092	4093	rBV3	14866	18568	0.75%	0.098%




Sum of corrected areas: 18889192

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
Data File : BG058043.D
Acq On : 6 Jul 2023 10:02
Operator : CG/JU
Sample : 03258-06
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCGW5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

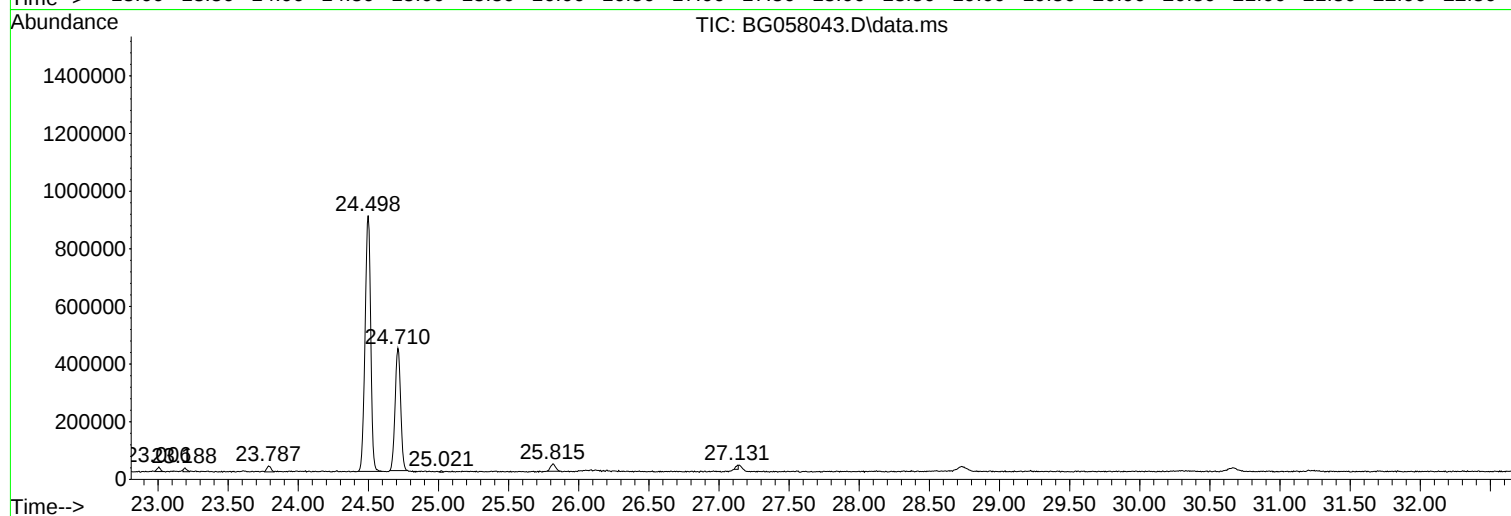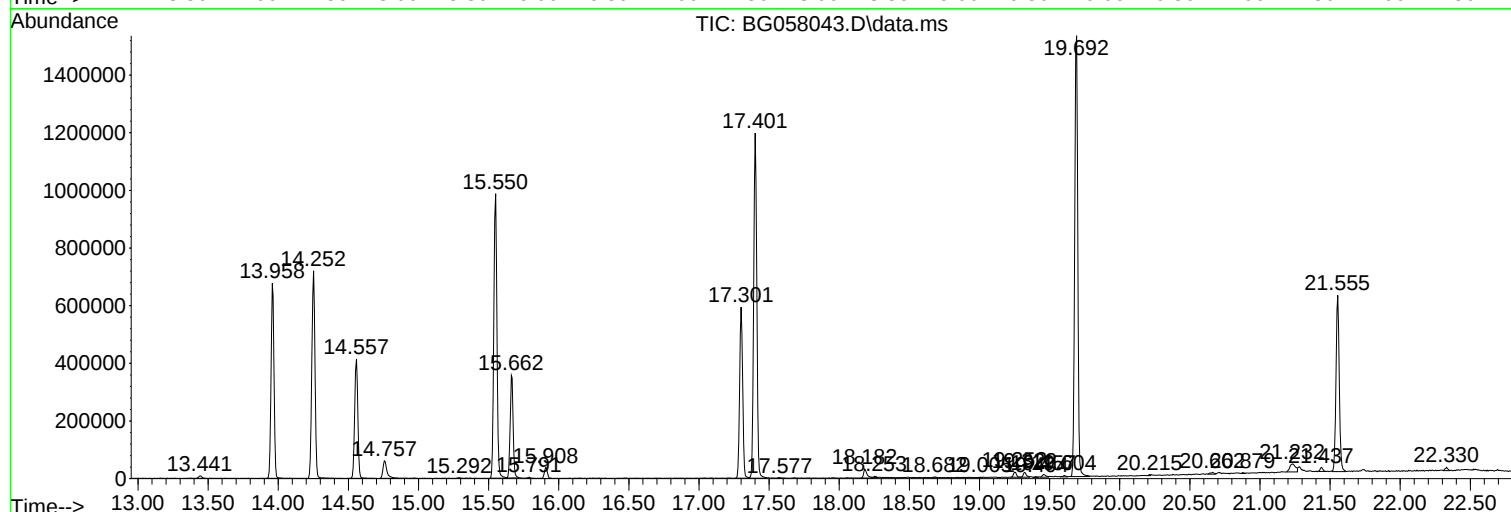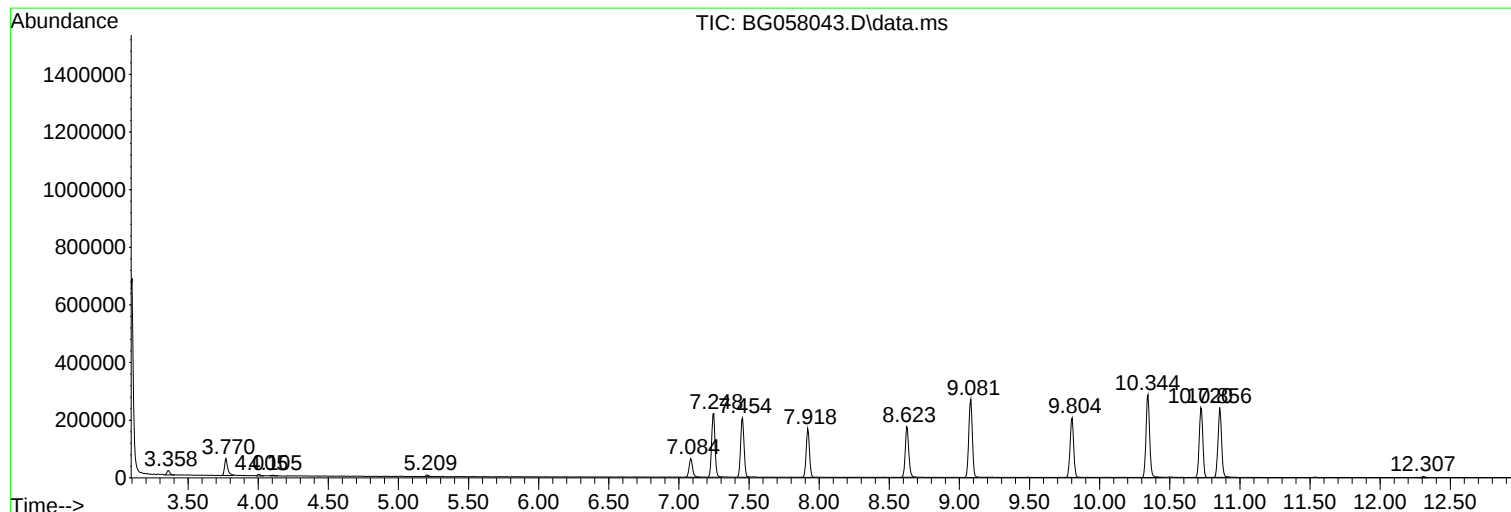

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
Data File : BG058043.D
Acq On : 6 Jul 2023 10:02
Operator : CG/JU
Sample : 03258-06
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCGW5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
Data File : BG058043.D
Acq On : 6 Jul 2023 10:02
Operator : CG/JU
Sample : 03258-06
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCGW5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------