

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
 Data File : BG058046.D
 Acq On : 6 Jul 2023 12:06
 Operator : CG/JU
 Sample : PB153592BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK592

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG058046.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	42	46	53	rVB	19077	27221	1.27%	0.157%
2	3.763	110	115	131	rBV	237126	382563	17.82%	2.204%
3	4.110	170	174	178	rBV4	4984	6720	0.31%	0.039%
4	7.083	673	680	697	rVV	234198	396341	18.47%	2.284%
5	7.241	700	707	718	rBV	186421	318448	14.84%	1.835%
6	7.453	736	743	750	rBV	222722	382454	17.82%	2.204%
7	7.917	815	822	832	rVB	140890	231593	10.79%	1.334%
8	8.622	935	942	954	rBV	284084	500070	23.30%	2.881%
9	9.080	1011	1020	1029	rBV	232508	404256	18.83%	2.329%
10	9.803	1135	1143	1153	rVB	188622	325828	15.18%	1.877%
11	10.344	1227	1235	1250	rBV	267969	482802	22.49%	2.782%
12	10.720	1292	1299	1309	rBV	201759	362396	16.88%	2.088%
13	10.855	1315	1322	1337	rBV	287566	531983	24.79%	3.065%
14	12.306	1565	1569	1577	rBV2	3847	6322	0.29%	0.036%
15	13.446	1757	1763	1769	rBV3	4622	7880	0.37%	0.045%
16	13.957	1844	1850	1860	rBV	589912	867569	40.42%	4.999%
17	14.251	1893	1900	1913	rBV	632113	996155	46.41%	5.740%
18	14.556	1945	1952	1964	rBV	351170	541132	25.21%	3.118%
19	14.756	1980	1986	2004	rBV	254547	457953	21.34%	2.639%
20	15.549	2114	2121	2134	rBV	866167	1296480	60.40%	7.470%
21	15.667	2134	2141	2149	rVB	312665	453652	21.14%	2.614%
22	15.784	2158	2161	2167	rVB2	3484	4462	0.21%	0.026%
23	17.300	2413	2419	2429	rBV	508969	760941	35.45%	4.385%
24	17.400	2429	2436	2452	rVB	1020625	1569001	73.10%	9.041%
25	19.257	2747	2752	2755	rBV4	15184	23450	1.09%	0.135%
26	19.321	2759	2763	2771	rVV2	11846	18679	0.87%	0.108%
27	19.691	2819	2826	2844	rVV	1371784	1971708	91.86%	11.361%
28	21.554	3136	3143	3151	rBV2	520700	856469	39.90%	4.935%
29	21.871	3195	3197	3198	rBV2	3147	2291	0.11%	0.013%
30	23.005	3388	3390	3395	rVB5	8495	10441	0.49%	0.060%
31	24.498	3632	3644	3656	rBV2	775466	2146386	100.00%	12.368%
32	24.709	3670	3680	3694	rVB2	364105	1011033	47.10%	5.826%




Sum of corrected areas: 17354679

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
Data File : BG058046.D
Acq On : 6 Jul 2023 12:06
Operator : CG/JU
Sample : PB153592BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK592

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

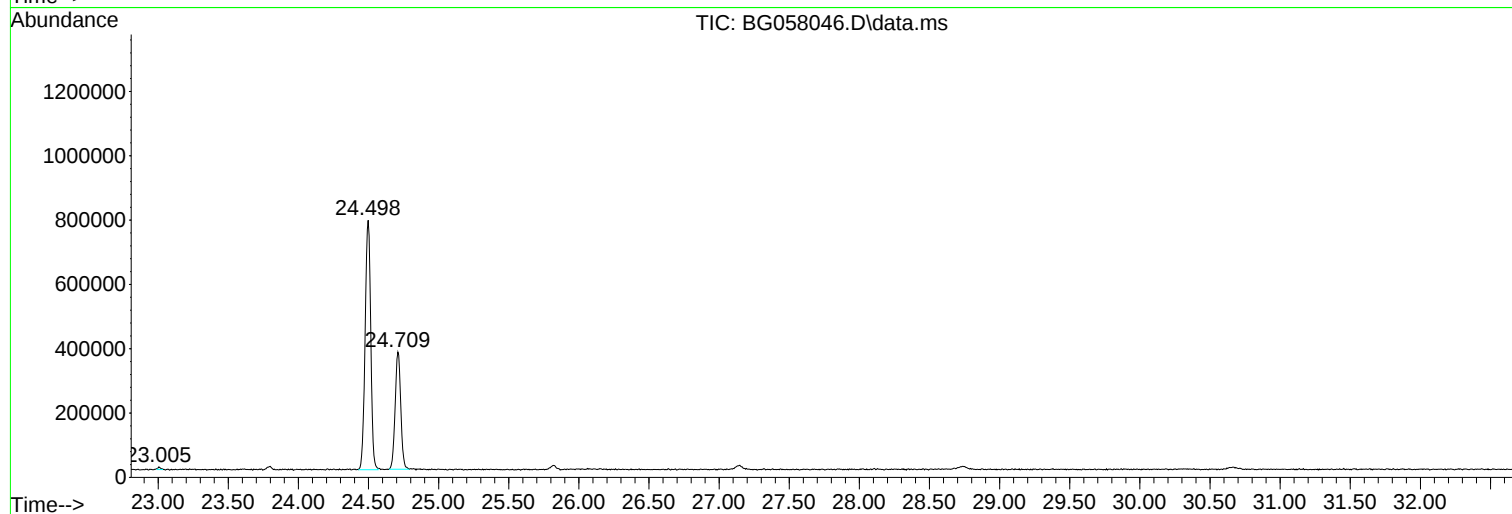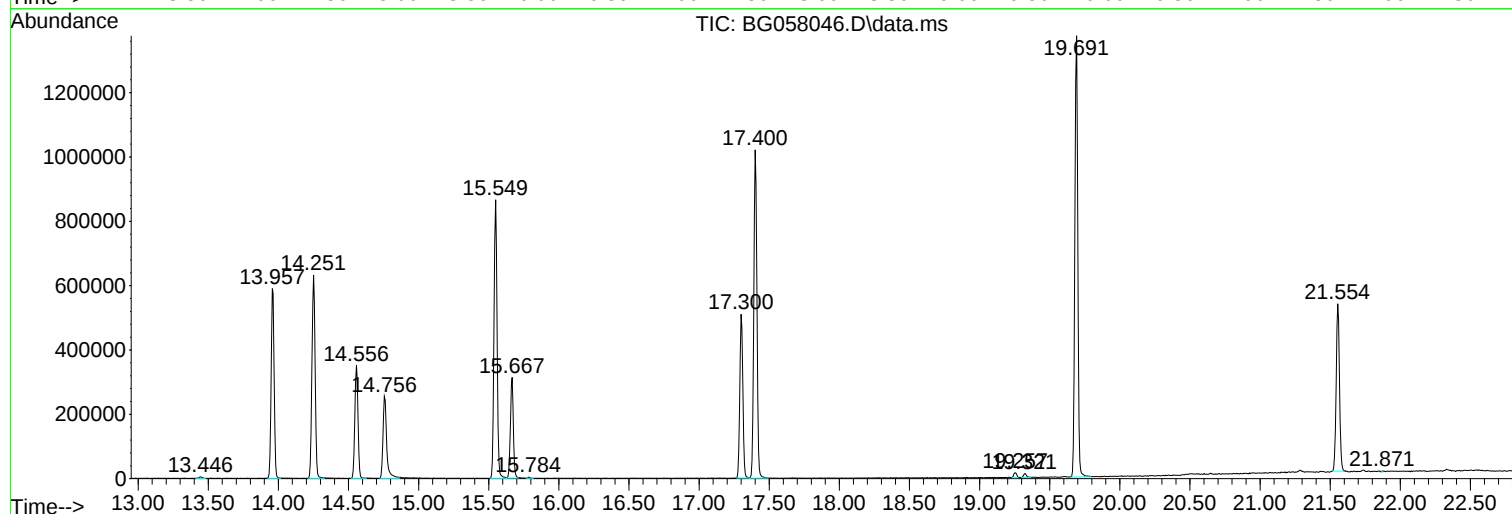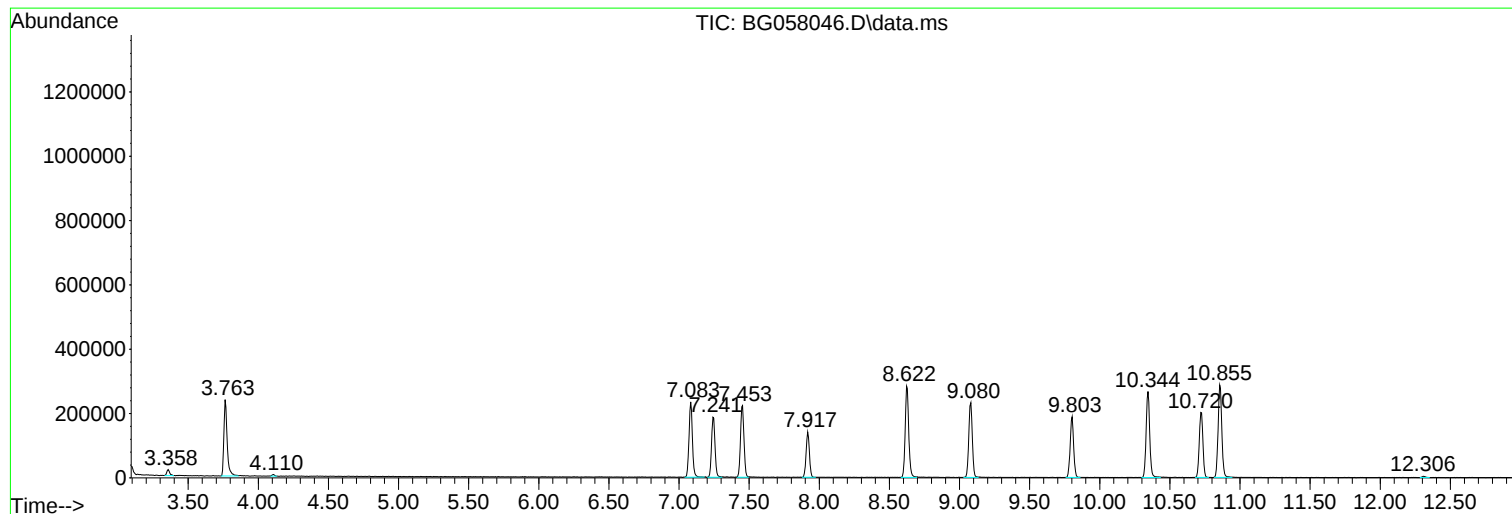

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
Data File : BG058046.D
Acq On : 6 Jul 2023 12:06
Operator : CG/JU
Sample : PB153592BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK592

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
Data File : BG058046.D
Acq On : 6 Jul 2023 12:06
Operator : CG/JU
Sample : PB153592BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK592

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------