

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
 Data File : BG058050.D
 Acq On : 6 Jul 2023 14:56
 Operator : CG/JU
 Sample : PB153588BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK588

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG058050.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.359	42	46	54	rVB	13910	20919	1.34%	0.167%
2	3.765	110	115	128	rBV	167345	265204	17.03%	2.119%
3	4.105	169	173	178	rBV4	2055	3169	0.20%	0.025%
4	7.084	673	680	693	rBV	158063	268923	17.27%	2.148%
5	7.243	701	707	720	rBV	134912	219082	14.07%	1.750%
6	7.449	736	742	754	rVB	152785	268187	17.22%	2.143%
7	7.919	816	822	829	rVB	112258	186320	11.97%	1.488%
8	8.624	933	942	957	rBV	189519	337981	21.71%	2.700%
9	9.076	1012	1019	1032	rBV	151435	273009	17.53%	2.181%
10	9.805	1136	1143	1151	rBV	116419	211574	13.59%	1.690%
11	10.345	1227	1235	1245	rBV	179279	318098	20.43%	2.541%
12	10.721	1291	1299	1306	rBV	160101	277822	17.84%	2.219%
13	10.856	1315	1322	1335	rBV	192003	352457	22.64%	2.816%
14	12.308	1565	1569	1575	rBV4	2261	4503	0.29%	0.036%
15	13.442	1758	1762	1766	rBV	3417	4915	0.32%	0.039%
16	13.959	1844	1850	1859	rBV	401099	571842	36.73%	4.568%
17	14.252	1893	1900	1910	rBV	410172	656501	42.16%	5.245%
18	14.558	1945	1952	1963	rBV	266905	409413	26.29%	3.271%
19	14.758	1979	1986	2002	rBV	151009	296734	19.06%	2.371%
20	15.545	2114	2120	2134	rBV	556853	867016	55.68%	6.927%
21	15.662	2134	2140	2152	rVB	193365	280746	18.03%	2.243%
22	15.786	2157	2161	2164	rVB3	2326	2365	0.15%	0.019%
23	17.302	2413	2419	2429	rBV	392938	590900	37.95%	4.721%
24	17.402	2429	2436	2450	rVB	692509	1090397	70.03%	8.711%
25	17.684	2479	2484	2488	rBV3	942	1829	0.12%	0.015%
26	19.252	2747	2751	2755	rBV3	10066	12672	0.81%	0.101%
27	19.323	2759	2763	2769	rBV	8872	12976	0.83%	0.104%
28	19.687	2819	2825	2839	rBV	1006985	1424508	91.49%	11.380%
29	19.834	2846	2850	2852	rVB4	2183	2453	0.16%	0.020%
30	19.863	2852	2855	2857	rBV2	1718	2059	0.13%	0.016%
31	19.916	2860	2864	2867	rBV4	1434	2348	0.15%	0.019%
32	20.316	2930	2932	2933	rBV2	1700	1647	0.11%	0.013%
33	20.416	2947	2949	2951	rBV2	1695	1566	0.10%	0.013%
34	20.539	2968	2970	2977	rVB8	1905	2089	0.13%	0.017%
35	20.598	2978	2980	2983	rVV3	2563	2075	0.13%	0.017%
36	20.645	2986	2988	2990	rVB3	2268	2065	0.13%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
 Data File : BG058050.D
 Acq On : 6 Jul 2023 14:56
 Operator : CG/JU
 Sample : PB153588BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK588

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
 Title : SVOA CALIBRATION

37	21.174	3077	3078	3080	rBV2	3041	1929	0.12%	0.015%
38	21.556	3136	3143	3157	rVB2	431581	712638	45.77%	5.693%
39	22.237	3256	3259	3260	rBV3	3772	4623	0.30%	0.037%
40	23.013	3386	3391	3396	rVB4	9307	18033	1.16%	0.144%
41	23.788	3520	3523	3531	rVB4	16098	31259	2.01%	0.250%
42	24.493	3632	3643	3660	rBV2	554394	1557062	100.00%	12.439%
43	24.711	3670	3680	3695	rVB2	307371	856784	55.03%	6.845%
44	25.821	3862	3869	3879	rVB4	22797	68965	4.43%	0.551%
45	28.729	4359	4364	4365	rBV5	9099	12972	0.83%	0.104%
46	29.999	4578	4580	4583	rBV4	4084	4584	0.29%	0.037%
47	30.239	4619	4621	4622	rBV2	3671	2143	0.14%	0.017%




Sum of corrected areas: 12517356

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
Data File : BG058050.D
Acq On : 6 Jul 2023 14:56
Operator : CG/JU
Sample : PB153588BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK588

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

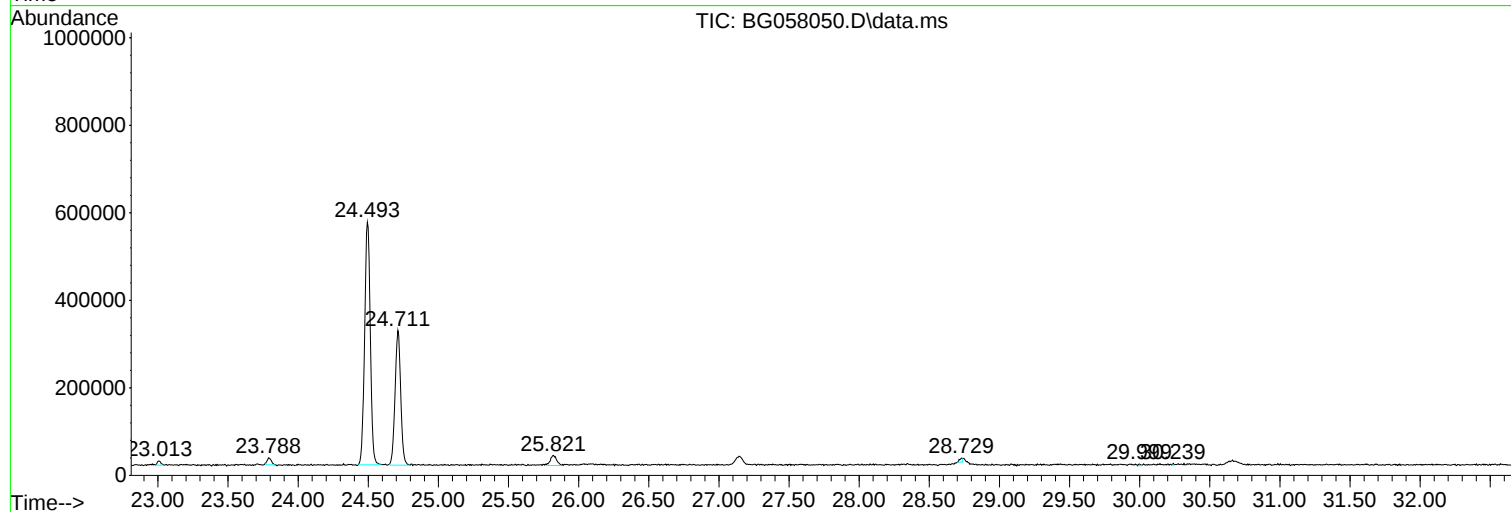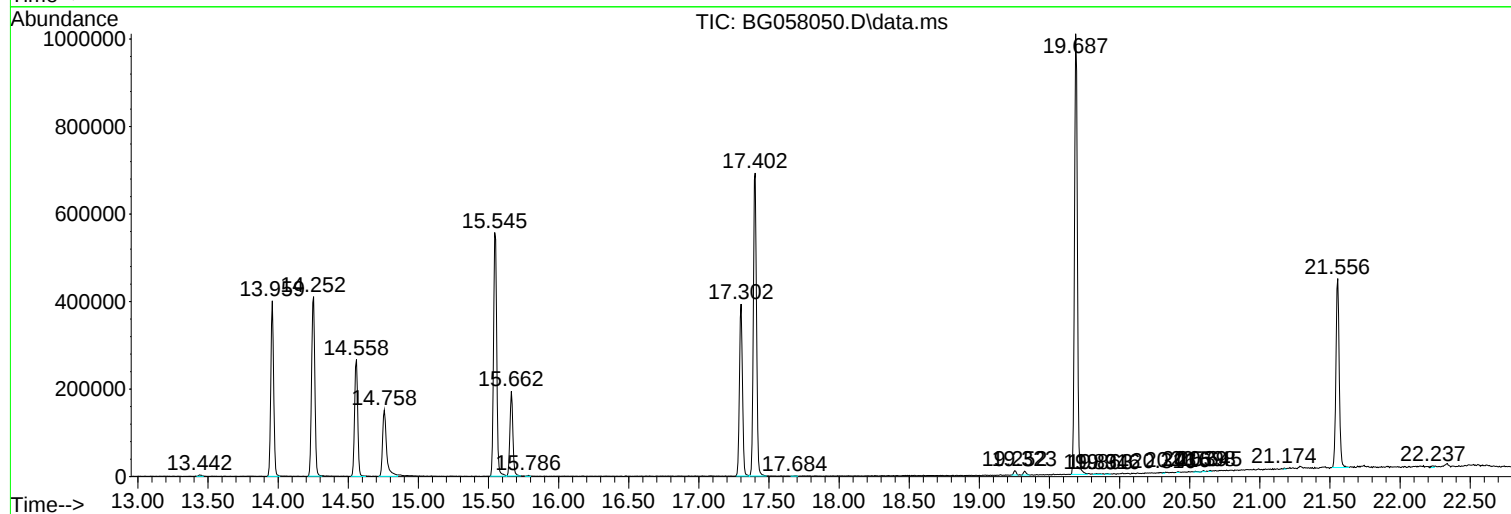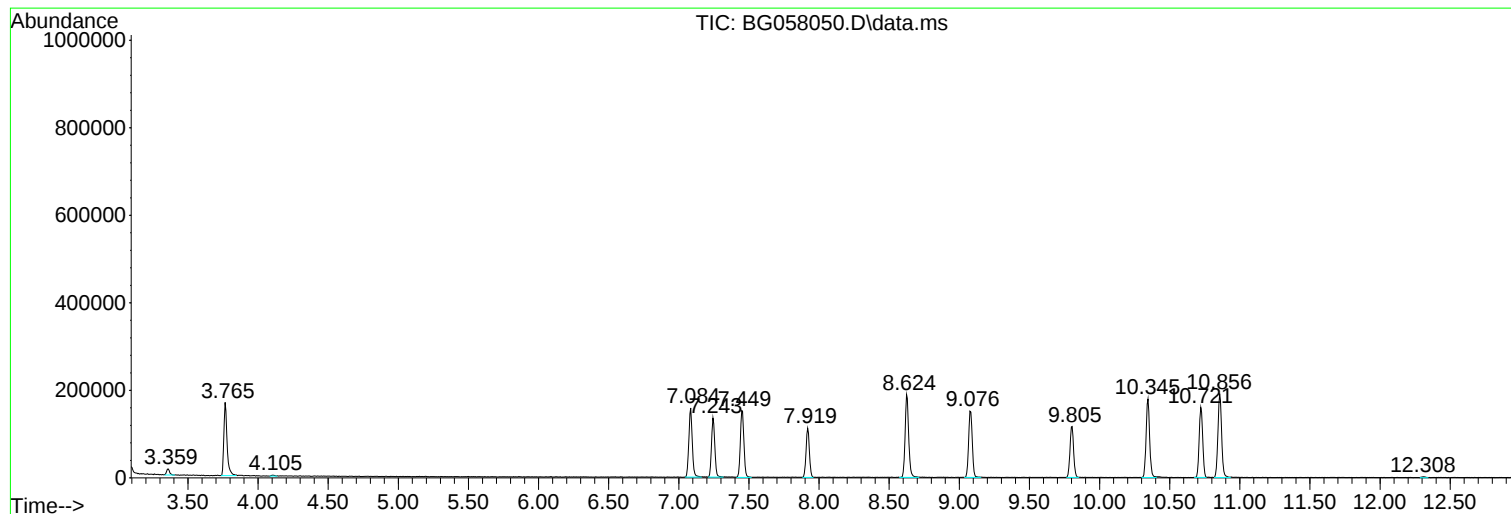

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
Data File : BG058050.D
Acq On : 6 Jul 2023 14:56
Operator : CG/JU
Sample : PB153588BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK588

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070523\
Data File : BG058050.D
Acq On : 6 Jul 2023 14:56
Operator : CG/JU
Sample : PB153588BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK588

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc